




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062223\
 Data File : VW026307.D
 Acq On : 22 Jun 2023 18:17
 Operator : SY/MD
 Sample : 03382-10
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW46

Manual IntegrationsAPPROVED

Quant Time: Jun 23 01:06:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 23 01:02:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/23/2023
 Supervised By :Mahesh Dadoda 06/26/2023

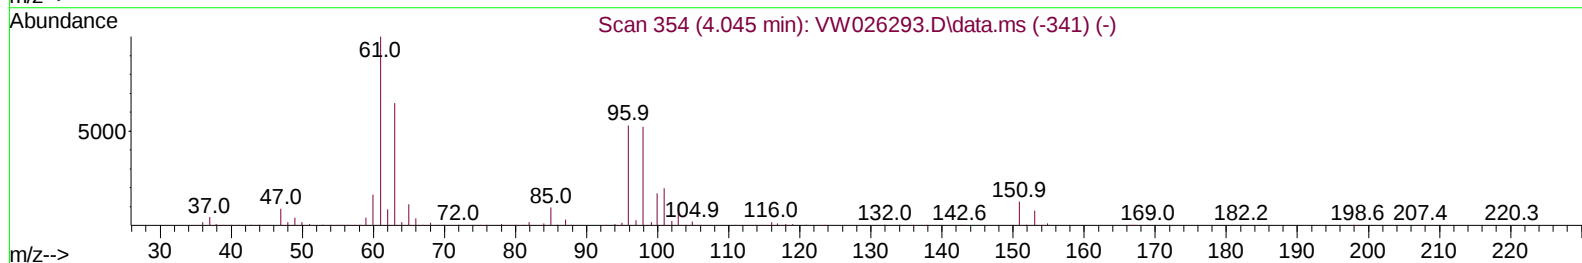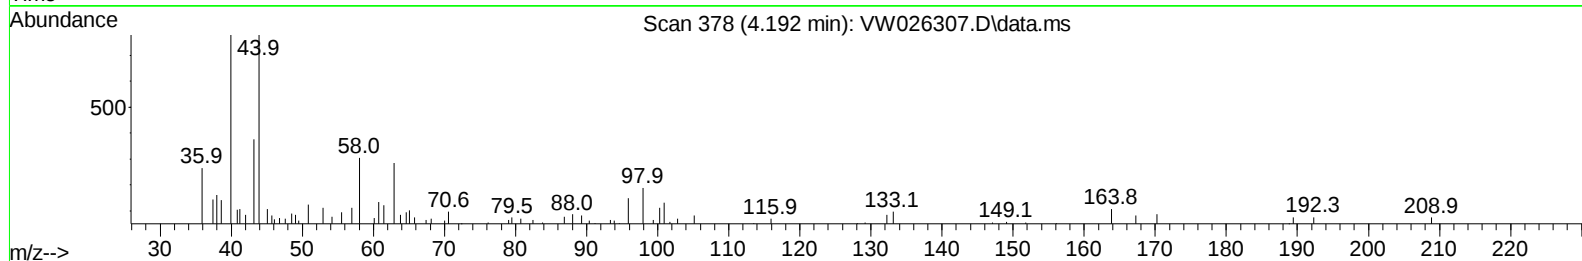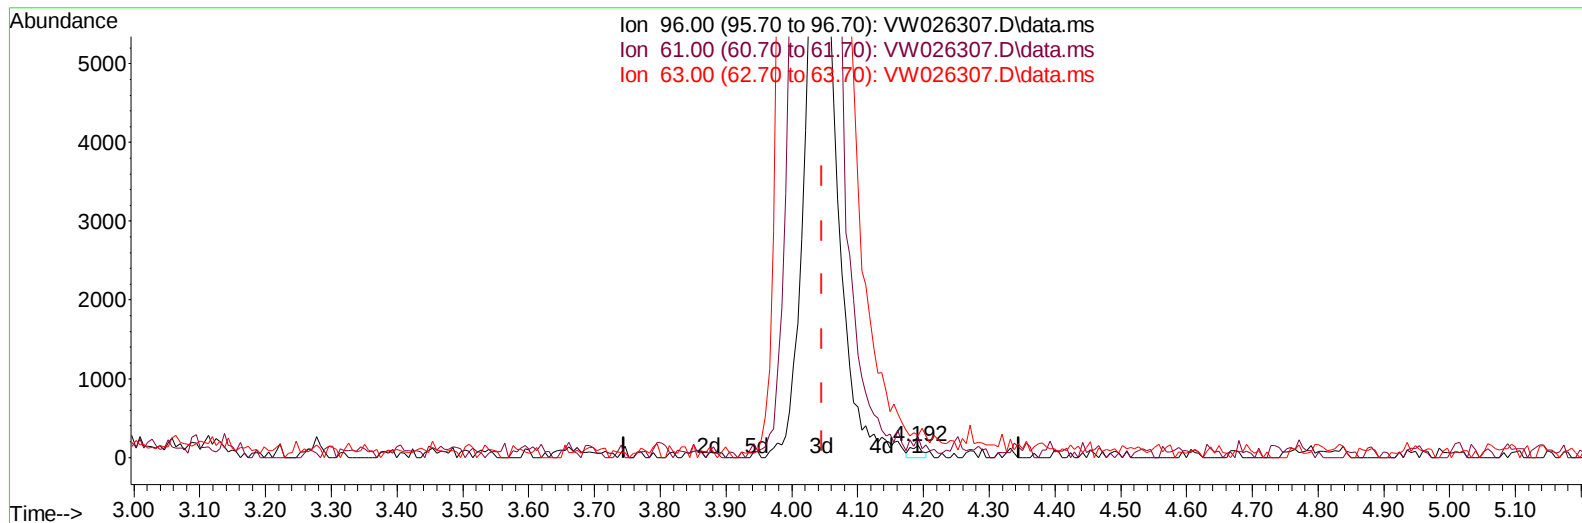

TIC: VW026307.D\data.ms

(12) 1,1-Dichloroethene (T)

4.192min (+ 0.146) 0.02 ug/L

response 189

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	200.80	171.81
63.00	188.10	191.28
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062223\
 Data File : VW026307.D
 Acq On : 22 Jun 2023 18:17
 Operator : SY/MD
 Sample : 03382-10
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW46

Manual IntegrationsAPPROVED

Quant Time: Jun 23 01:06:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 23 01:02:45 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/23/2023
 Supervised By :Mahesh Dadoda 06/26/2023

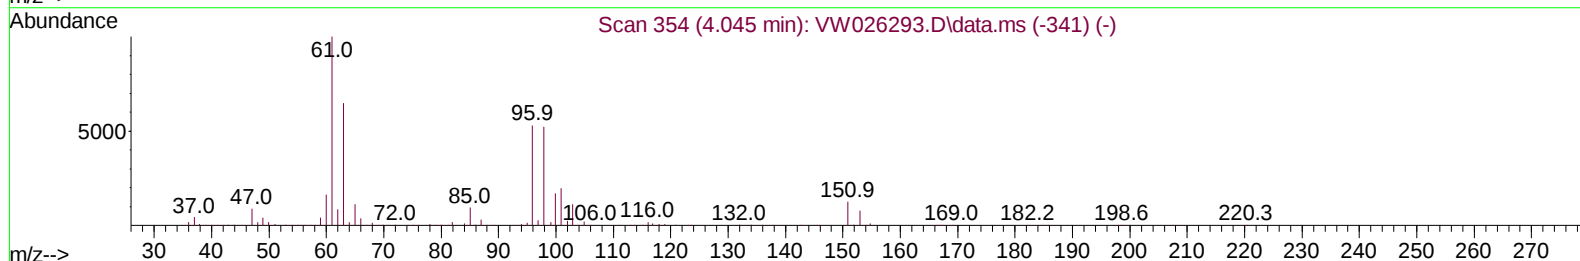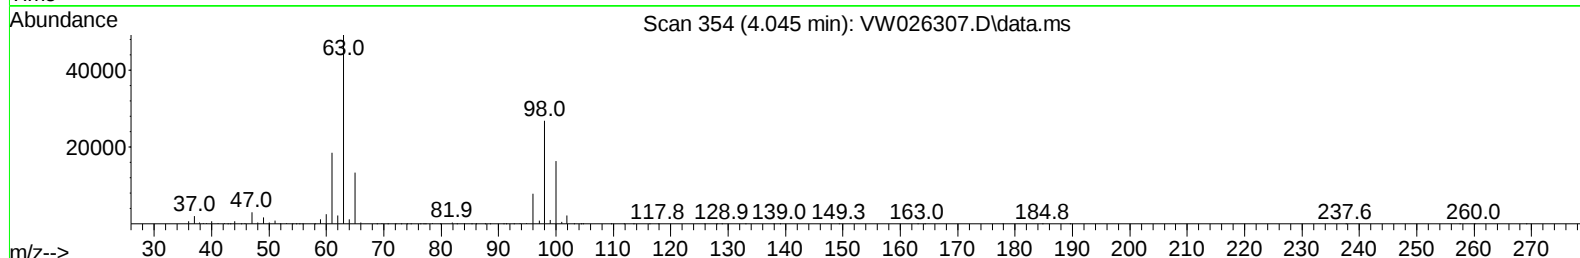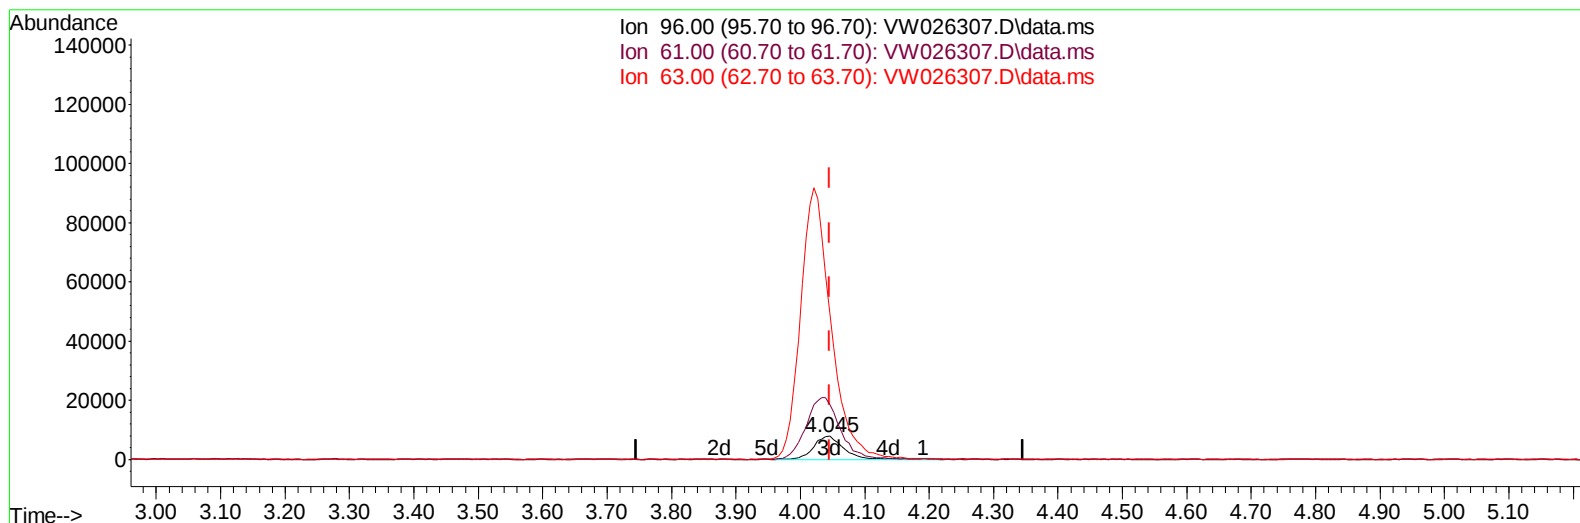

TIC: VW026307.D\data.ms

(12) 1,1-Dichloroethene (T)

4.045min (0.000) 2.52 ug/L m

response 25595

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	200.80	236.08
63.00	188.10	625.25#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062223\
 Data File : VW026307.D
 Acq On : 22 Jun 2023 18:17
 Operator : SY/MD
 Sample : 03382-10
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/23/2023
 Supervised By :Mahesh Dadoda 06/26/2023

Quant Time: Jun 23 01:06:53 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 23 01:02:45 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		798511	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		639823	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		219115	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		166550	14.826	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	59.320%		
7) Chloroethane-d5	2.893	69		169761	20.188	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	80.760%		
11) 1,1-Dichloroethene-d2	4.021	65		87876	15.865	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	63.440%		
21) 2-Butanone-d5	7.075	46		178969	54.723	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	109.440%		
24) Chloroform-d	7.648	84		464370	19.859	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	79.440%		
26) 1,2-Dichloroethane-d4	8.307	65		264996	20.725	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	82.880%		
32) Benzene-d6	8.276	84		876257	20.353	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	81.400%		
36) 1,2-Dichloropropane-d6	9.270	67		303321	22.238	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	88.960%		
41) Toluene-d8	10.325	98		680416	17.821	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	71.280%		
43) trans-1,3-Dichloroprop...	10.575	79		91945	17.011	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	68.040%		
47) 2-Hexanone-d5	10.922	63		107239	49.863	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	99.720%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		246077	24.793	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	99.160%		
66) 1,2-Dichlorobenzene-d4	13.849	152		169125	20.166	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	80.680%		
Target Compounds							
						Qvalue	
12) 1,1-Dichloroethene	4.045	96		25595m	2.518	ug/L	
13) Acetone	4.125	43		14808	5.852	ug/L	97
16) Methylene chloride	4.917	84		23628	1.854	ug/L	92
19) 1,1-Dichloroethane	6.216	63		62270	2.681	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062223\
Data File : VW026307.D
Acq On : 22 Jun 2023 18:17
Operator : SY/MD
Sample : 03382-10
Misc : 5.22g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBW46

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/23/2023
Supervised By :Mahesh Dadoda 06/26/2023

Quant Time: Jun 23 01:06:53 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 23 01:02:45 2023
Response via : Initial Calibration

