

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
Data File : VW019288.D
Acq On : 23 Jun 2021 13:54
Operator : SY/VA
Sample : M2808-07
Misc : 3.91G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDQ8

Manual Integrations
APPROVED

MMDadoda
6/24/2021 4:32:12 PM

Quant Time: Jun 24 01:13:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 24 01:10:00 2021
Response via : Initial Calibration

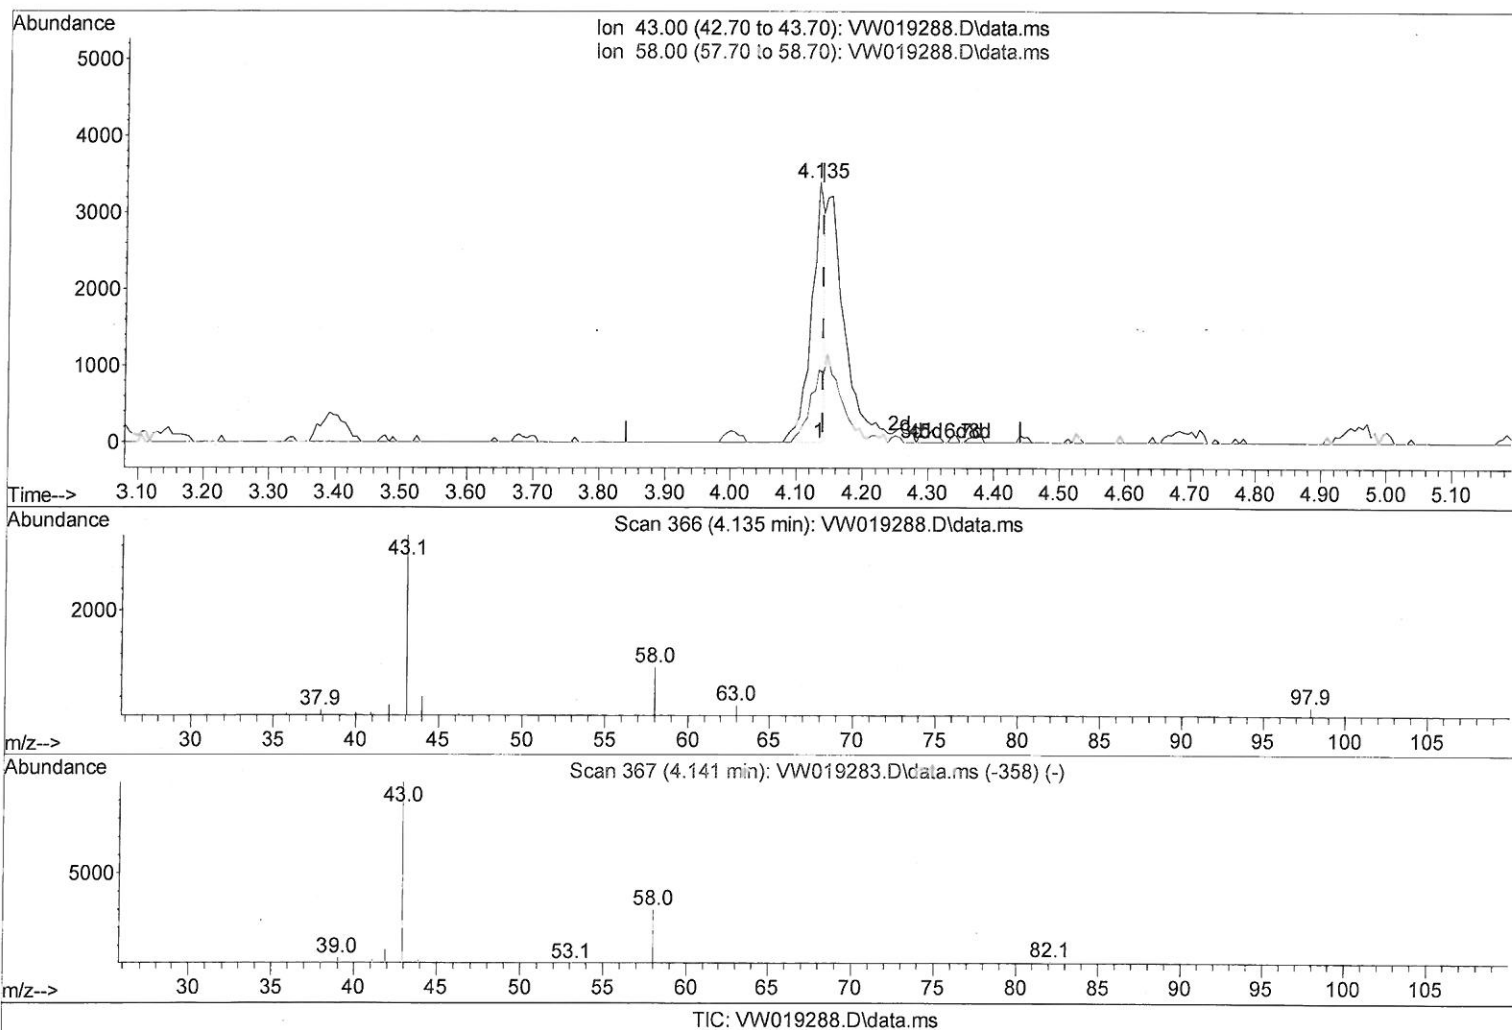

(13) Acetone (T)

4.135min (-0.006) 2.98 ug/L

response 4771

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	68.20#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019288.D
 Acq On : 23 Jun 2021 13:54
 Operator : SY/VA
 Sample : M2808-07
 Misc : 3.91G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDQ8

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:12 PM

Quant Time: Jun 24 01:13:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

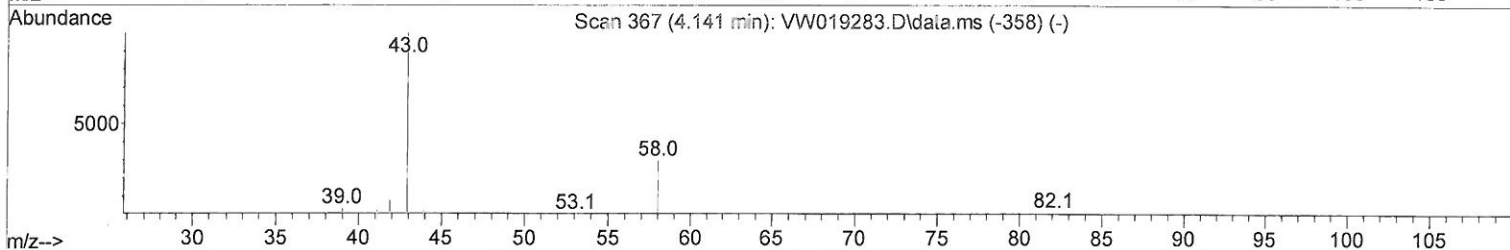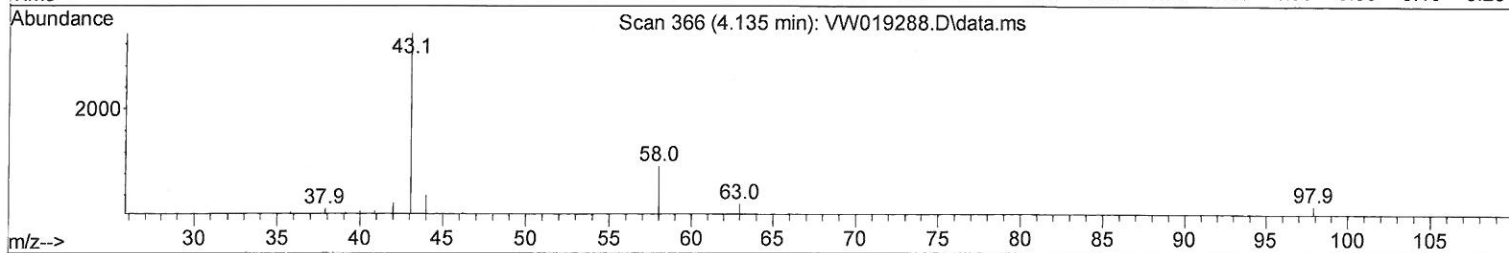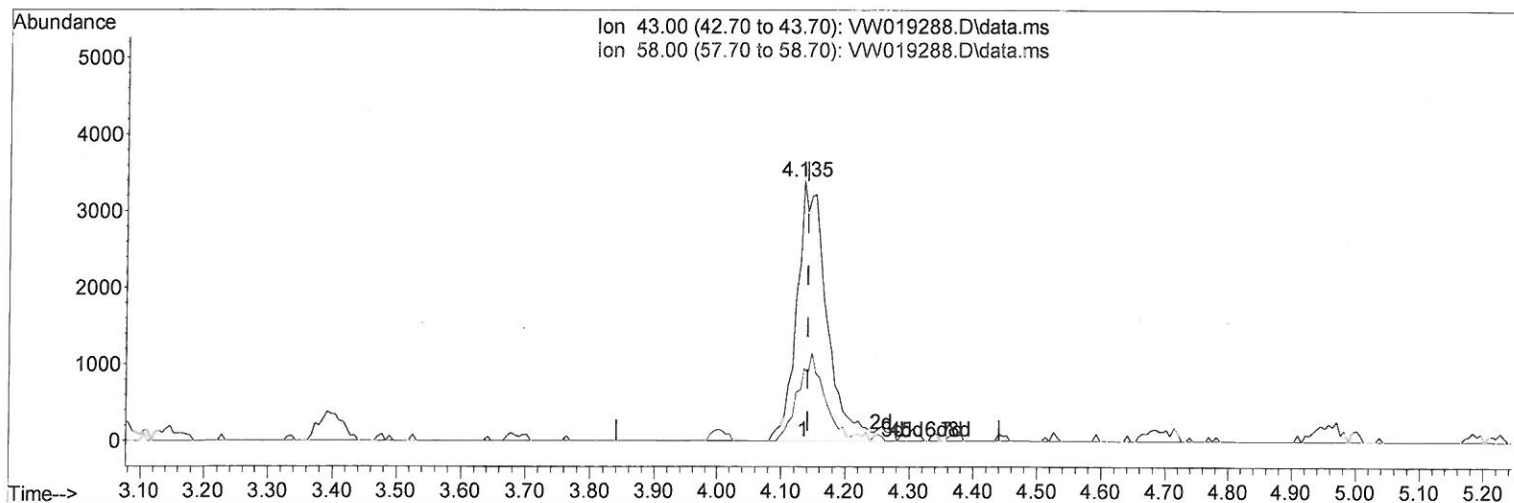

TIC: VW019288.D\data.ms

(13) Acetone (T)

4.135min (-0.006) 6.85 ug/L m

response 10962

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	29.68
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019288.D
 Acq On : 23 Jun 2021 13:54
 Operator : SY/VA
 Sample : M2808-07
 Misc : 3.91G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDQ8

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:12 PM

Quant Time: Jun 24 01:13:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

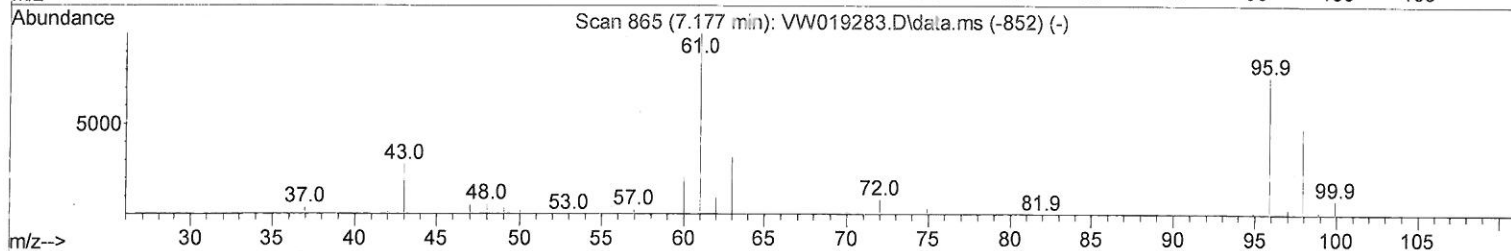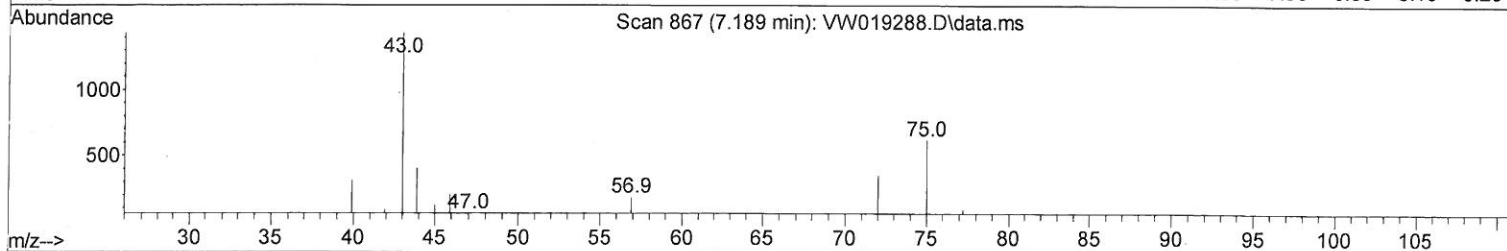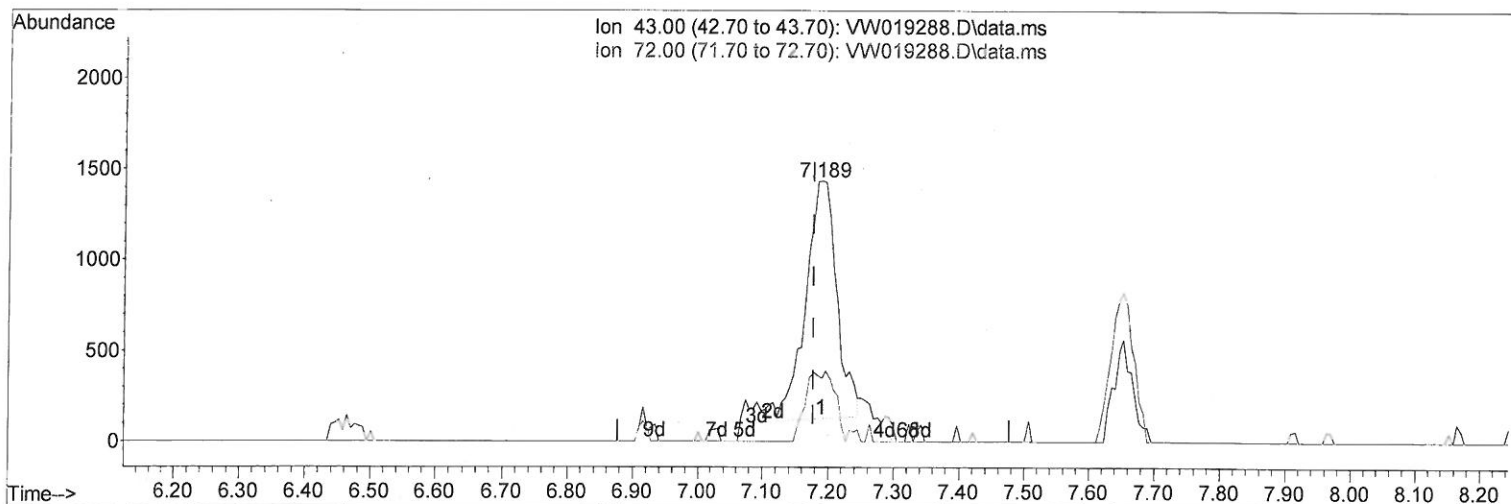

TIC: VW019288.D\data.ms

(22) 2-Butanone (T)

7.189min (+ 0.012) 1.98 ug/L

response 4246

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	16.13
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019288.D
 Acq On : 23 Jun 2021 13:54
 Operator : SY/VA
 Sample : M2808-07
 Misc : 3.91G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDQ8

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:12 PM

Quant Time: Jun 24 01:13:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

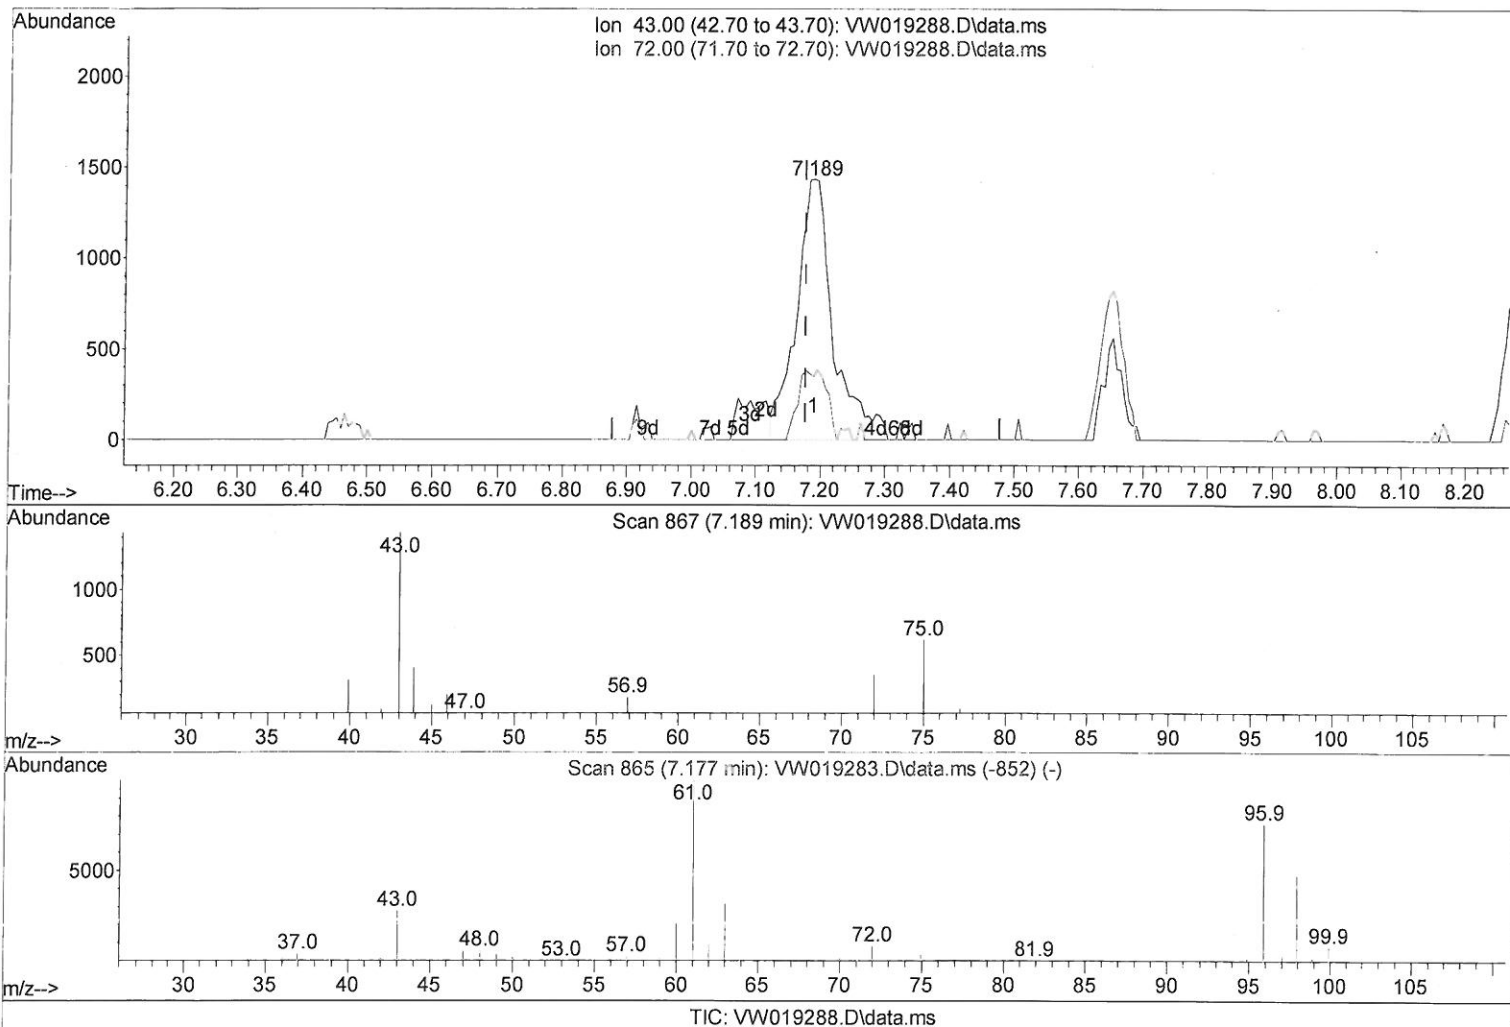

(22) 2-Butanone (T)

7.189min (+ 0.012) 2.55 ug/L m

response 5455

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	12.56#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019288.D
 Acq On : 23 Jun 2021 13:54
 Operator : SY/VA
 Sample : M2808-07
 Misc : 3.91G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDQ8

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:12 PM

Quant Time: Jun 24 01:13:21 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	521707	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	399983	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	117927	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	150253	21.780	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.120%		
7) Chloroethane-d5	2.891	69	125213	21.310	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.240%		
11) 1,1-Dichloroethene-d2	4.025	63	221568	16.165	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	64.680%		
21) 2-Butanone-d5	7.080	46	54932	30.398	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	60.800%		
24) Chloroform-d	7.653	84	314089	22.393	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	89.560%		
26) 1,2-Dichloroethane-d4	8.311	65	159426	20.264	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	81.040%		
32) Benzene-d6	8.281	84	623910	27.378	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	109.520%		
36) 1,2-Dichloropropane-d6	9.274	67	183646	26.582	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	106.320%		
41) Toluene-d8	10.323	98	511374	24.434	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	97.720%		
43) trans-1,3-Dichloroprop...	10.579	79	62705	20.957	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.840%		
47) 2-Hexanone-d5	10.927	63	43328	36.984	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	73.960%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	101575	17.824	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	71.280%		
66) 1,2-Dichlorobenzene-d4	13.853	152	88367	21.469	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	85.880%		
Target Compounds						
13) Acetone	4.135	43	10962m	6.846	ug/L	Qvalue 97
16) Methylene chloride	4.922	84	31926	3.298	ug/L	
22) 2-Butanone	7.189	43	5455m	2.548	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
Data File : VW019288.D
Acq On : 23 Jun 2021 13:54
Operator : SY/VA
Sample : M2808-07
Misc : 3.91G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDQ8

Manual Integrations
APPROVED

MMDadoda
6/24/2021 4:32:12 PM

Quant Time: Jun 24 01:13:21 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 24 01:10:00 2021
Response via : Initial Calibration

