

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019297.D
 Acq On : 23 Jun 2021 17:30
 Operator : SY/VA
 Sample : M2825-05RE
 Misc : 4.29G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDQ9RE

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:23 PM

Quant Time: Jun 24 01:14:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

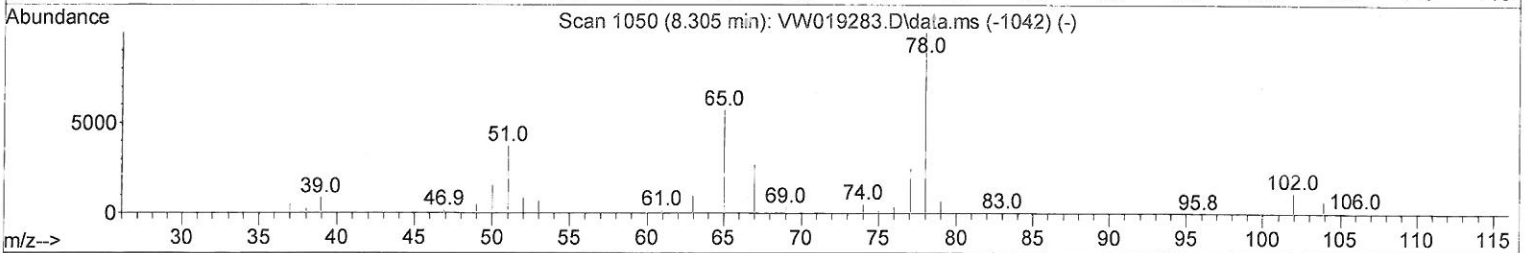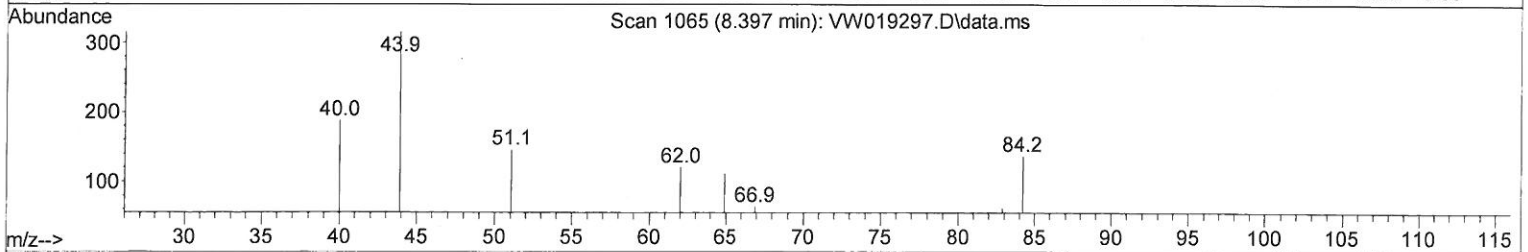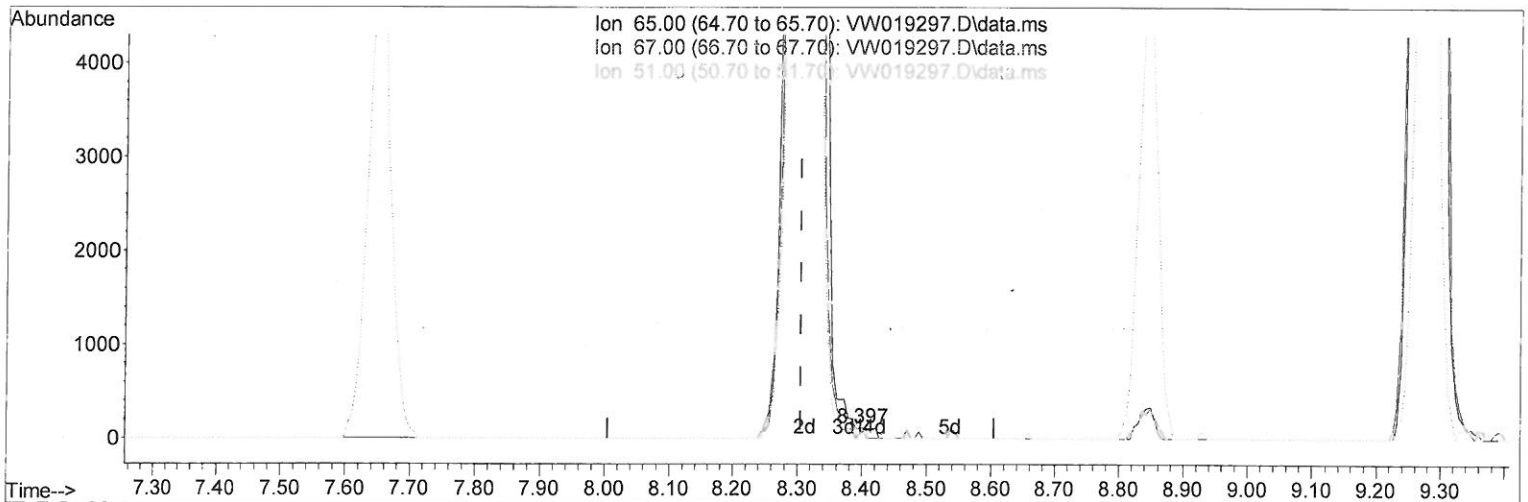

TIC: VW019297.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.397min (+ 0.091) 0.01 ug/L

response 103

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	40.78
51.00	98.00	75.73
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
Data File : VW019297.D
Acq On : 23 Jun 2021 17:30
Operator : SY/VA
Sample : M2825-05RE
Misc : 4.29G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDQ9RE

Manual Integrations
APPROVED

MMDadoda
6/24/2021 4:32:23 PM

Quant Time: Jun 24 01:14:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 24 01:10:00 2021
Response via : Initial Calibration

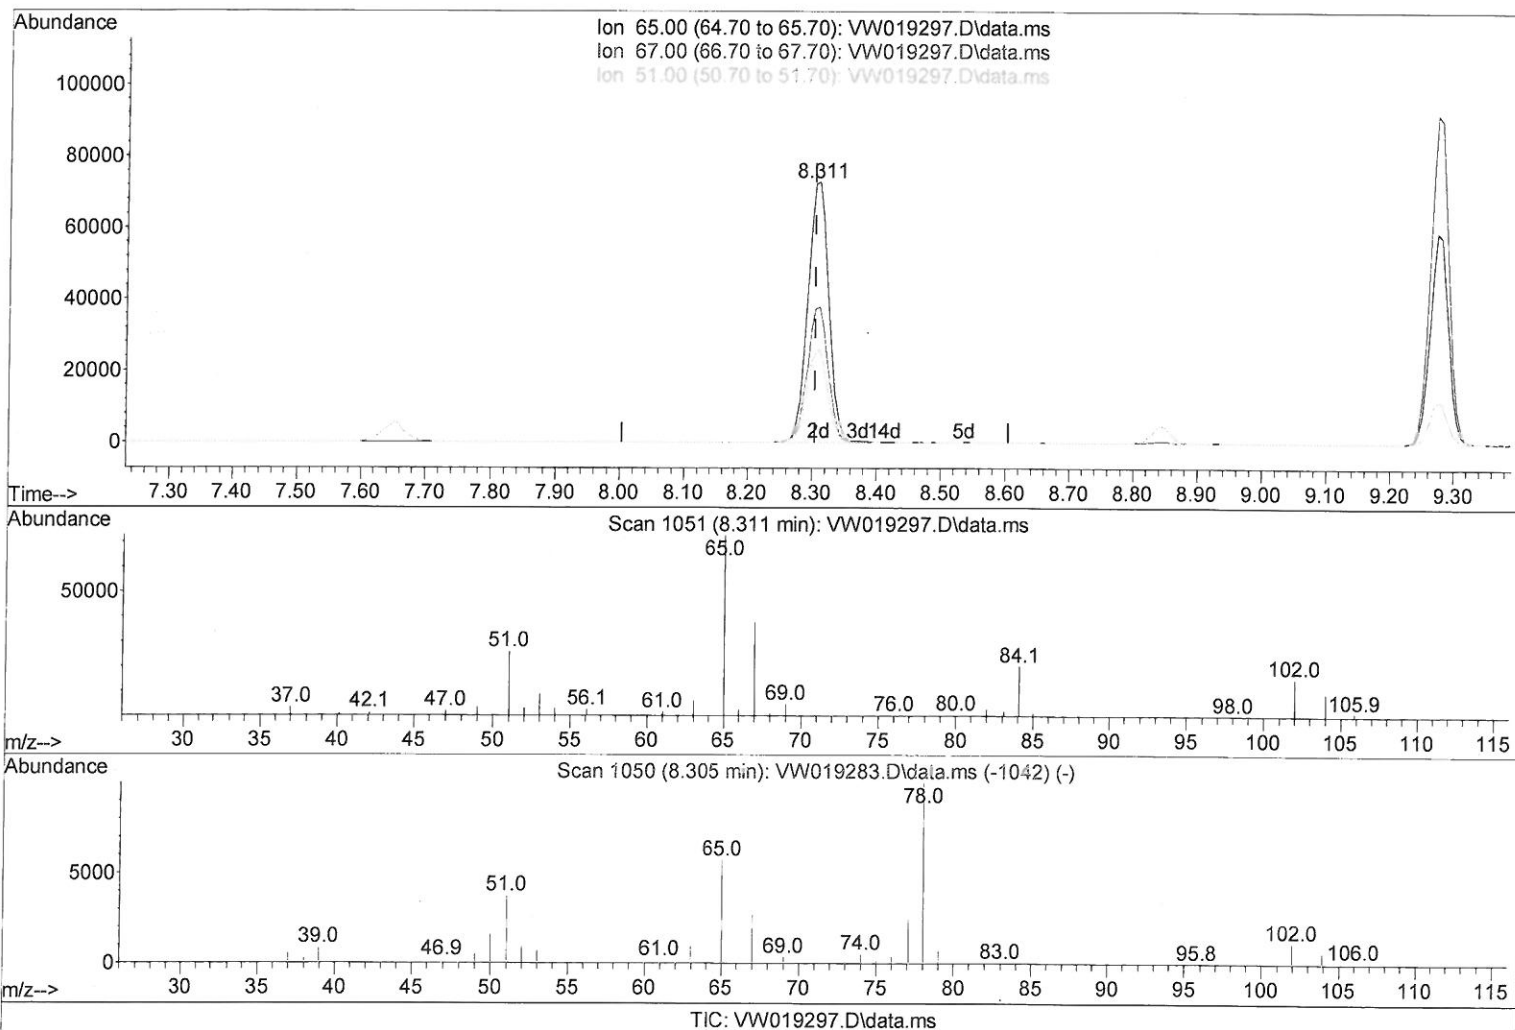

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+ 0.006) 23.17 ug/L m

response 164184

Ion Exp% Act%

65.00 100.00 100.00

67.00 51.70 0.03#

51.00 98.00 0.05#

0.00 0.00 0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019297.D
 Acq On : 23 Jun 2021 17:30
 Operator : SY/VA
 Sample : M2825-05RE
 Misc : 4.29G/10ML/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDQ9RE

Manual Integrations
 APPROVED

MMDadoda
 6/24/2021 4:32:23 PM

Quant Time: Jun 24 01:14:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	469882	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	372313	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	114517	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	143485	23.093	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.360%		
7) Chloroethane-d5	2.898	69	121977	23.049	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.200%		
11) 1,1-Dichloroethene-d2	4.025	63	206729	16.746	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.000%		
21) 2-Butanone-d5	7.086	46	61548	37.816	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	75.640%		
24) Chloroform-d	7.653	84	312041	24.701	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	98.800%		
26) 1,2-Dichloroethane-d4	8.311	65	164184m	23.170	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.680%		
32) Benzene-d6	8.275	84	608561	28.689	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	114.760%		
36) 1,2-Dichloropropane-d6	9.275	67	185377	28.827	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	115.320%		
41) Toluene-d8	10.323	98	500216	25.677	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	102.720%		
43) trans-1,3-Dichloroprop...	10.579	79	67776	24.335	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	97.360%		
47) 2-Hexanone-d5	10.927	63	48872	44.817	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	89.640%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	113116	21.324	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.280%		
66) 1,2-Dichlorobenzene-d4	13.853	152	95048	23.779	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	95.120%		
Target Compounds						
13) Acetone	4.141	43	40042	27.764	ug/L	89
16) Methylene chloride	4.922	84	45675	5.239	ug/L	94
22) 2-Butanone	7.183	43	16602	8.609	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/25/21 84

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
Data File : VW019297.D
Acq On : 23 Jun 2021 17:30
Operator : SY/VA
Sample : M2825-05RE
Misc : 4.29G/10ML/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDQ9RE

Manual Integrations
APPROVED

MMDadoda
6/24/2021 4:32:23 PM

Quant Time: Jun 24 01:14:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 24 01:10:00 2021
Response via : Initial Calibration

