

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
 Data File : VW019285.D
 Acq On : 23 Jun 2021 12:43
 Operator : SY/VA
 Sample : M2808-02
 Misc : 5.12G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGG08

Quant Time: Jun 24 01:12:52 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 24 01:10:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	615431	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	515163	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	185961	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	177613	21.825	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.320%
7) Chloroethane-d5	2.898	69	154208	22.248	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.000%
11) 1,1-Dichloroethene-d2	4.025	63	277260	17.148	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.600%
21) 2-Butanone-d5	7.092	46	48946	22.961	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	45.920%
24) Chloroform-d	7.653	84	382042	23.090	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.360%
26) 1,2-Dichloroethane-d4	8.311	65	183450	19.766	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.080%
32) Benzene-d6	8.281	84	757536	25.810	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.240%
36) 1,2-Dichloropropane-d6	9.274	67	220809	24.816	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.280%
41) Toluene-d8	10.323	98	670829	24.887	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.560%
43) trans-1,3-Dichloroprop...	10.579	79	76170	19.765	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.080%
47) 2-Hexanone-d5	10.927	63	42330	28.054	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.100%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	123586	16.837	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	67.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	148625	22.898	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.600%
Target Compounds						Qvalue
16) Methylene chloride	4.928	84	24973	2.187	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062321\
Data File : VW019285.D
Acq On : 23 Jun 2021 12:43
Operator : SY/VA
Sample : M2808-02
Misc : 5.12G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGG08

Quant Time: Jun 24 01:12:52 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 24 01:10:00 2021
Response via : Initial Calibration

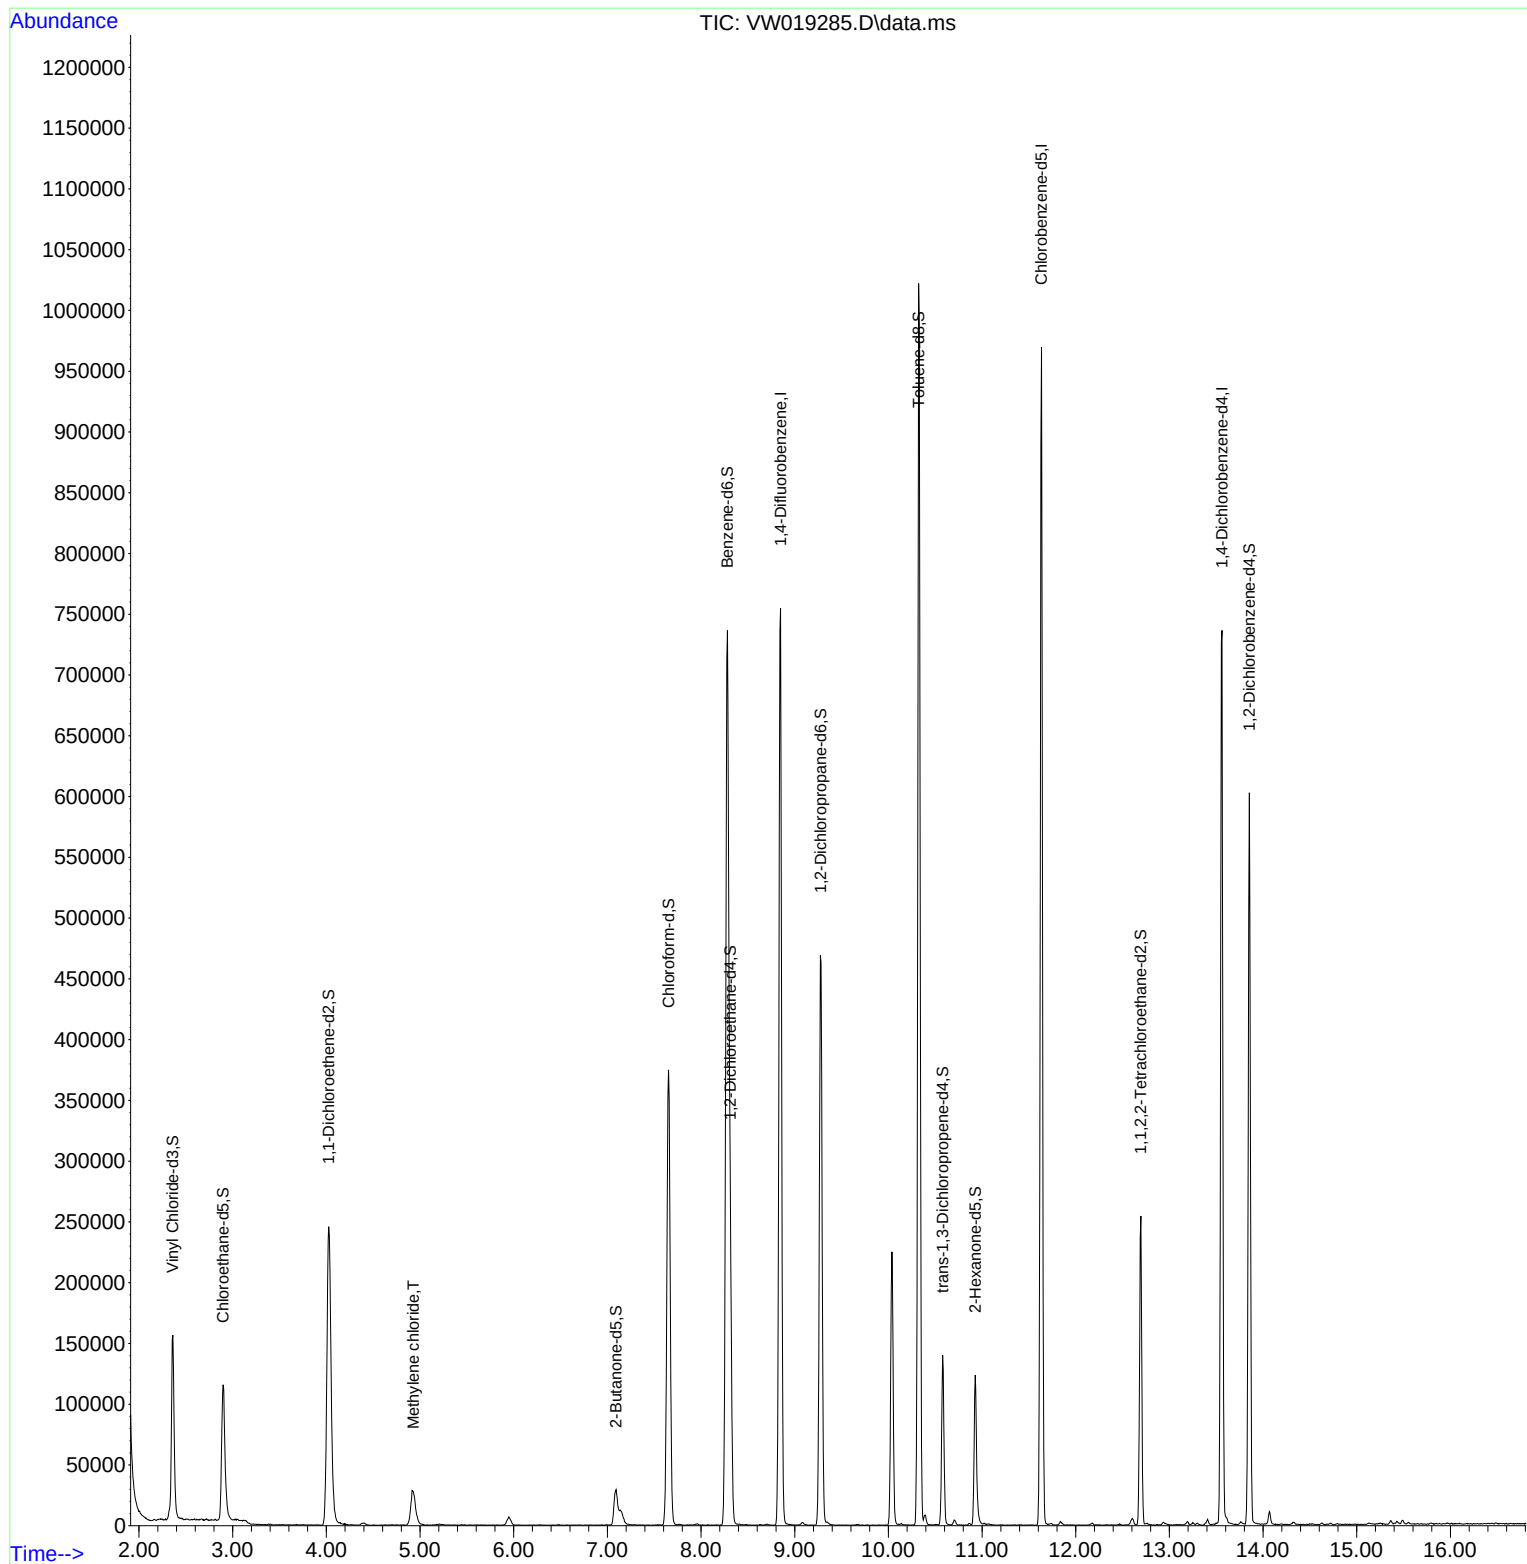

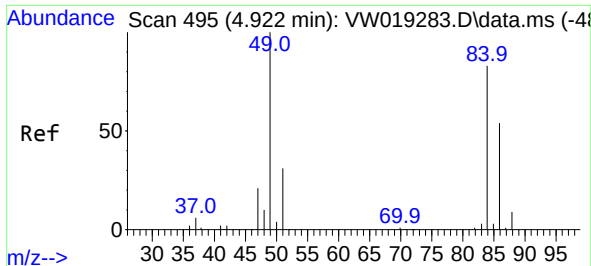

#16
Methylene chloride
Concen: 2.187 ug/L
RT: 4.928 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019285.D
Acq: 23 Jun 2021 12:43

Instrument :
MSVOA_W
ClientSampled :
BGG08

Tgt Ion:	84	Resp:	24973
Ion	Ratio	Lower	Upper
84	100		
86	59.7	45.3	84.1
49	114.0	86.6	160.8

