

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062419\
 Data File : VW010944.D
 Acq On : 24 Jun 2019 21:43
 Operator : SY/VA
 Sample : K3456-12
 Misc : 3.56G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANT6

Quant Time: Jun 25 04:05:23 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 25 02:43:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	122117	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	161479	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	80834	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	8105	5.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	20.48%#
7) Chloroethane-d5	2.89	69	12782	10.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	41.92%
10) 1,1-Dichloroethene-d2	4.02	63	19983	5.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	21.36%#
20) 2-Butanone-d5	0.00	46	0d	0.00	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.00%#
24) Chloroform-d	7.65	84	95299	28.94	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	115.76%
26) 1,2-Dichloroethane-d4	8.31	65	102197	50.06	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	200.24%#
29) Benzene-d6	8.27	84	160543	16.56	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	66.24%
33) 1,2-Dichloropropane-d6	9.27	67	84319	26.32	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.28%
37) Toluene-d8	10.32	98	143456	16.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	65.60%
38) trans-1,3-Dichloropropene-	10.58	79	28413	20.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.16%
39) 2-Hexanone-d5	0.00	63	0d	0.00	ug/L	
Spiked Amount	50.000	Range	20 - 135	Recovery	=	0.00%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104996	39.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	159.08%#
61) 1,2-Dichlorobenzene-d4	13.86	152	83544	27.38	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.52%


Target Compounds					Ovalue
13) Acetone	4.12	43	14807	20.801 ug/L	100
15) Methyl Acetate	4.68	43	7415	6.018 ug/L #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062419\
Data File : VW010944.D
Acq On : 24 Jun 2019 21:43
Operator : SY/VA
Sample : K3456-12
Misc : 3.56G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANT6

Quant Time: Jun 25 04:05:23 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 25 02:43:13 2019
Response via : Initial Calibration

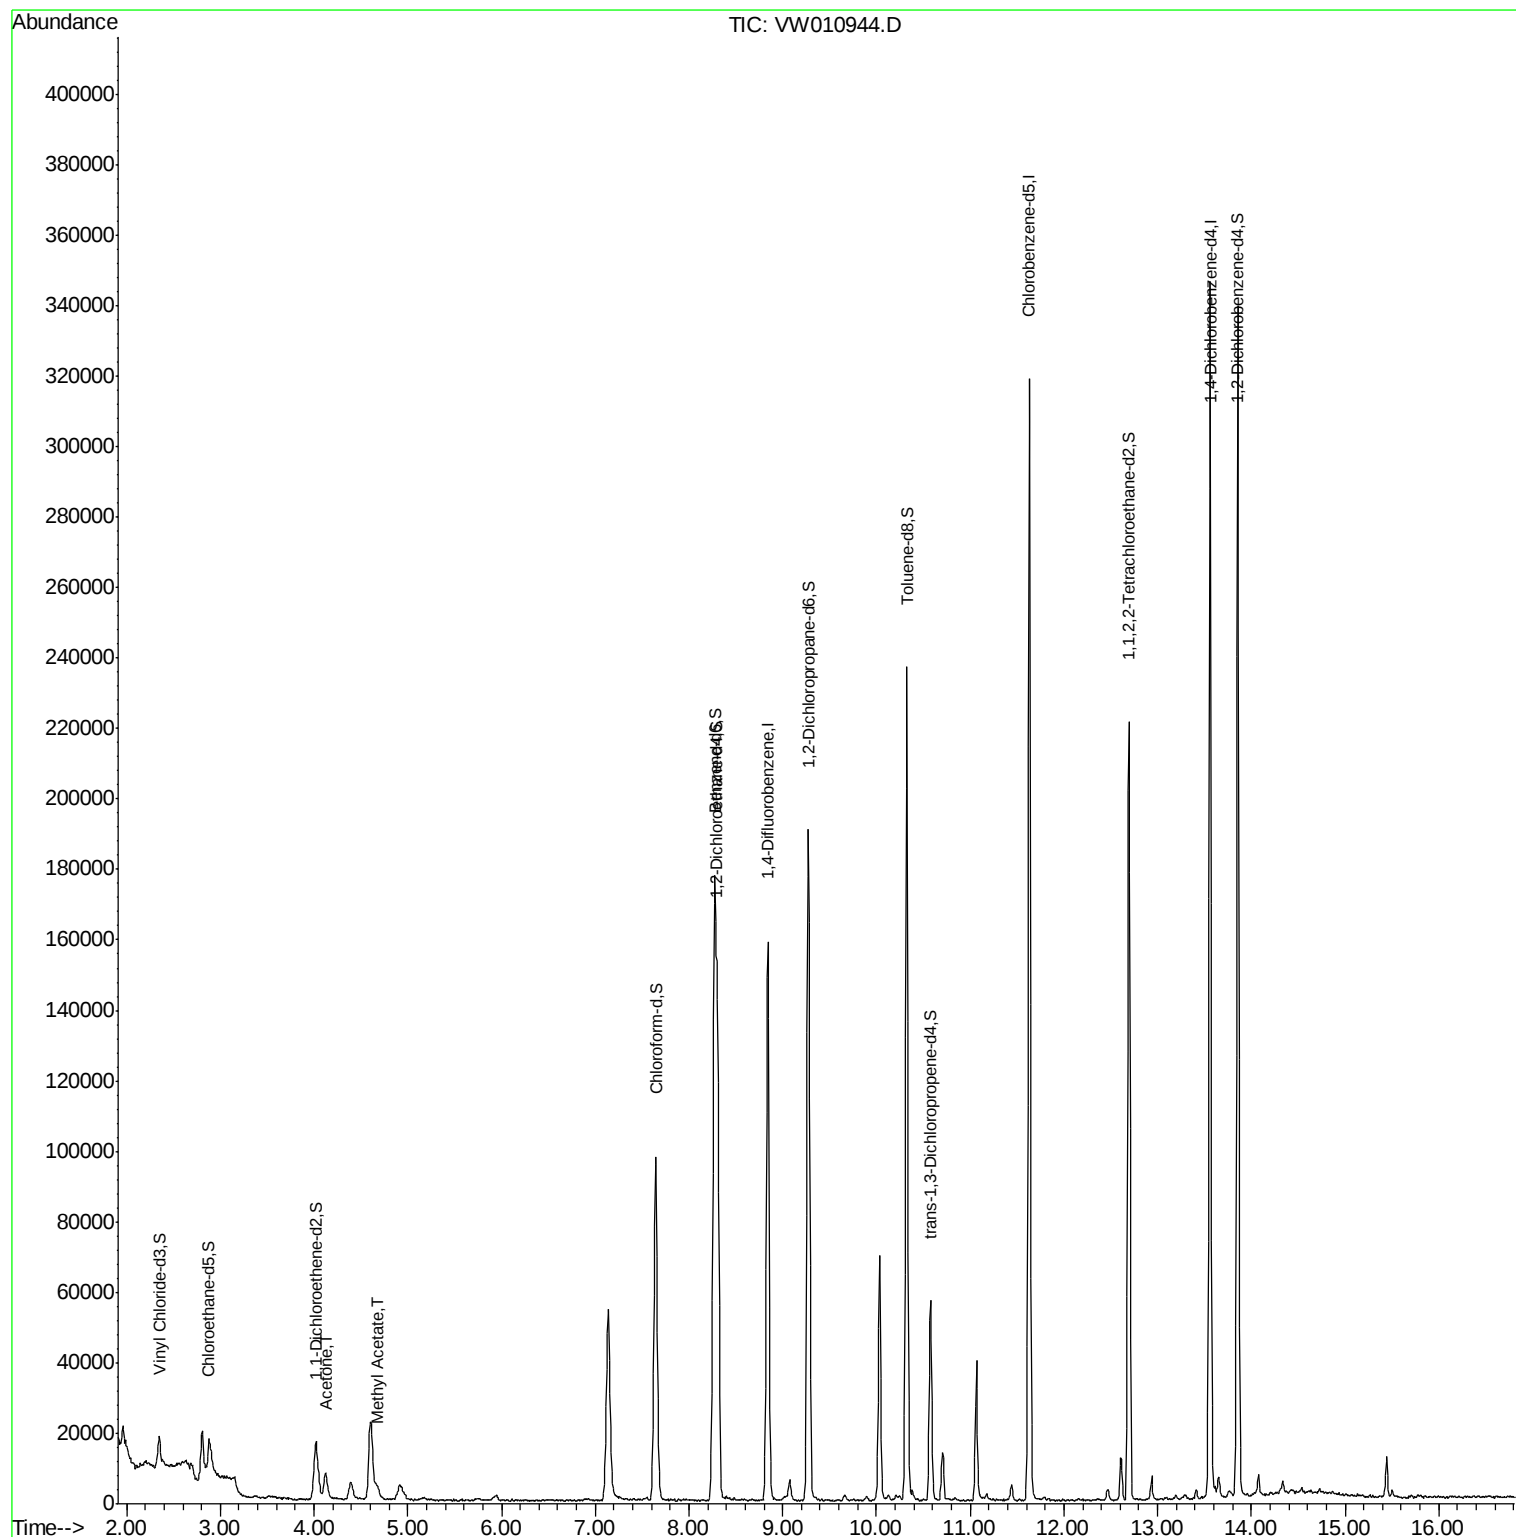

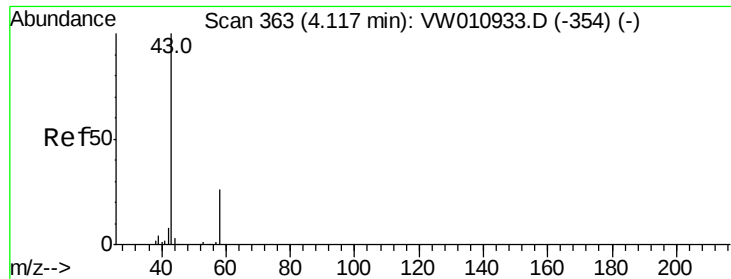

#13

Acetone

Concen: 20.801 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW010944.D

Acq: 24 Jun 2019 21:43

Instrument :

MSVOA_W

ClientSampled :


YANT6

Tot Ion: 43 Resp: 14807

Ion Ratio Lower Upper




43 100

58 26.4 0.0 53.2

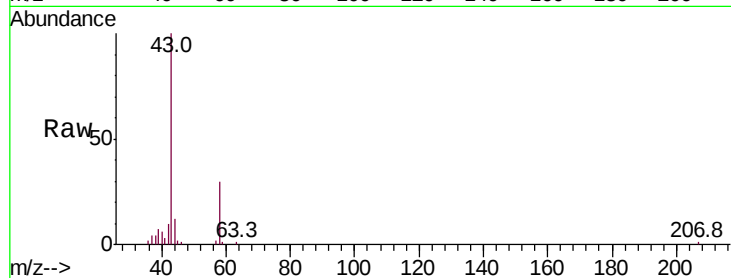

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

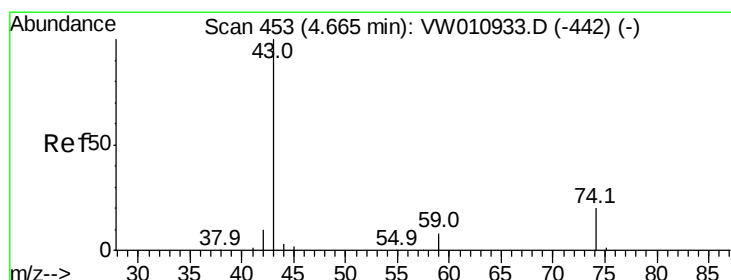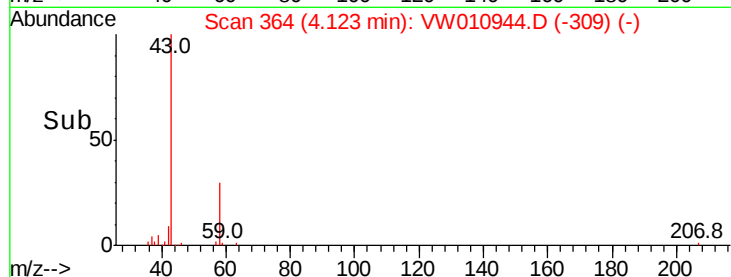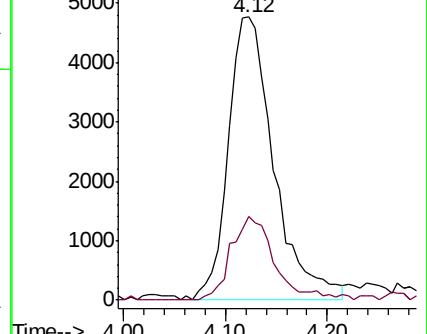

#15

Methyl Acetate

Concen: 6.018 ug/L

RT: 4.68 min Scan# 455

Delta R.T. 0.01 min

Lab File: VW010944.D


Acq: 24 Jun 2019 21:43

Tgt Ion: 43 Resp: 7415

Ion Ratio Lower Upper

43 100

74 14.3 15.3 22.9#

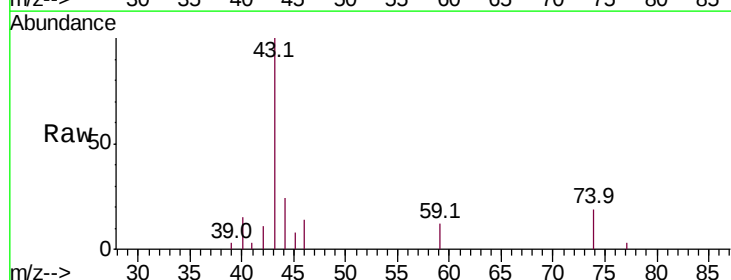

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 74.00 (73.70 to 74.70): VW

