

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019311.D
 Acq On : 24 Jun 2021 16:31
 Operator : SY/VA
 Sample : M2808-13
 Misc : 4.95G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGD1

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:12 PM

Quant Time: Jun 25 01:19:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

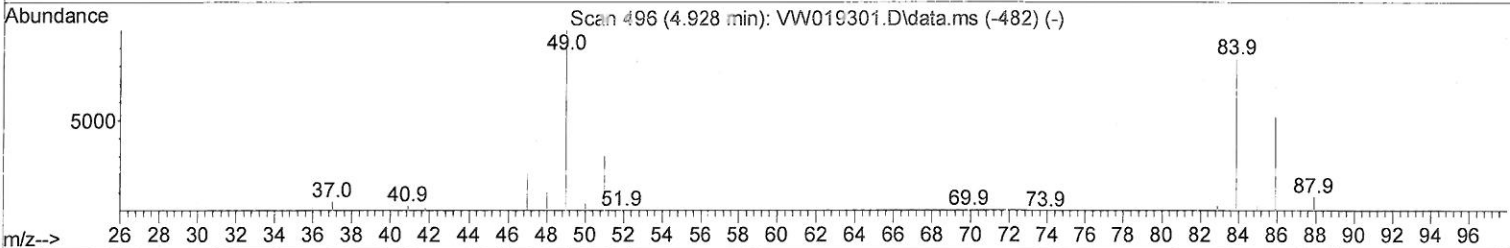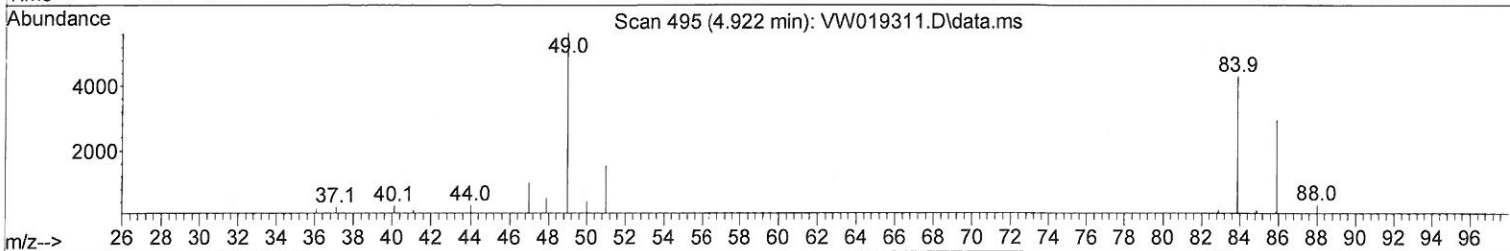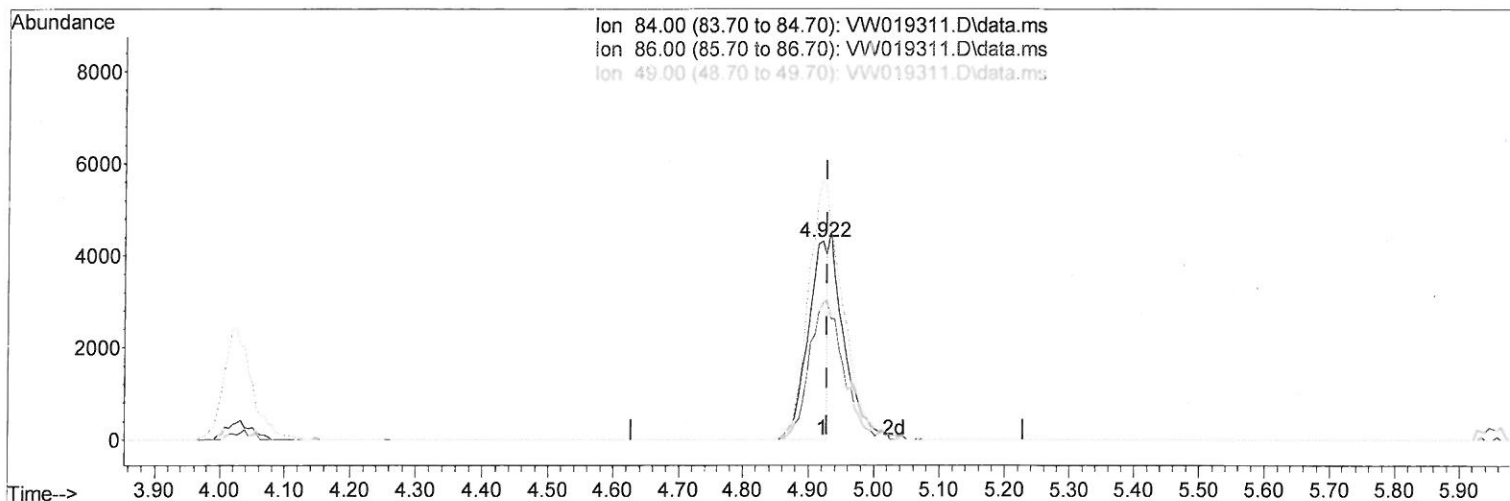

TIC: VW019311.D\data.ms

(16) Methylene chloride (T)

4.922min (-0.006) 0.92 ug/L

response 8987

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	68.87
49.00	123.70	131.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019311.D
 Acq On : 24 Jun 2021 16:31
 Operator : SY/VA
 Sample : M2808-13
 Misc : 4.95G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BGD1

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:12 PM

Quant Time: Jun 25 01:19:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

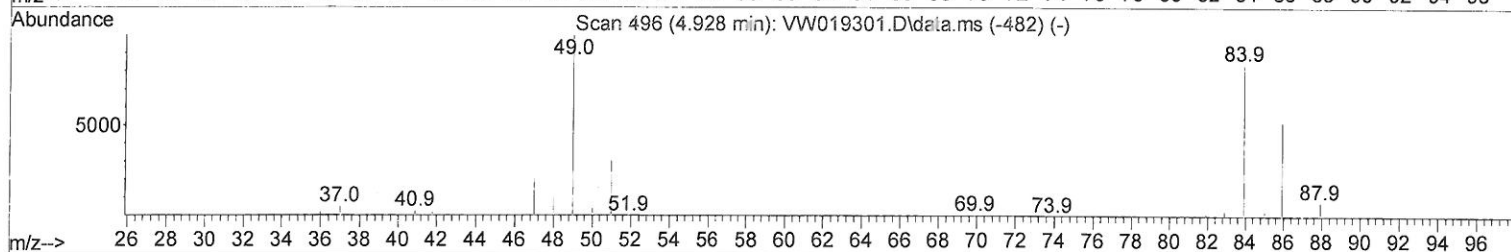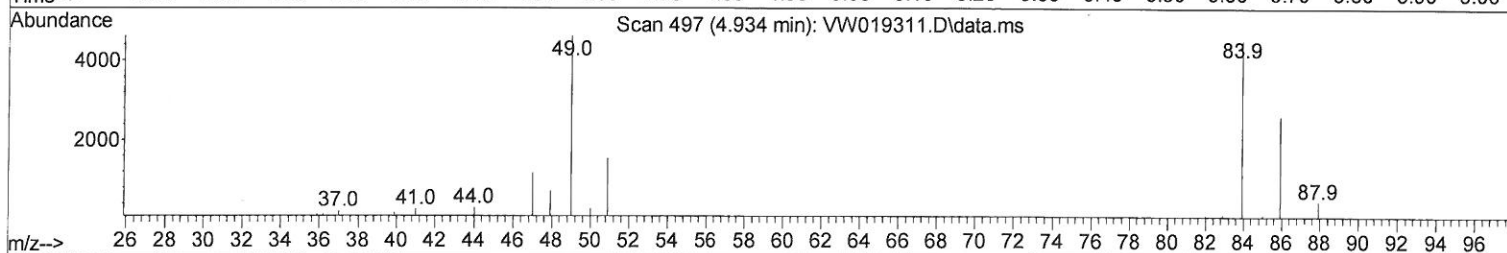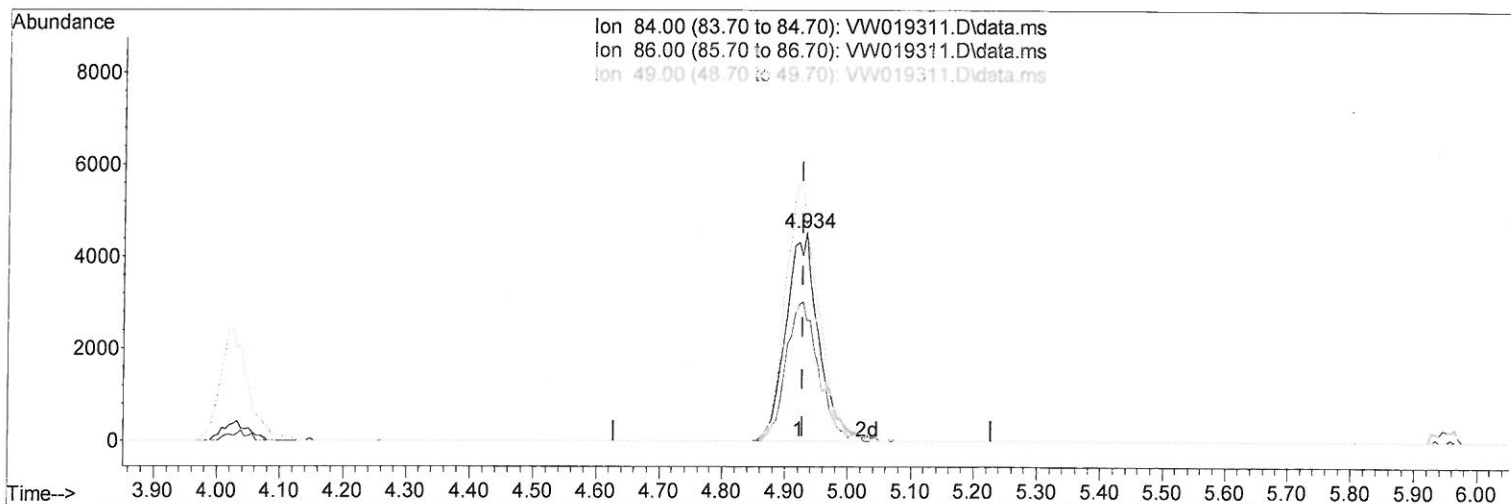

TIC: VW019311.D\data.ms

(16) Methylene chloride (T)

4.934min (+ 0.006) 1.69 ug/L m

response 16411

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	57.87
49.00	123.70	101.94
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019311.D
 Acq On : 24 Jun 2021 16:31
 Operator : SY/VA
 Sample : M2808-13
 Misc : 4.95G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGD1

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:12 PM

Quant Time: Jun 25 01:19:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	524548	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	450453	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	169386	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	165748	23.896	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	95.600%		
7) Chloroethane-d5	2.898	69	144816	24.513	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.040%		
11) 1,1-Dichloroethene-d2	4.025	63	247637	17.969	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.880%		
21) 2-Butanone-d5	7.080	46	70037	38.547	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.100%		
24) Chloroform-d	7.653	84	367254	26.042	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	104.160%		
26) 1,2-Dichloroethane-d4	8.311	65	189650	23.975	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	95.880%		
32) Benzene-d6	8.275	84	713239	27.791	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	111.160%		
36) 1,2-Dichloropropane-d6	9.274	67	219032	28.152	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	112.600%		
41) Toluene-d8	10.323	98	630400	26.746	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	107.000%		
43) trans-1,3-Dichloroprop...	10.579	79	71966	21.357	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.440%		
47) 2-Hexanone-d5	10.927	63	55104	41.766	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	83.540%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	141704	22.079	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.320%		
66) 1,2-Dichlorobenzene-d4	13.853	152	161731	27.356	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	109.440%		
Target Compounds						
13) Acetone	4.141	43	18617	11.563	ug/L	81
14) Carbon disulfide	4.391	76	7625	0.324	ug/L	98
16) Methylene chloride	4.934	84	16411m	1.686	ug/L	97
22) 2-Butanone	7.183	43	6150	2.857	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
Data File : VW019311.D
Acq On : 24 Jun 2021 16:31
Operator : SY/VA
Sample : M2808-13
Misc : 4.95G/10ML/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDT1

Manual Integrations
APPROVED

MMDadoda
6/25/2021 1:47:12 PM

Quant Time: Jun 25 01:19:19 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 25 01:15:57 2021
Response via : Initial Calibration

