

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019313.D
 Acq On : 24 Jun 2021 17:19
 Operator : SY/VA
 Sample : M2825-17
 Misc : 5.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDR5

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:15 PM

Quant Time: Jun 25 01:19:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

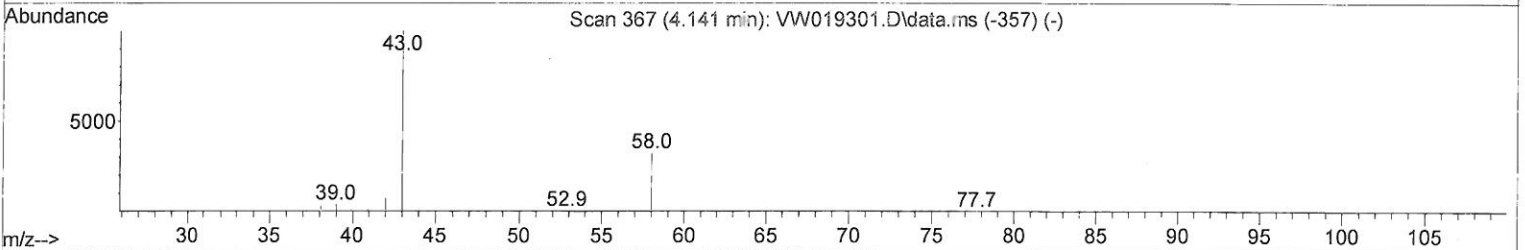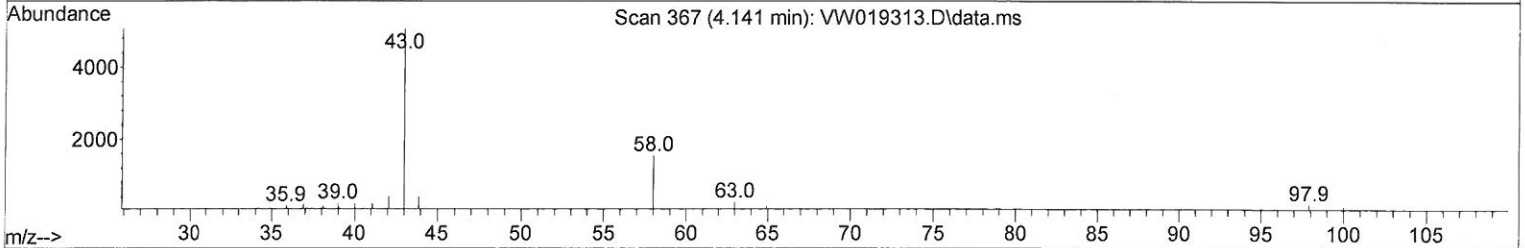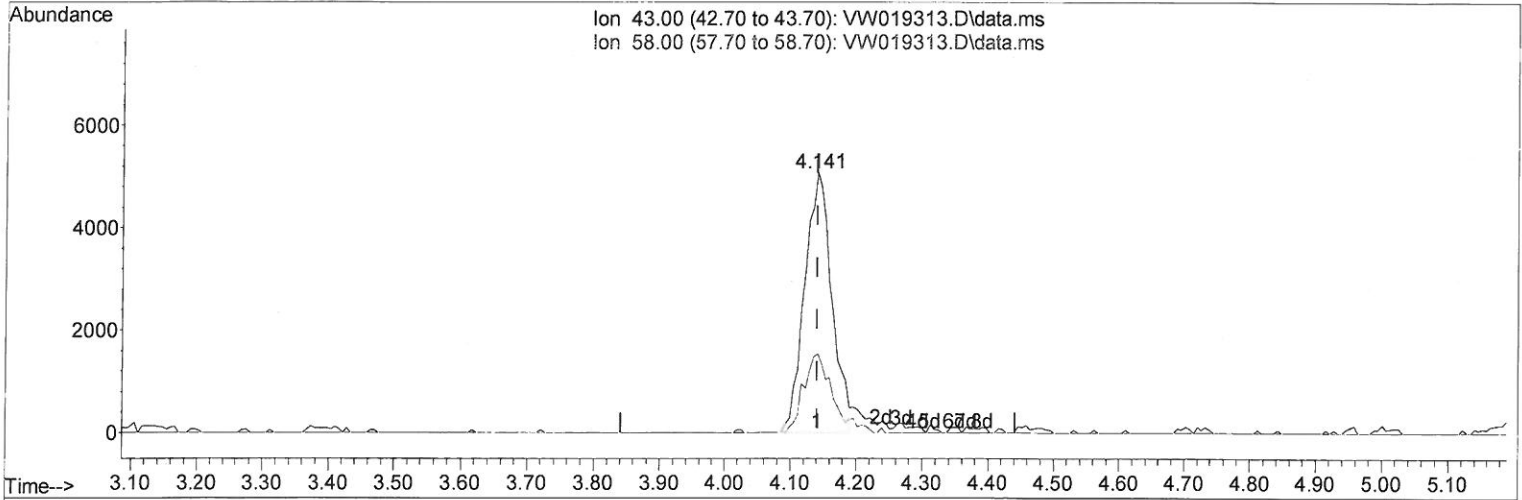

TIC: VW019313.D\data.ms

(13) Acetone (T)

4.141min (0.000) 9.05 ug/L

response 14639

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	29.73
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019313.D
 Acq On : 24 Jun 2021 17:19
 Operator : SY/VA
 Sample : M2825-17
 Misc : 5.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDR5

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:15 PM

Quant Time: Jun 25 01:19:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

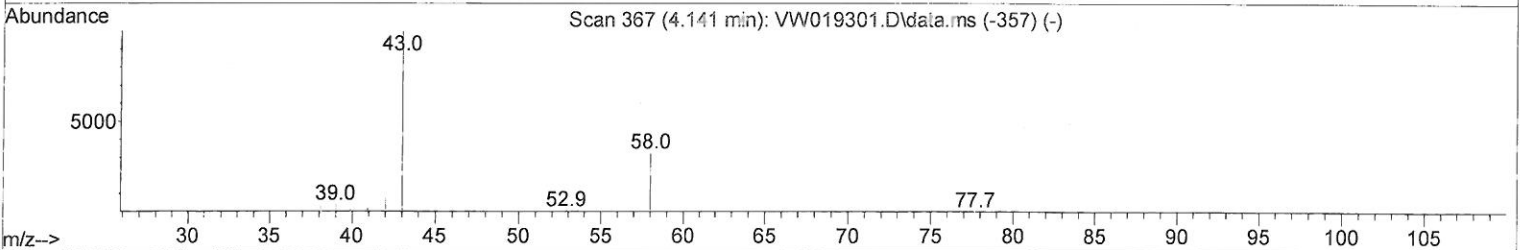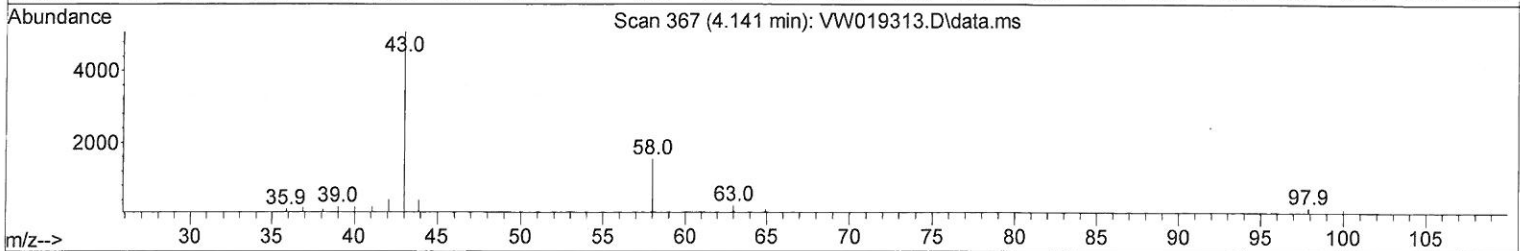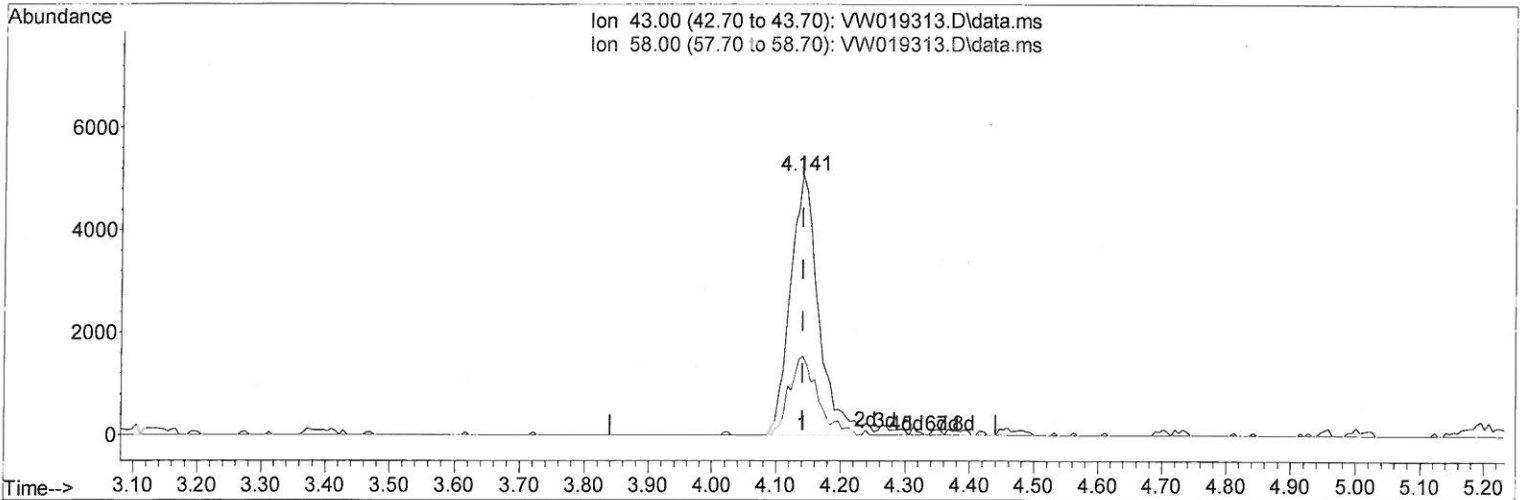

TIC: VW019313.D\data.ms

(13) Acetone (T)

4.141min (0.000) 9.54 ug/L m

response 15442

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	28.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019313.D
 Acq On : 24 Jun 2021 17:19
 Operator : SY/VA
 Sample : M2825-17
 Misc : 5.78G/10ML/MSVOA_W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDR5

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:15 PM

Quant Time: Jun 25 01:19:37 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	527155	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	476888	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	206467	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	159560	22.890	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.560%		
7) Chloroethane-d5	2.898	69	136443	22.982	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.920%		
11) 1,1-Dichloroethene-d2	4.025	63	233829	16.883	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.520%		
21) 2-Butanone-d5	7.086	46	64031	35.067	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	70.140%		
24) Chloroform-d	7.653	84	351114	24.774	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.080%		
26) 1,2-Dichloroethane-d4	8.305	65	176438	22.194	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.760%		
32) Benzene-d6	8.275	84	690888	25.428	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	101.720%		
36) 1,2-Dichloropropane-d6	9.274	67	207891	25.239	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	100.960%		
41) Toluene-d8	10.323	98	618478	24.786	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	99.160%		
43) trans-1,3-Dichloroprop...	10.579	79	74759	20.956	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.840%		
47) 2-Hexanone-d5	10.927	63	51292	36.722	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	73.440%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	134276	19.762	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	79.040%		
66) 1,2-Dichlorobenzene-d4	13.853	152	179790	24.948	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.800%		
Target Compounds						
13) Acetone	4.141	43	15442m	9.544	ug/L	Qvalue 96/25/21 Sey
14) Carbon disulfide	4.397	76	31458	1.331	ug/L #	94
16) Methylene chloride	4.922	84	16654	1.703	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
Data File : VW019313.D
Acq On : 24 Jun 2021 17:19
Operator : SY/VA
Sample : M2825-17
Misc : 5.78G/10ML/MSVOA_W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDR5

Manual Integrations
APPROVED

MMDadoda
6/25/2021 1:47:15 PM

Quant Time: Jun 25 01:19:37 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 25 01:15:57 2021
Response via : Initial Calibration

