

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019316.D
 Acq On : 24 Jun 2021 18:31
 Operator : SY/VA
 Sample : M2854-02RE
 Misc : 5.68G/10ML/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BGDS3RE

Manual Integrations
APPROVED

MMDadoda
 6/25/2021 1:47:20 PM

Quant Time: Jun 25 01:20:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

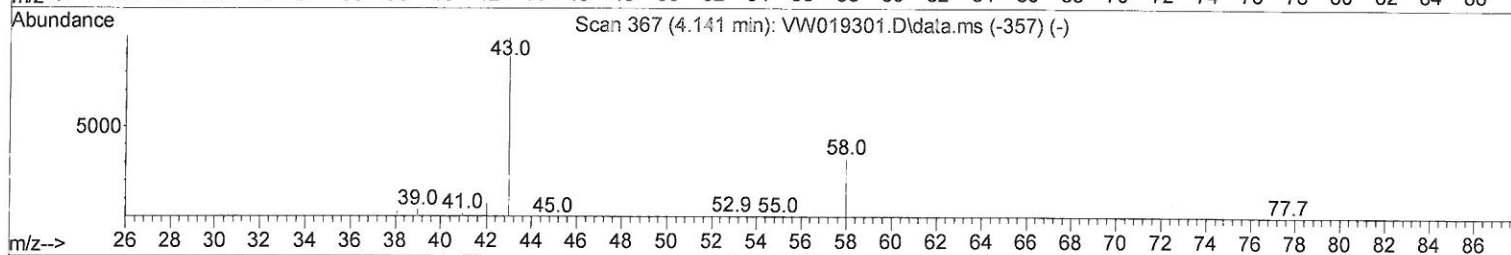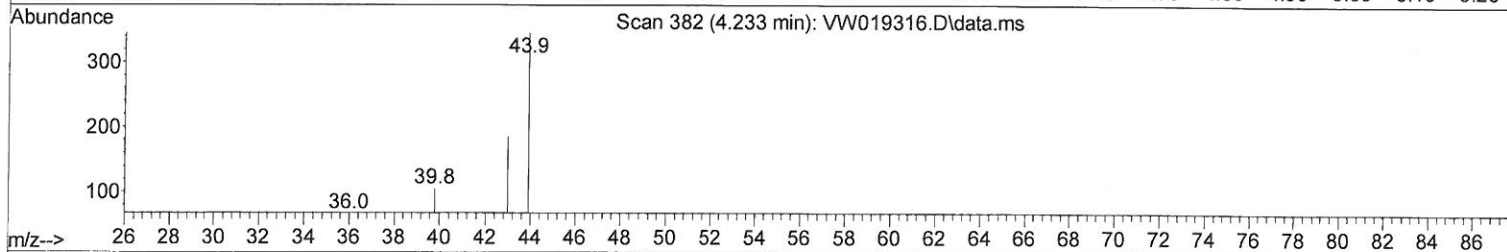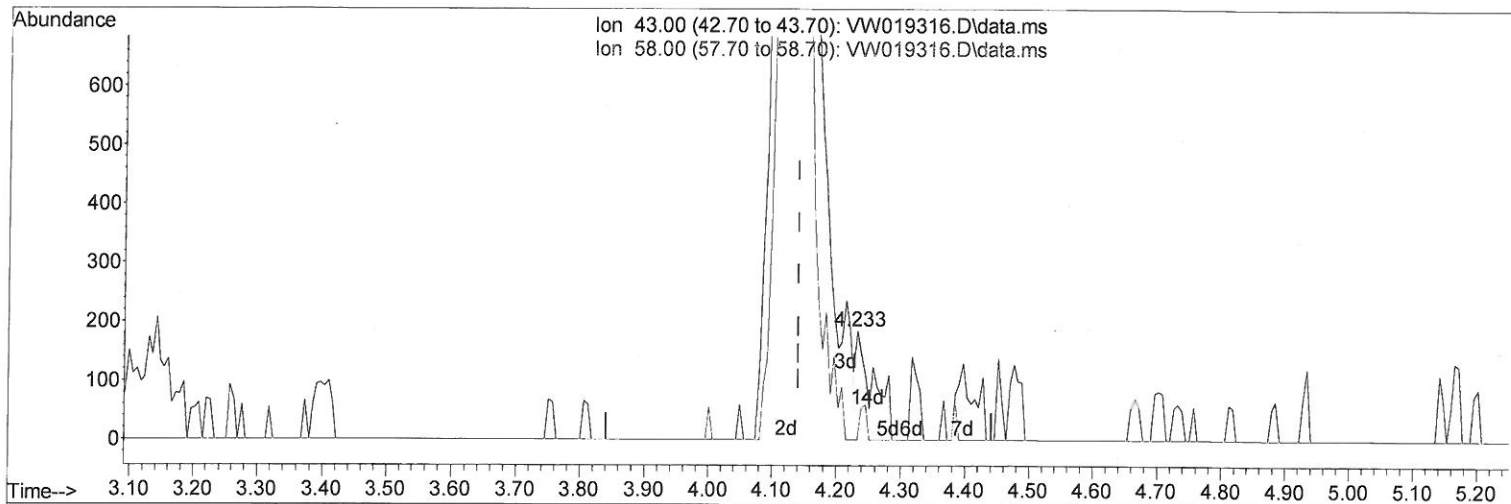

TIC: VW019316.D\data.ms

(13) Acetone (T)

4.233min (+ 0.091) 0.13 ug/L

response 102

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	41.18
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019316.D
 Acq On : 24 Jun 2021 18:31
 Operator : SY/VA
 Sample : M2854-02RE
 Misc : 5.68G/10ML/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDS3RE

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:20 PM

Quant Time: Jun 25 01:20:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

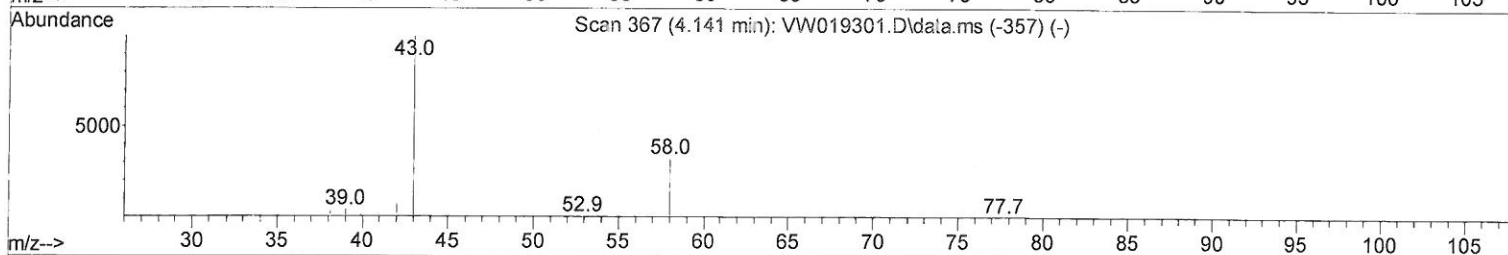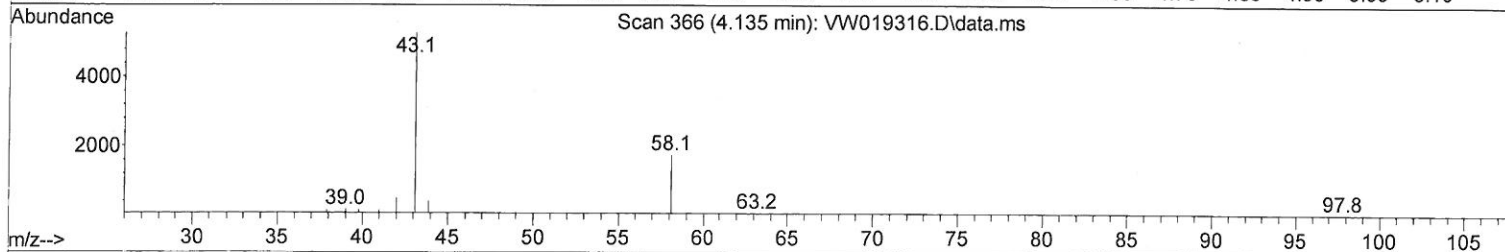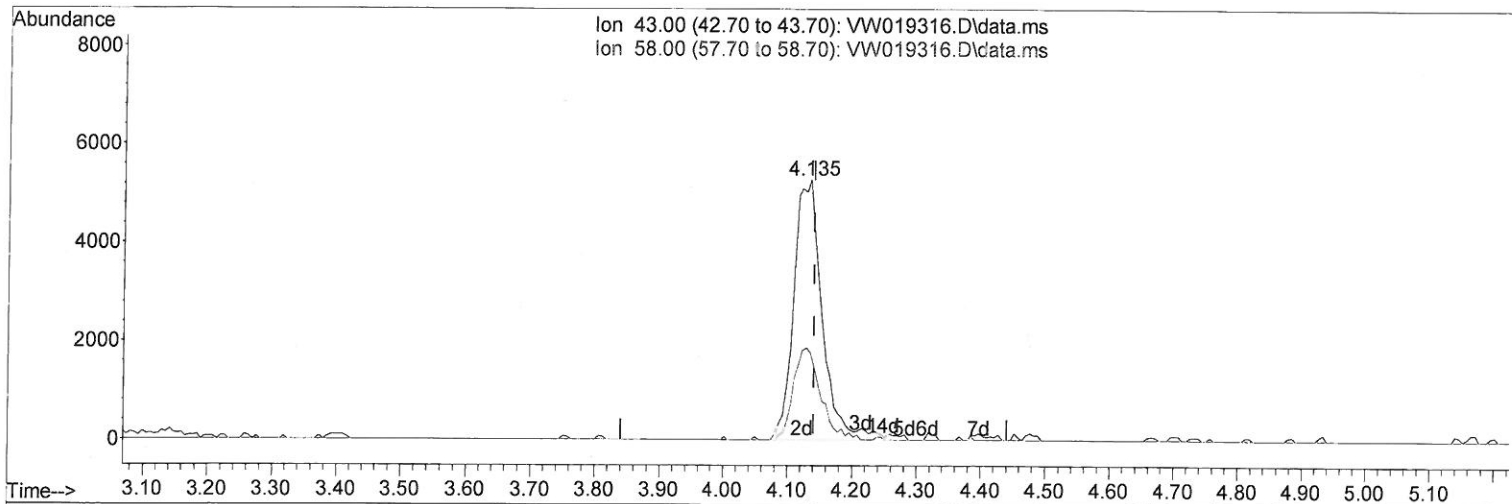

TIC: VW019316.D\data.ms

(13) Acetone (T)

4.135min (-0.006) 20.43 ug/L m

response 15880

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	0.26
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
Data File : VW019316.D
Acq On : 24 Jun 2021 18:31
Operator : SY/VA
Sample : M2854-02RE
Misc : 5.68G/10ML/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDS3RE

Manual Integrations
APPROVED

MMDadoda
6/25/2021 1:47:20 PM

Quant Time: Jun 25 01:20:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 25 01:15:57 2021
Response via : Initial Calibration

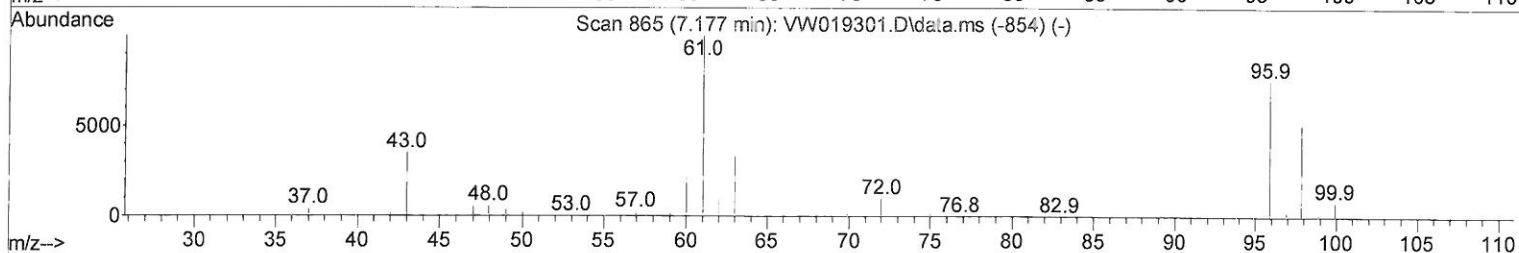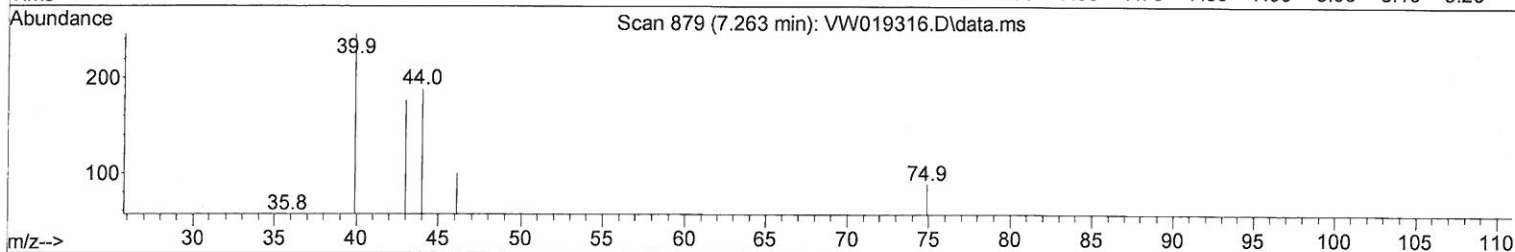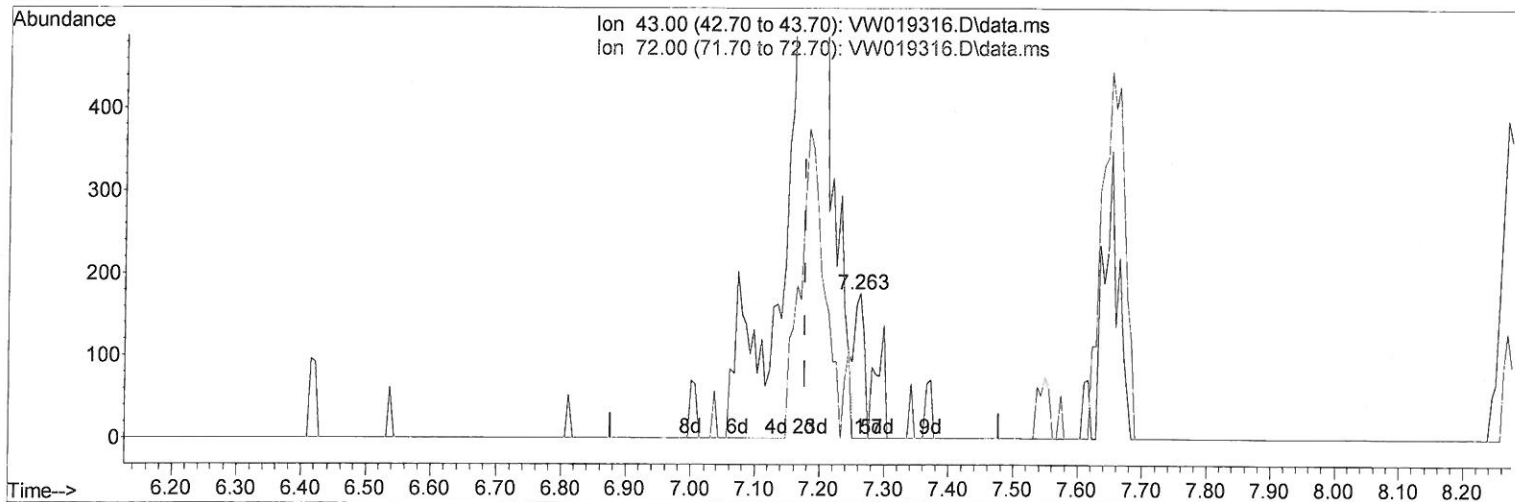

TIC: VW019316.D\data.ms

(22) 2-Butanone (T)

7.263min (+ 0.085) 0.16 ug/L

response 169

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	37.87
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019316.D
 Acq On : 24 Jun 2021 18:31
 Operator : SY/VA
 Sample : M2854-02RE
 Misc : 5.68G/10ML/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDS3RE

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:20 PM

Quant Time: Jun 25 01:20:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

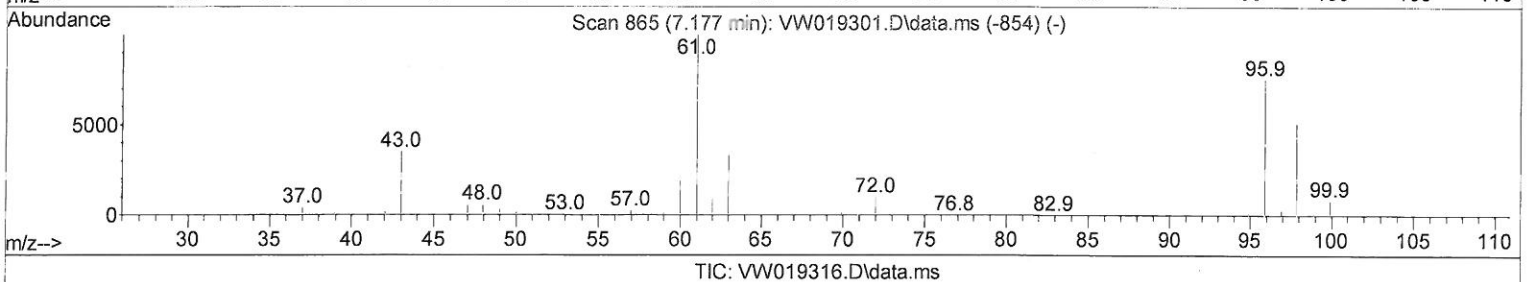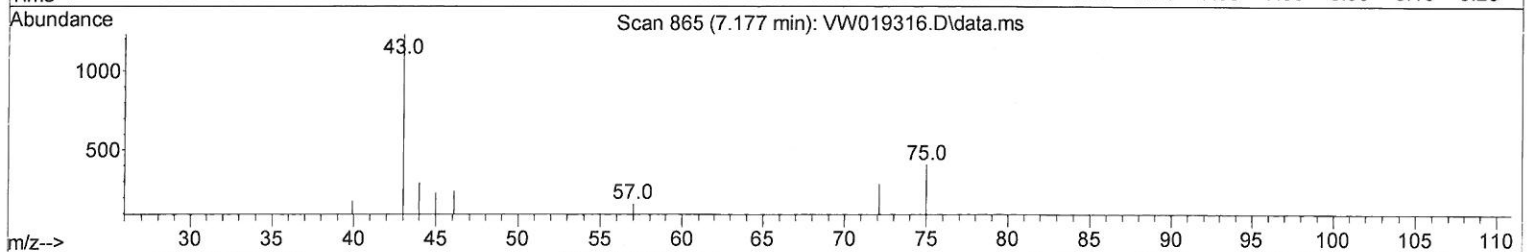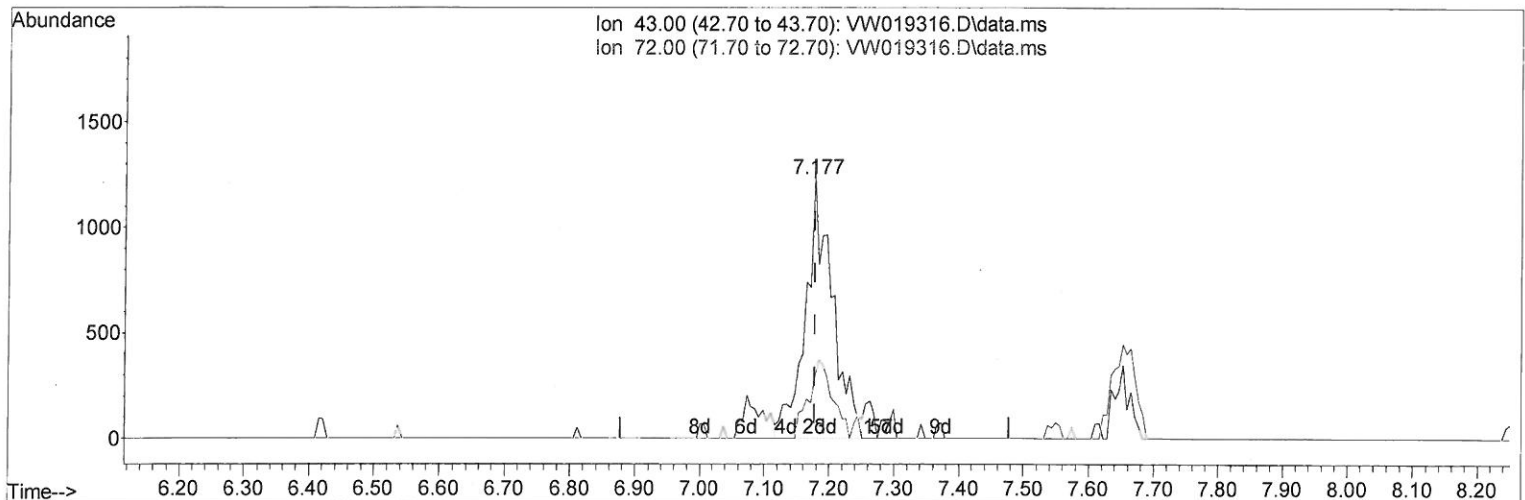

(22) 2-Butanone (T)

7.177min (-0.000) 3.43 ug/L m

response 3562

Ion	Exp%	Act%
43.00	100.00	100.00
72.00	29.80	1.80#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
 Data File : VW019316.D
 Acq On : 24 Jun 2021 18:31
 Operator : SY/VA
 Sample : M2854-02RE
 Misc : 5.68G/10ML/MSVOA_W/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDS3RE

Manual Integrations
 APPROVED

MMDadoda
 6/25/2021 1:47:20 PM

Quant Time: Jun 25 01:20:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 25 01:15:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	253228	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	240288	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	98673	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	72068	21.522	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	86.080%		
7) Chloroethane-d5	2.897	69	63121	22.133	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	88.520%		
11) 1,1-Dichloroethene-d2	4.019	63	111925	16.823	ug/L	-0.01
Spiked Amount	25.000	Range 45 - 110	Recovery =	67.280%		
21) 2-Butanone-d5	7.080	46	40056	45.668	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	91.340%		
24) Chloroform-d	7.653	84	175457	25.772	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	103.080%		
26) 1,2-Dichloroethane-d4	8.311	65	95507	25.010	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	100.040%		
32) Benzene-d6	8.275	84	333299	24.346	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	97.400%		
36) 1,2-Dichloropropane-d6	9.274	67	108648	26.178	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	104.720%		
41) Toluene-d8	10.323	98	282061	22.434	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	89.720%		
43) trans-1,3-Dichloroprop...	10.579	79	39530	21.992	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	87.960%		
47) 2-Hexanone-d5	10.927	63	30684	43.598	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	87.200%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	79191	23.131	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	92.520%		
66) 1,2-Dichlorobenzene-d4	13.853	152	90356	26.235	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	104.960%		
Target Compounds						
13) Acetone	4.135	43	15880m	20.431	ug/L	Qvalue
14) Carbon disulfide	4.379	76	3783	0.333	ug/L	# 90
16) Methylene chloride	4.922	84	7699	1.639	ug/L	85
22) 2-Butanone	7.177	43	3562m	3.428	ug/L	0.6/25/21 Sy

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062421\
Data File : VW019316.D
Acq On : 24 Jun 2021 18:31
Operator : SY/VA
Sample : M2854-02RE
Misc : 5.68G/10ML/MSVOA_W/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDS3RE

Manual Integrations
APPROVED

MMDadoda
6/25/2021 1:47:20 PM

Quant Time: Jun 25 01:20:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
Qlast Update : Fri Jun 25 01:15:57 2021
Response via : Initial Calibration

