

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062518\
 Data File : VW003550.D
 Acq On : 25 Jun 2018 15:54
 Operator : SY/AP
 Sample : J3621-18
 Misc : 8.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAZ84

Quant Time: Jun 26 03:05:59 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 26 03:05:07 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	240752	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.64	117	230286	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	98189	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	71019	21.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.00%
7) Chloroethane-d5	2.89	69	60215	22.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.40%
10) 1,1-Dichloroethene-d2	4.01	63	108562	16.74	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.96%
20) 2-Butanone-d5	7.09	46	44221	42.98	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.96%
24) Chloroform-d	7.65	84	161788	25.55	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.20%
26) 1,2-Dichloroethane-d4	8.31	65	99812	26.52	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.08%
29) Benzene-d6	8.28	84	293968	24.06	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.24%
33) 1,2-Dichloropropane-d6	9.28	67	98766	25.54	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.16%
37) Toluene-d8	10.33	98	259883	22.25	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.00%
38) trans-1,3-Dichloropropene-	10.58	79	38846	21.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.56%
39) 2-Hexanone-d5	10.93	63	28955	36.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.26%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	89735	24.94	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.76%
61) 1,2-Dichlorobenzene-d4	13.87	152	95070	25.64	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.56%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.15	43	2597	2.368	ug/L	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW062518\
Data File : VW003550.D
Acq On : 25 Jun 2018 15:54
Operator : SY/AP
Sample : J3621-18
Misc : 8.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAZ84

Quant Time: Jun 26 03:05:59 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 26 03:05:07 2018
Response via : Initial Calibration

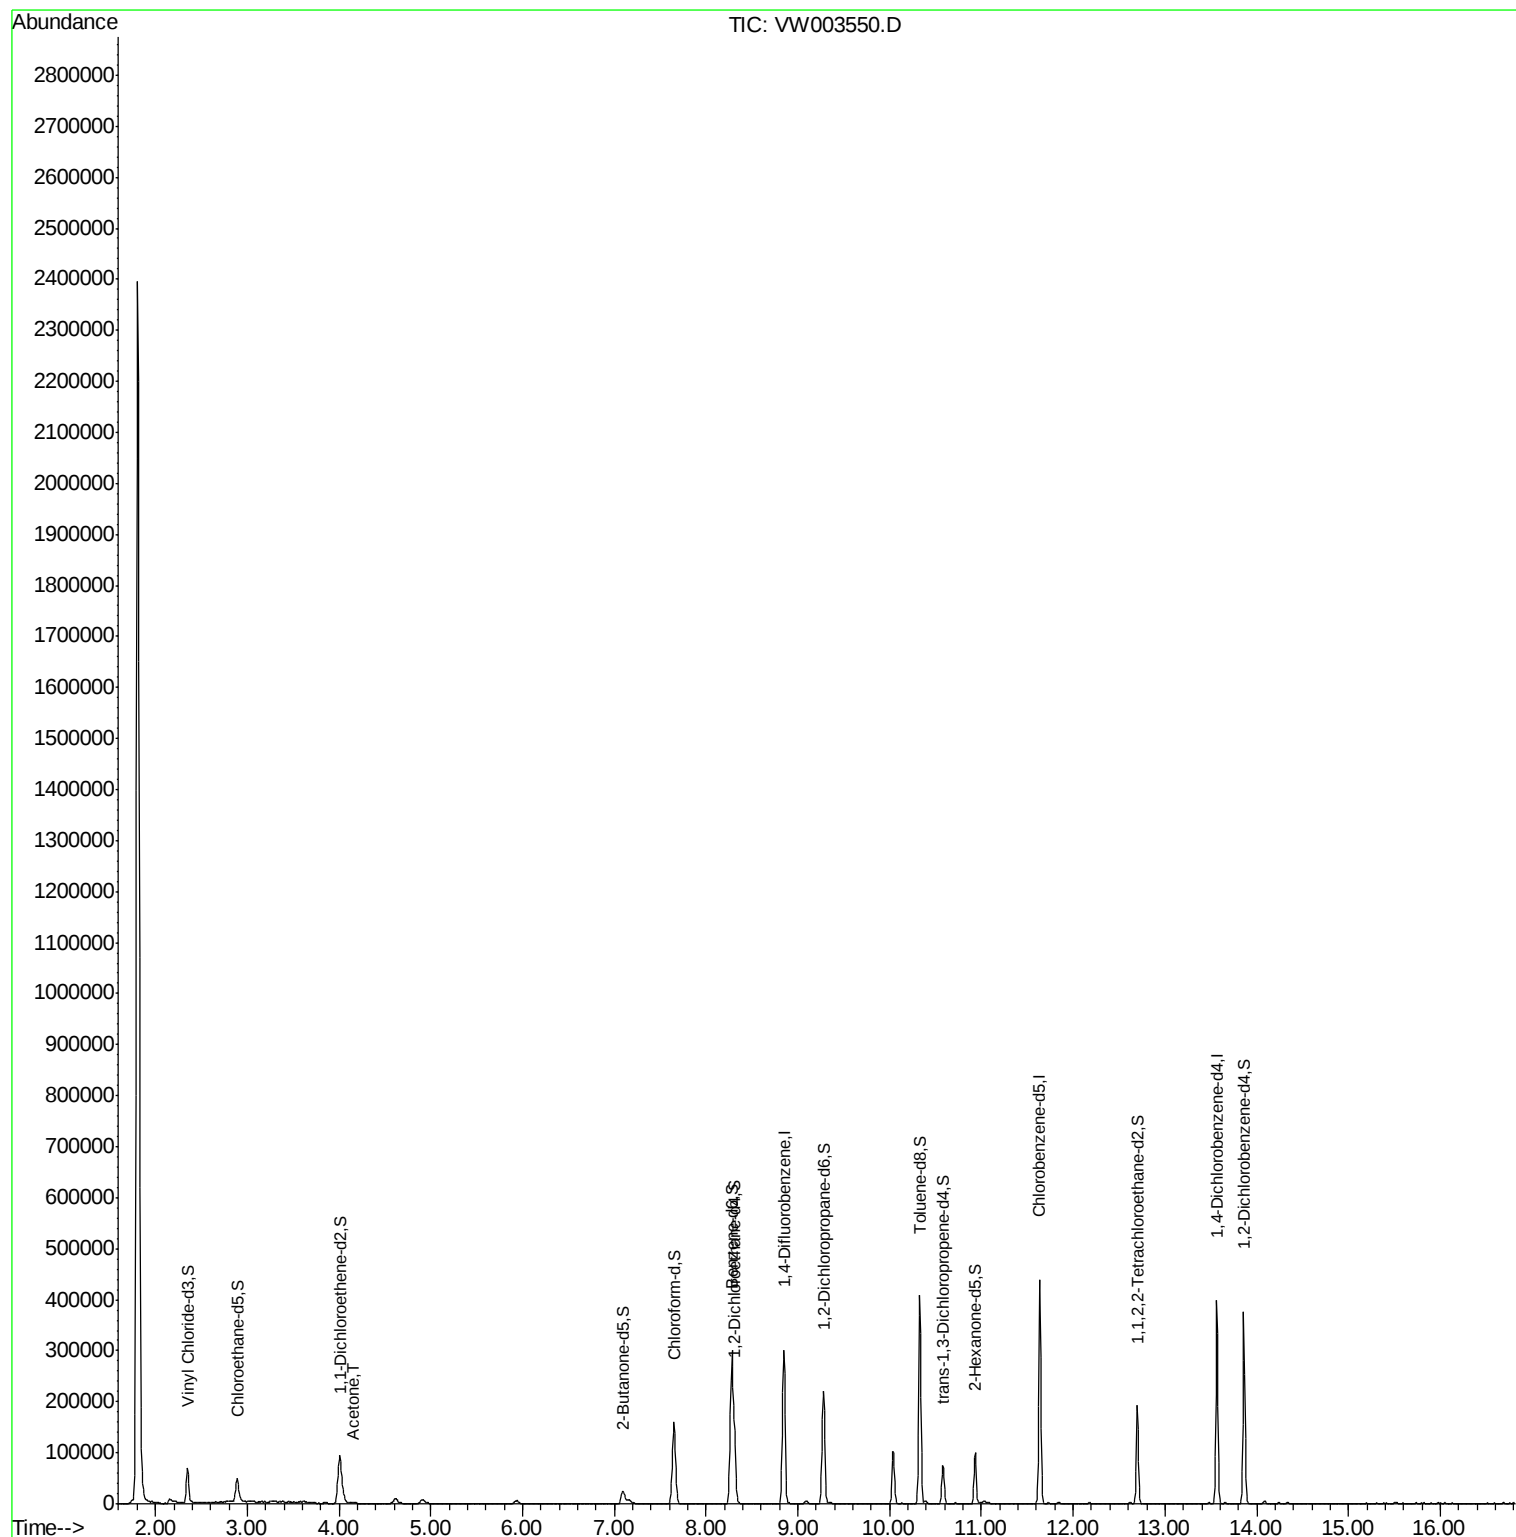

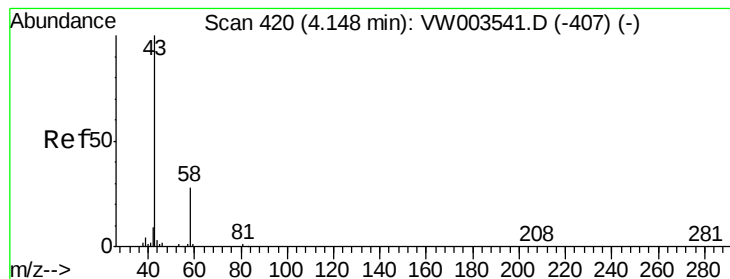

#13

Acetone

Concen: 2.368 ug/L

RT: 4.15 min Scan# 421

Delta R.T. 0.01 min

Lab File: VW003550.D

Acq: 25 Jun 2018 15:54

Instrument :

MSVOA_W

ClientSampleId :


DAZ84

Tgt Ion: 43 Resp: 2597

Ion Ratio Lower Upper

43 100

58 1.4 0.0 58.6

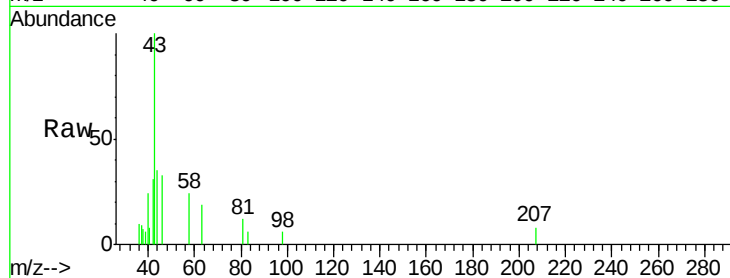

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

