

Data File : VW010961.D
Acq On : 25 Jun 2019 12:07
Operator : SY/VA
Sample : K3456-04
Misc : 1.91G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANX4

Quant Time: Jun 26 02:59:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 02:56:20 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	358845	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	316363	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	145880	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	98672	21.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.84%
7) Chloroethane-d5	2.88	69	73807	20.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.32%
10) 1,1-Dichloroethene-d2	4.01	63	169046	15.38	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.52%
20) 2-Butanone-d5	7.07	46	84902	38.87	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	77.74%
24) Chloroform-d	7.65	84	216514	22.37	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.48%
26) 1,2-Dichloroethane-d4	8.31	65	134787	22.47	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.88%
29) Benzene-d6	8.27	84	445420	23.45	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.80%
33) 1,2-Dichloropropane-d6	9.27	67	147093	23.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.76%
37) Toluene-d8	10.32	98	400308	23.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.44%
38) trans-1,3-Dichloropropene-	10.58	79	55451	19.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.84%
39) 2-Hexanone-d5	10.93	63	56587	40.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	108649	21.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	131740	23.92	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.68%


Target Compounds					Qvalue
13) Acetone	4.13	43	3754	1.795 ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW010961.D
Acq On : 25 Jun 2019 12:07
Operator : SY/VA
Sample : K3456-04
Misc : 1.91G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANX4

Quant Time: Jun 26 02:59:24 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 02:56:20 2019
Response via : Initial Calibration

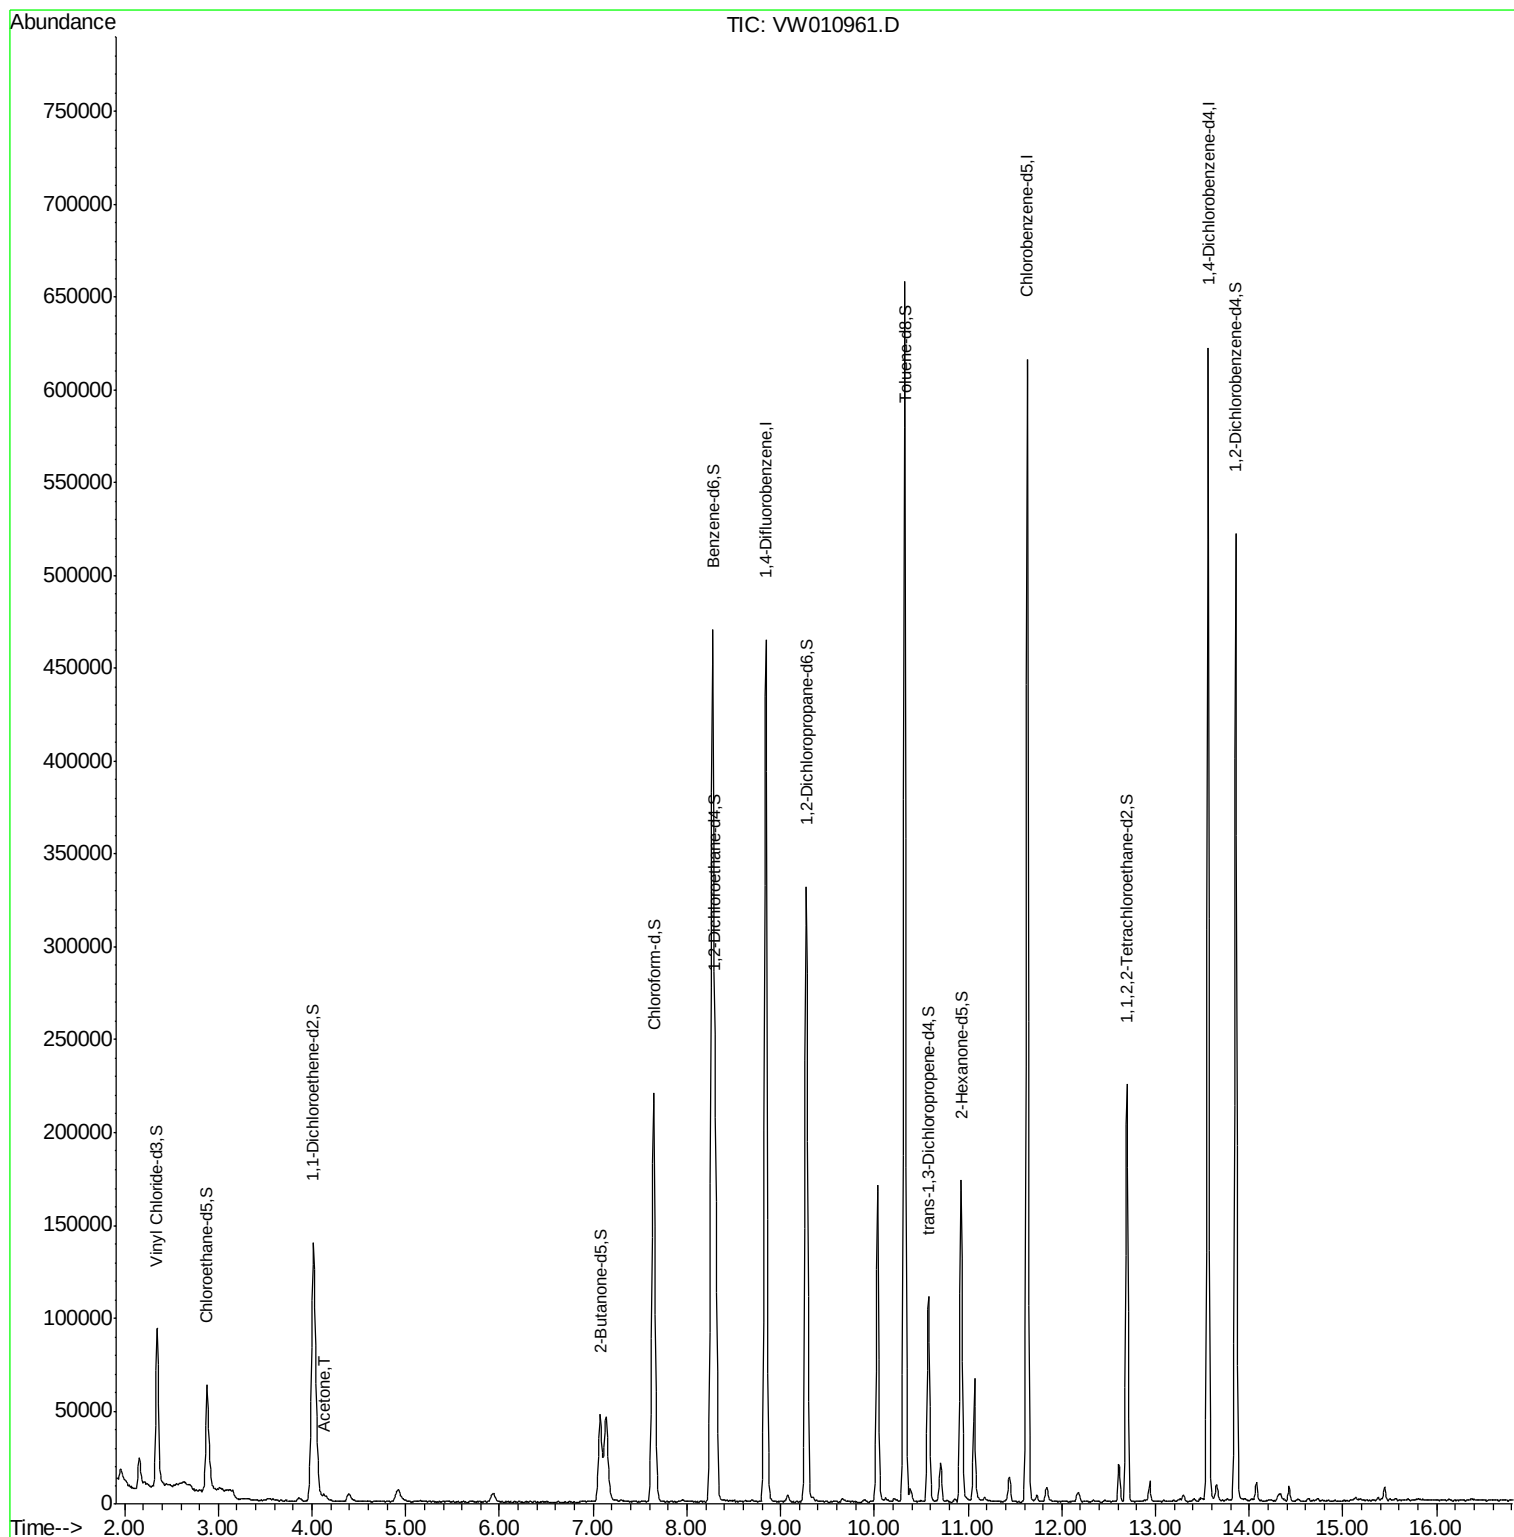

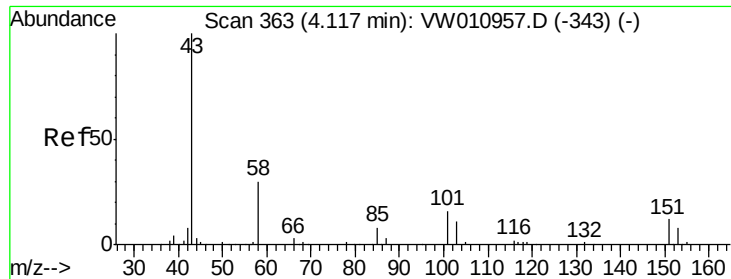

#13

Acetone

Concen: 1.795 ug/L

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW010961.D

Acq: 25 Jun 2019 12:07

Instrument :
MSVOA_W
ClientSampleId :
YANX4

Tgt Ion: 43 Resp: 3754

Ion Ratio Lower Upper

43 100

58 28.7 0.0 53.2

