

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062519\
Quantitation Report (Qedit)




Data File : VW010981.D
Acq On : 25 Jun 2019 21:42
Operator : SY/VA
Sample : K3460-09
Misc : 3.60G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANW3

Manual Integrations
APPROVED

MMDadoda
7/3/2019 9:13:15 AM

Quant Time: Jun 26 04:41:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 04:33:18 2019
Response via : Initial Calibration

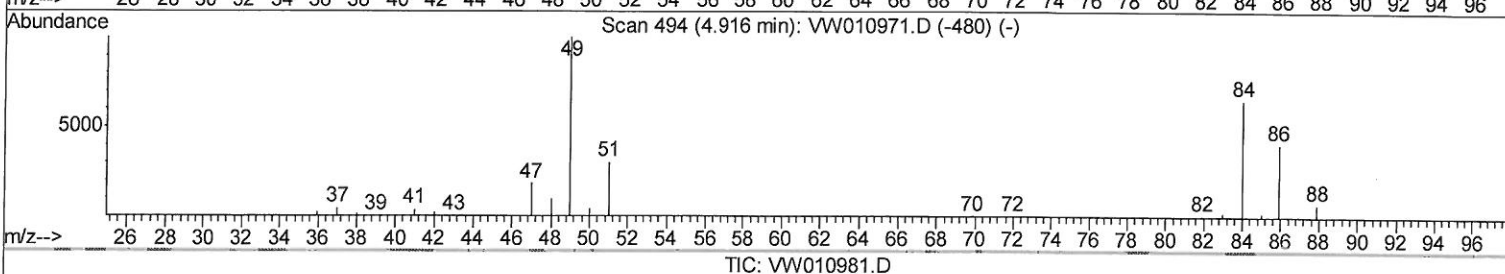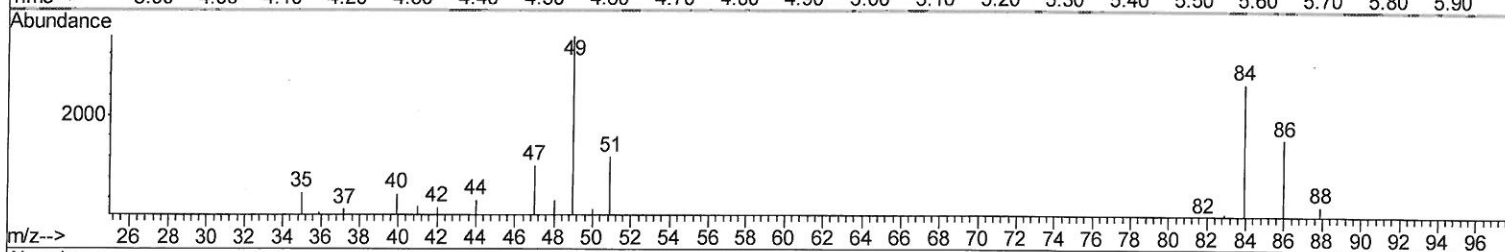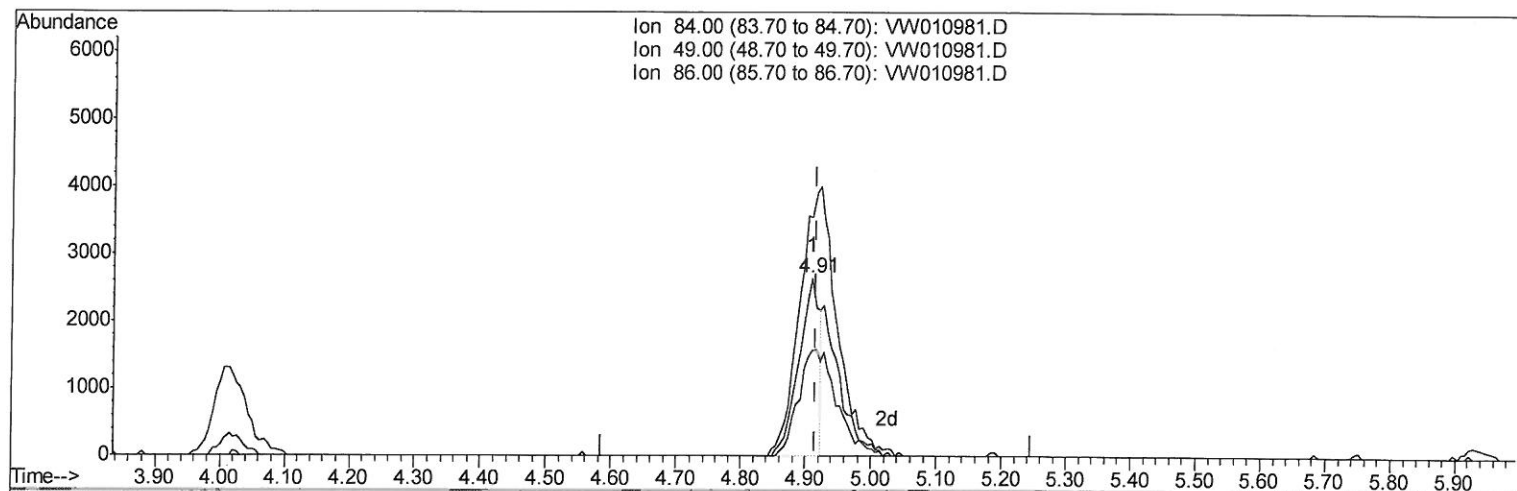

TIC: VW010981.D

(16) Methylene chloride (T)

4.910min (-0.006) 1.24ug/L

response 5793

Ion	Exp%	Act%
84.00	100	100
49.00	152.90	134.09
86.00	63.50	58.87
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062519\
Quantitation Report (Qedit)




Data File : VW010981.D
Acq On : 25 Jun 2019 21:42
Operator : SY/VA
Sample : K3460-09
Misc : 3.60G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANW3

Manual Integrations
APPROVED

MMDadoda
7/3/2019 9:13:15 AM

Quant Time: Jun 26 04:41:20 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 04:33:18 2019
Response via : Initial Calibration

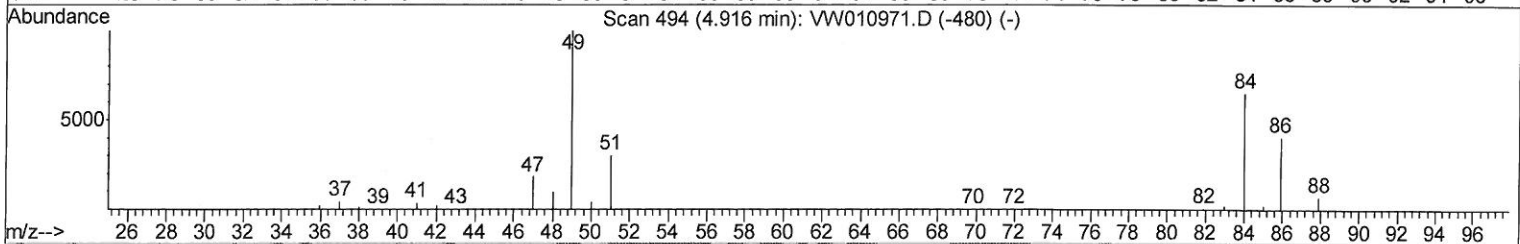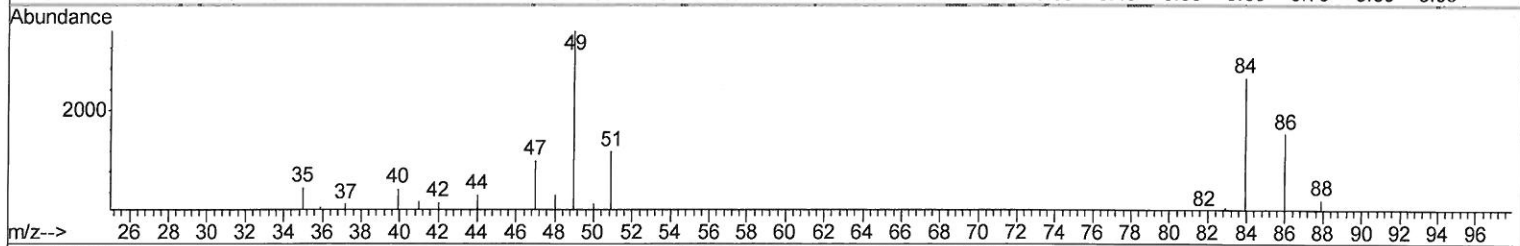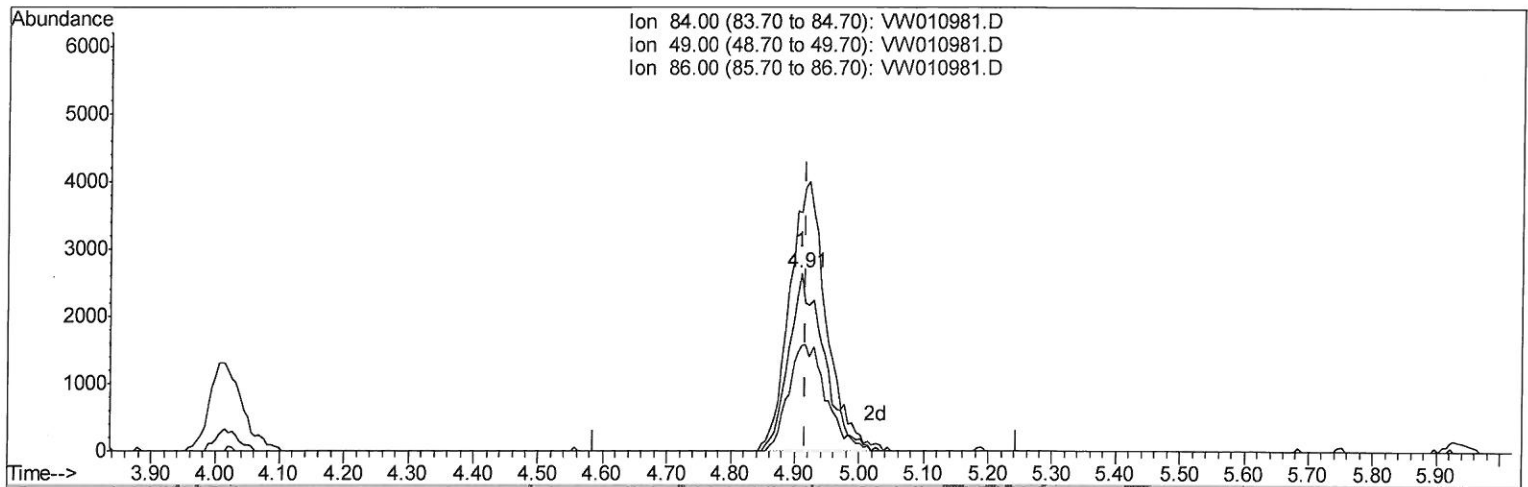

TIC: VW010981.D

(16) Methylene chloride (T)

4.910min (-0.006) 2.15ug/L m

response 10049

Ion	Exp%	Act%
84.00	100	100
49.00	152.90	134.09
86.00	63.50	58.87
0.00	0.00	0.00

706/26/19 53

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062519\
Quantitation Report (QT Reviewed)

Data File : VW010981.D
Acq On : 25 Jun 2019 21:42
Operator : SY/VA
Sample : K3460-09
Misc : 3.60G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANW3

Manual Integrations
APPROVED

MMDadoda
7/3/2019 9:13:15 AM

Quant Time: Jun 26 05:26:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 04:33:18 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	315637	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	260643	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	88714	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	88960	21.74	ug/L	-0.01
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.96%		
7) Chloroethane-d5	2.88	69	67956	21.55	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	86.20%		
10) 1,1-Dichloroethene-d2	4.01	63	151347	15.65	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.60%		
20) 2-Butanone-d5	7.07	46	86823	45.19	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.38%		
24) Chloroform-d	7.64	84	211044	24.79	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.16%		
26) 1,2-Dichloroethane-d4	8.31	65	143370	27.17	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	108.68%		
29) Benzene-d6	8.27	84	421440	26.93	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	107.72%		
33) 1,2-Dichloropropane-d6	9.27	67	148211	28.66	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	114.64%		
37) Toluene-d8	10.32	98	356965	25.28	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	101.12%		
38) trans-1,3-Dichloropropene-	10.58	79	52294	22.85	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.40%		
39) 2-Hexanone-d5	10.93	63	58823	50.62	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	101.24%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	115035	26.99	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	107.96%		
61) 1,2-Dichlorobenzene-d4	13.85	152	84379	25.20	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	100.80%		

Target Compounds

					Qvalue
13) Acetone	4.12	43	5117	2.781 ug/L	97
16) Methylene chloride	4.91	84	10049m	2.150 ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062519\
Quantitation Report (QT Reviewed)

Data File : VW010981.D
Acq On : 25 Jun 2019 21:42
Operator : SY/VA
Sample : K3460-09
Misc : 3.60G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANW3

Manual Integrations
APPROVED

MMDadoda
7/3/2019 9:13:15 AM

Quant Time: Jun 26 05:26:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 04:33:18 2019
Response via : Initial Calibration

