

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062519\
 Data File : VW010960.D
 Acq On : 25 Jun 2019 11:40
 Operator : SY/VA
 Sample : K3456-11
 Misc : 4.98G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANT5

Quant Time: Jun 26 03:51:35 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 26 02:56:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	367918	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	318679	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	136887	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	105411	22.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.40%
7) Chloroethane-d5	2.89	69	80816	21.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.92%
10) 1,1-Dichloroethene-d2	4.01	63	181889	16.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.56%
20) 2-Butanone-d5	7.07	46	95930	42.83	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.66%
24) Chloroform-d	7.65	84	225031	22.68	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.72%
26) 1,2-Dichloroethane-d4	8.31	65	141896	23.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	92.28%
29) Benzene-d6	8.27	84	466185	24.37	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.48%
33) 1,2-Dichloropropane-d6	9.27	67	155610	24.61	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.44%
37) Toluene-d8	10.32	98	415032	24.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	96.16%
38) trans-1,3-Dichloropropene-	10.58	79	59146	21.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.56%
39) 2-Hexanone-d5	10.93	63	63579	44.75	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.50%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	118625	22.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.08%
61) 1,2-Dichlorobenzene-d4	13.86	152	125271	24.24	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.96%


Target Compounds					Ovalue
13) Acetone	4.12	43	9027	4.209 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062519\
Data File : VW010960.D
Acq On : 25 Jun 2019 11:40
Operator : SY/VA
Sample : K3456-11
Misc : 4.98G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANT5

Quant Time: Jun 26 03:51:35 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 02:56:20 2019
Response via : Initial Calibration

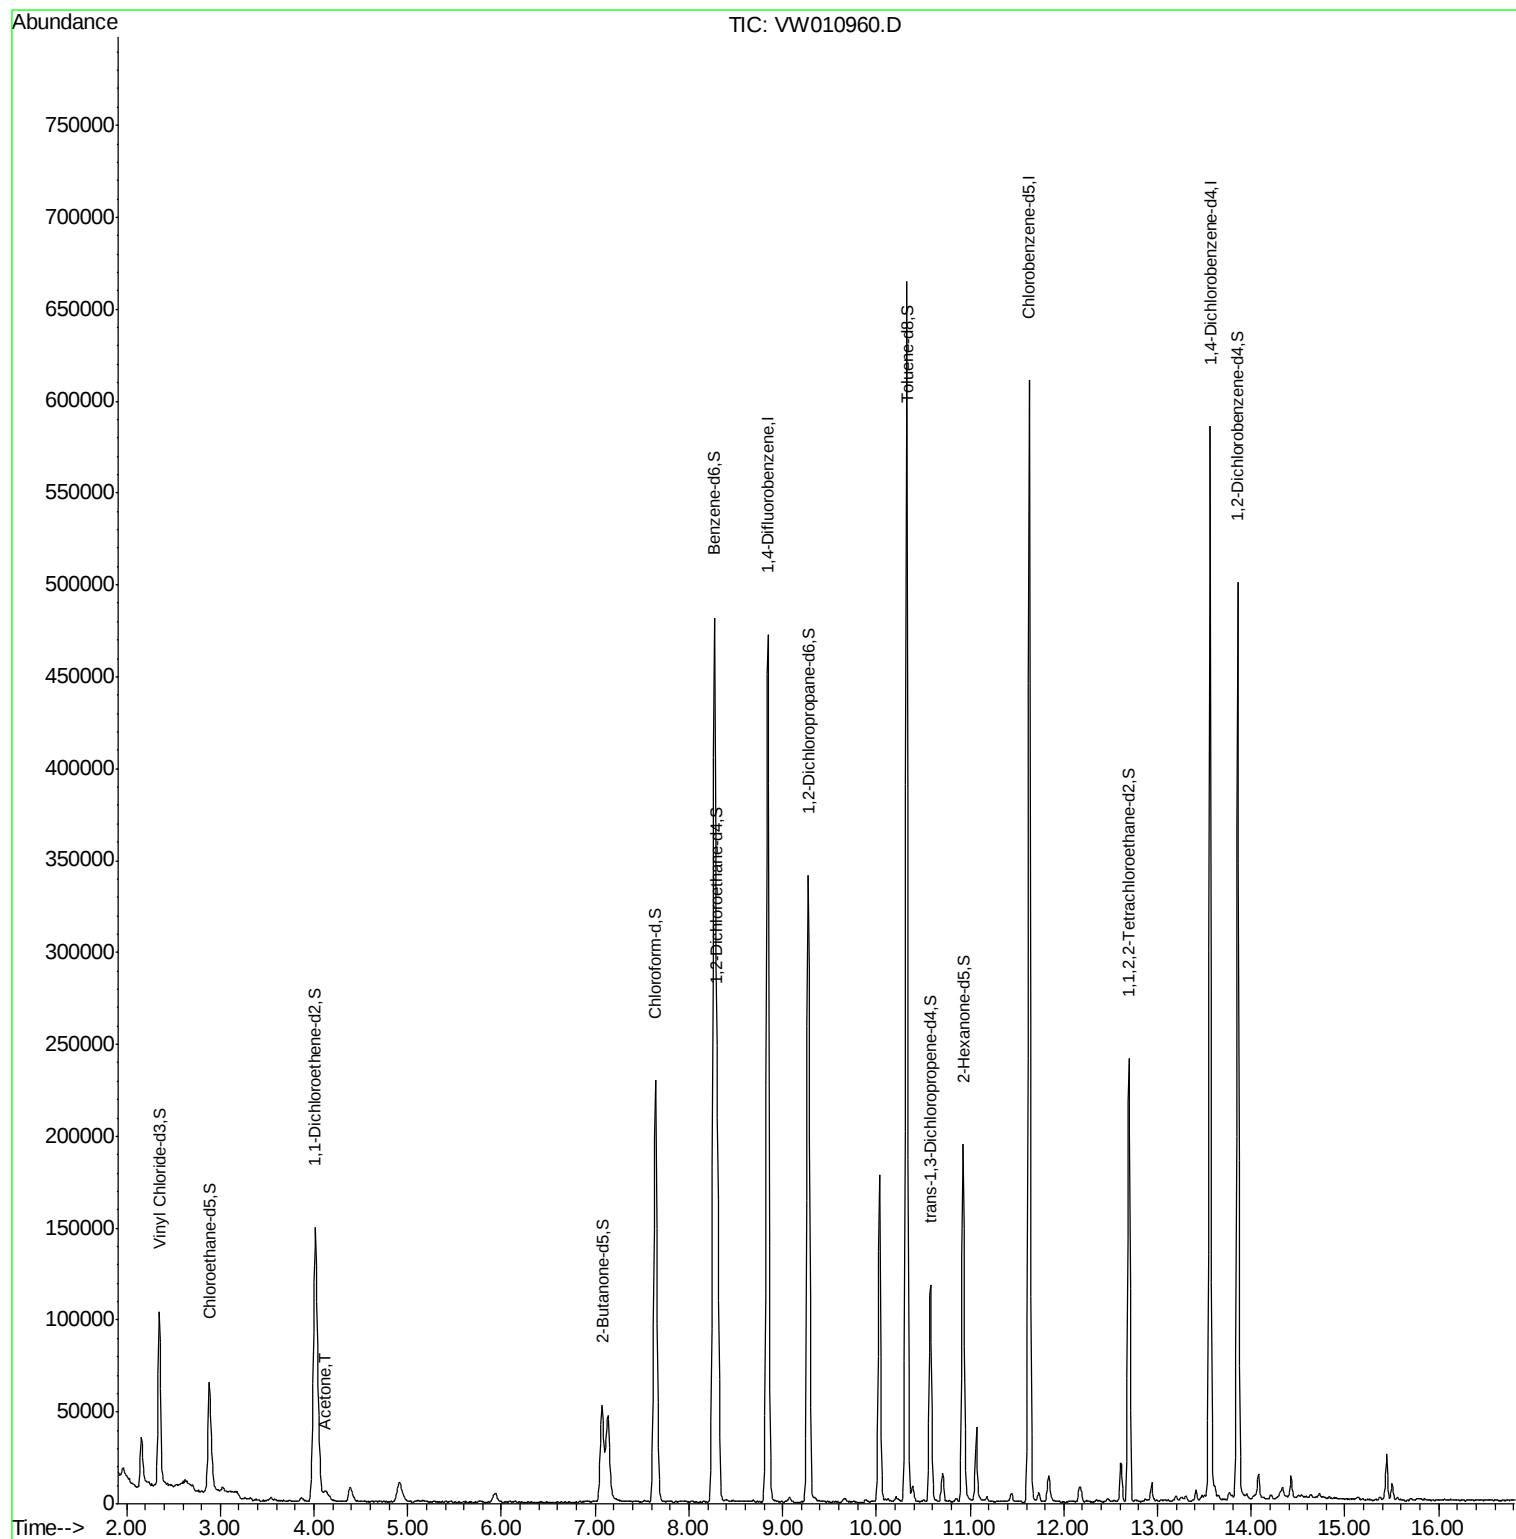

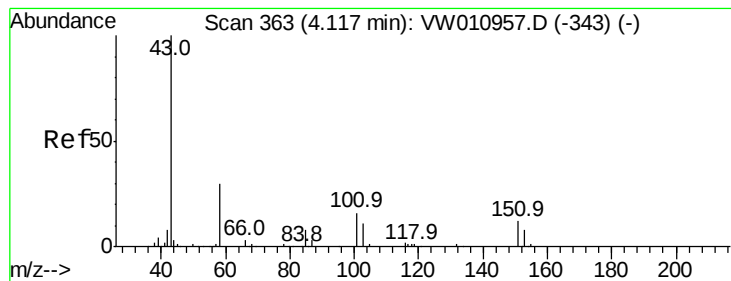

#13

Acetone

Concen: 4.209 ug/L

RT: 4.12 min Scan# 363

Delta R.T. 0.00 min

Lab File: VW010960.D

Acq: 25 Jun 2019 11:40

Instrument :
MSVOA_W
ClientSampleId :
YANT5

Tot Ion: 43 Resp: 9027

Ion Ratio Lower Upper

43 100

58 25.7 0.0 53.2

