

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062519\
 Data File : VW010965.D
 Acq On : 25 Jun 2019 13:54
 Operator : SY/VA
 Sample : K3456-07
 Misc : 2.78G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANX7

Quant Time: Jun 26 04:10:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 26 02:56:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	344622	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	309146	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	145088	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	102437	22.93	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.72%
7) Chloroethane-d5	2.89	69	75481	21.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	87.68%
10) 1,1-Dichloroethene-d2	4.01	63	176782	16.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	67.00%
20) 2-Butanone-d5	7.07	46	89379	42.61	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.22%
24) Chloroform-d	7.65	84	223447	24.04	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	96.16%
26) 1,2-Dichloroethane-d4	8.31	65	138996	24.13	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.52%
29) Benzene-d6	8.27	84	461931	24.89	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.56%
33) 1,2-Dichloropropane-d6	9.27	67	153533	25.03	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.12%
37) Toluene-d8	10.32	98	415910	24.83	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.32%
38) trans-1,3-Dichloropropene-	10.58	79	57508	21.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.76%
39) 2-Hexanone-d5	10.93	63	60376	43.81	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.62%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	114122	22.58	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	138735	25.33	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.32%


Target Compounds					Ovalue
13) Acetone	4.13	43	3777	1.880 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062519\
Data File : VW010965.D
Acq On : 25 Jun 2019 13:54
Operator : SY/VA
Sample : K3456-07
Misc : 2.78G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANX7

Quant Time: Jun 26 04:10:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 02:56:20 2019
Response via : Initial Calibration

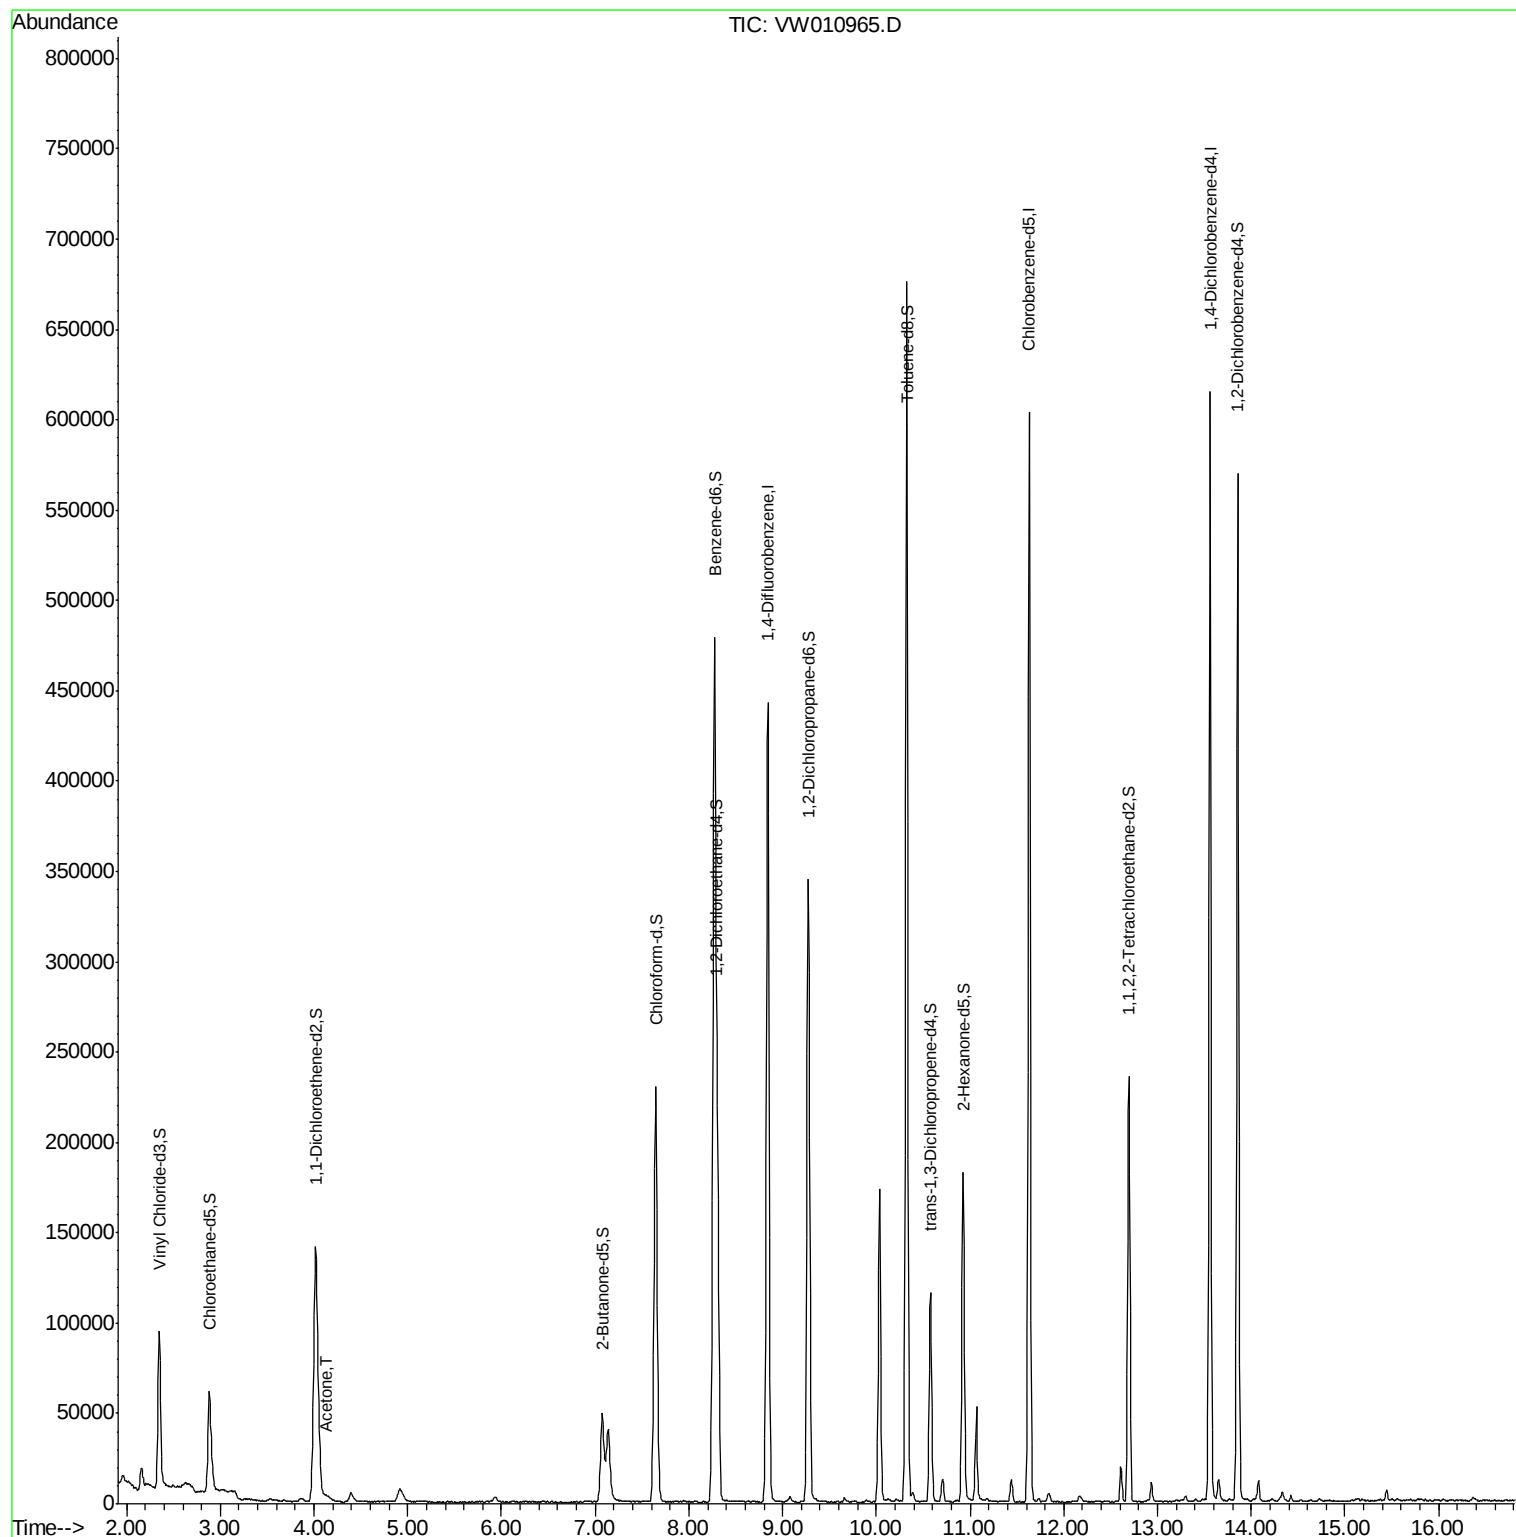

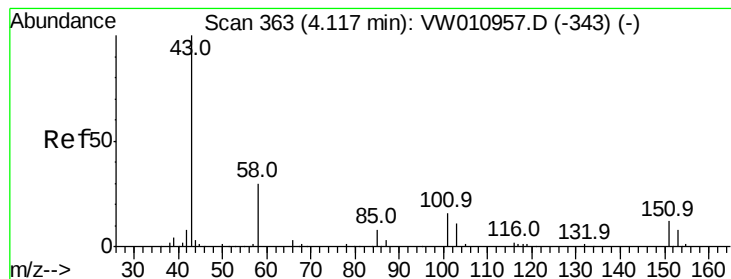

#13

Acetone

Concen: 1.880 ug/L

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW010965.D

Acq: 25 Jun 2019 13:54

Instrument :
MSVOA_W
ClientSampleId :
YANX7

Tot Ion: 43 Resp: 3777

Ion Ratio Lower Upper

43 100

58 18.3 0.0 53.2

