

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062519\
 Data File : VW010967.D
 Acq On : 25 Jun 2019 14:49
 Operator : SY/VA
 Sample : K3456-12
 Misc : 3.44G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANT6

Quant Time: Jun 26 04:17:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 26 02:56:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	349805	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	313456	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	146460	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	100986	22.27	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.08%
7) Chloroethane-d5	2.89	69	74834	21.41	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.64%
10) 1,1-Dichloroethene-d2	4.02	63	174189	16.25	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.00%
20) 2-Butanone-d5	7.08	46	95735	44.96	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.92%
24) Chloroform-d	7.65	84	221713	23.50	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	8.31	65	143541	24.55	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.20%
29) Benzene-d6	8.27	84	459752	24.43	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	97.72%
33) 1,2-Dichloropropane-d6	9.27	67	155188	24.96	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.84%
37) Toluene-d8	10.32	98	416353	24.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.08%
38) trans-1,3-Dichloropropene-	10.58	79	58144	21.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	84.52%
39) 2-Hexanone-d5	10.93	63	64308	46.02	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	119872	23.39	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.56%
61) 1,2-Dichlorobenzene-d4	13.86	152	141916	25.67	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.68%


Target Compounds					Ovalue
13) Acetone	4.12	43	3775	1.851 ug/L	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062519\
Data File : VW010967.D
Acq On : 25 Jun 2019 14:49
Operator : SY/VA
Sample : K3456-12
Misc : 3.44G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANT6

Quant Time: Jun 26 04:17:07 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 02:56:20 2019
Response via : Initial Calibration

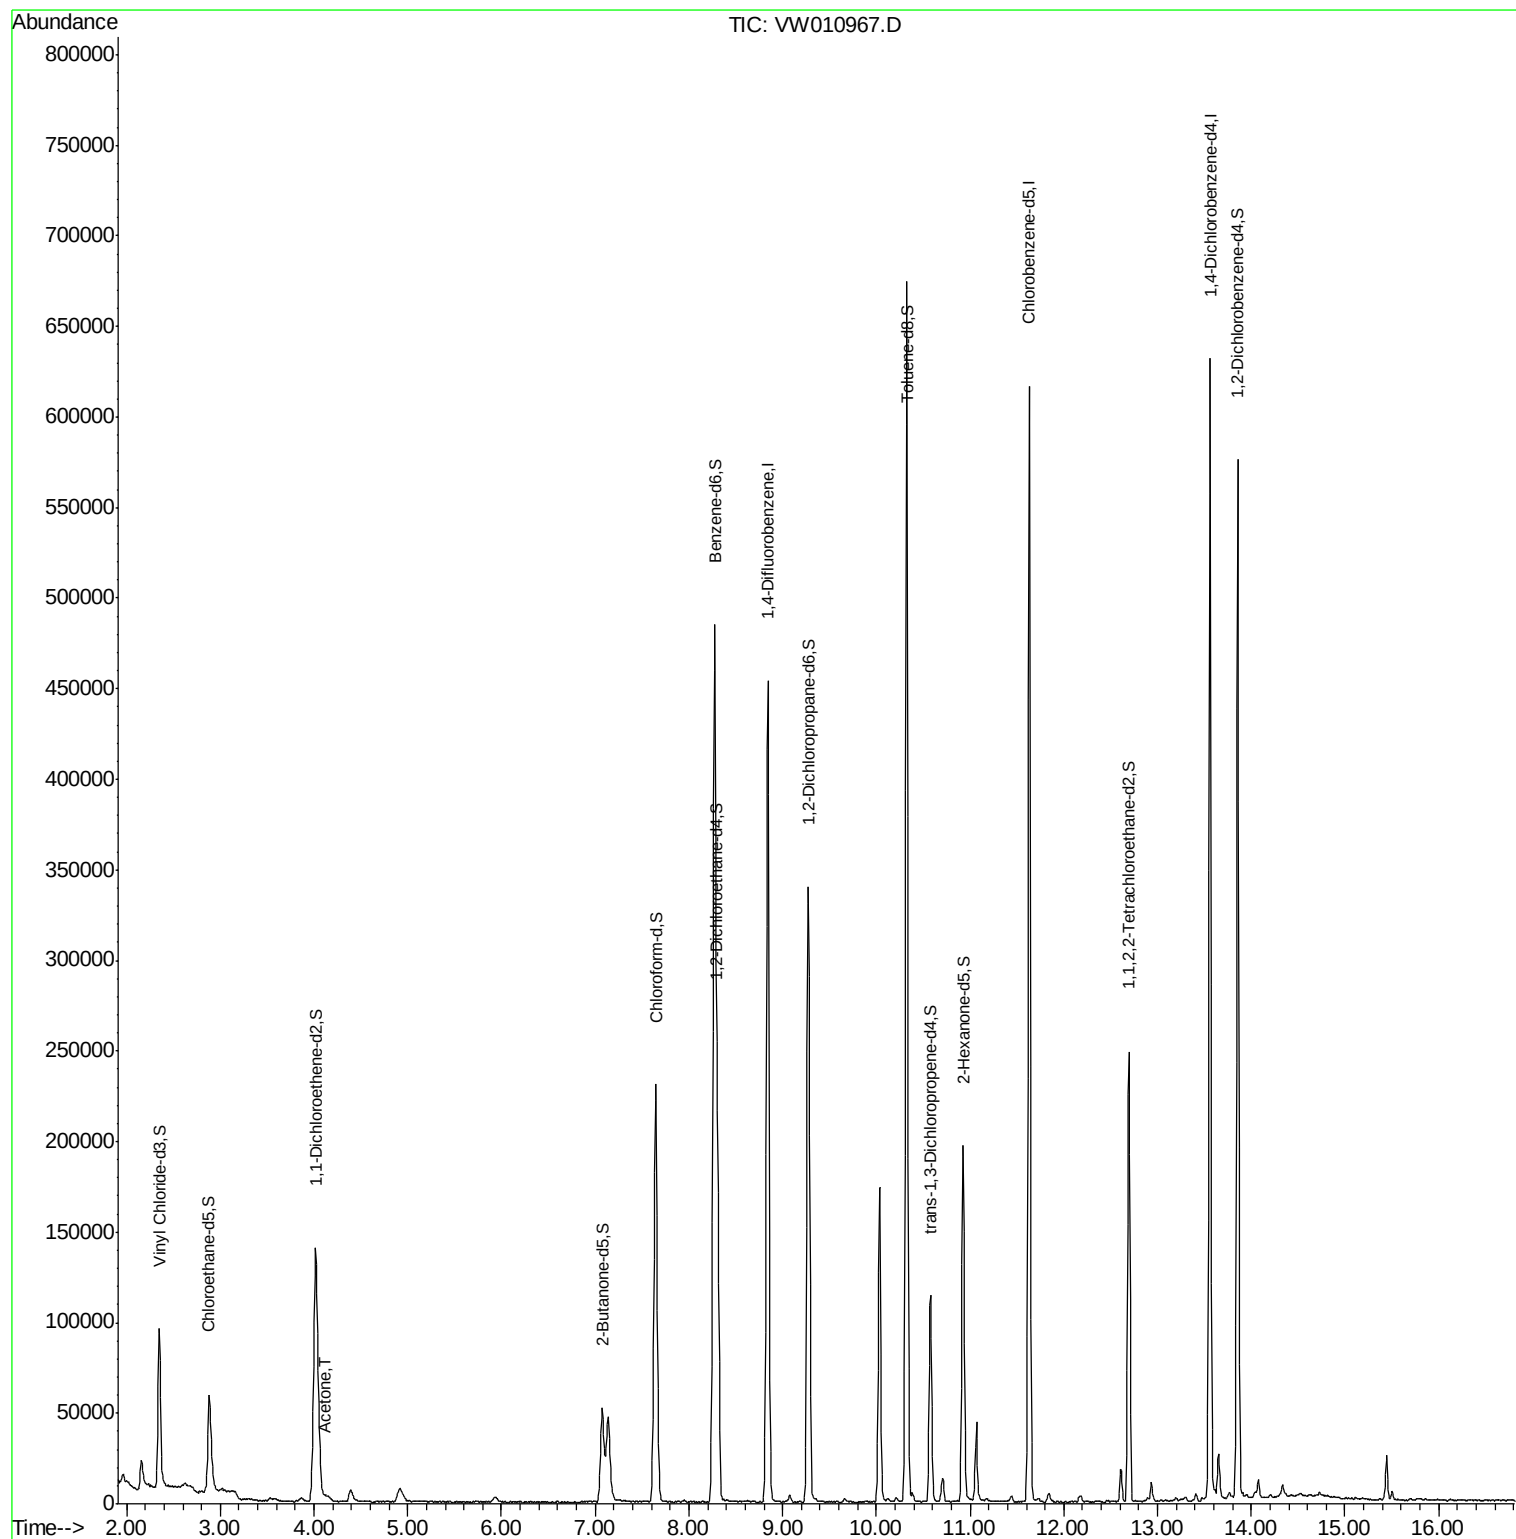

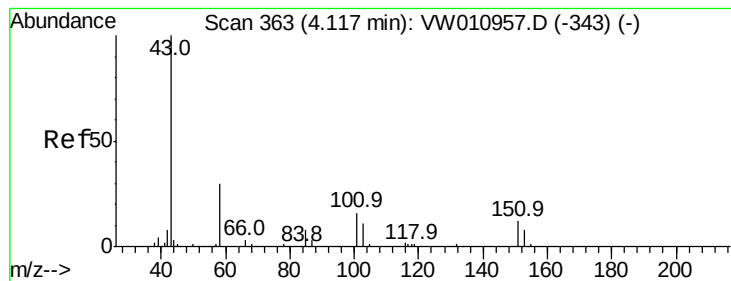

#13

Acetone

Concen: 1.851 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW010967.D

Acq: 25 Jun 2019 14:49

Instrument :
MSVOA_W
ClientSampleId :
YANT6

Tot Ion: 43 Resp: 3775

Ion Ratio Lower Upper

43 100

58 9.2 0.0 53.2

