

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062519\
 Data File : VW010977.D
 Acq On : 25 Jun 2019 19:54
 Operator : SY/VA
 Sample : K3460-05
 Misc : 4.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANT9

Quant Time: Jun 26 05:15:20 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 26 04:33:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	296660	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	268692	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	115659	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	80661	20.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.92%
7) Chloroethane-d5	2.89	69	59341	20.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.08%
10) 1,1-Dichloroethene-d2	4.02	63	138426	15.23	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	60.92%
20) 2-Butanone-d5	7.07	46	95261	52.75	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.50%
24) Chloroform-d	7.65	84	178496	22.31	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.24%
26) 1,2-Dichloroethane-d4	8.30	65	120871	24.37	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.48%
29) Benzene-d6	8.27	84	367051	22.75	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.00%
33) 1,2-Dichloropropane-d6	9.27	67	126290	23.69	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.76%
37) Toluene-d8	10.32	98	323032	22.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.76%
38) trans-1,3-Dichloropropene-	10.58	79	46835	19.85	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.40%
39) 2-Hexanone-d5	10.92	63	65379	54.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	110886	25.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.96%
61) 1,2-Dichlorobenzene-d4	13.85	152	104652	23.97	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.88%


Target Compounds					Ovalue
13) Acetone	4.12	43	3939	2.278 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062519\
Data File : VW010977.D
Acq On : 25 Jun 2019 19:54
Operator : SY/VA
Sample : K3460-05
Misc : 4.09G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANT9

Quant Time: Jun 26 05:15:20 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 04:33:18 2019
Response via : Initial Calibration

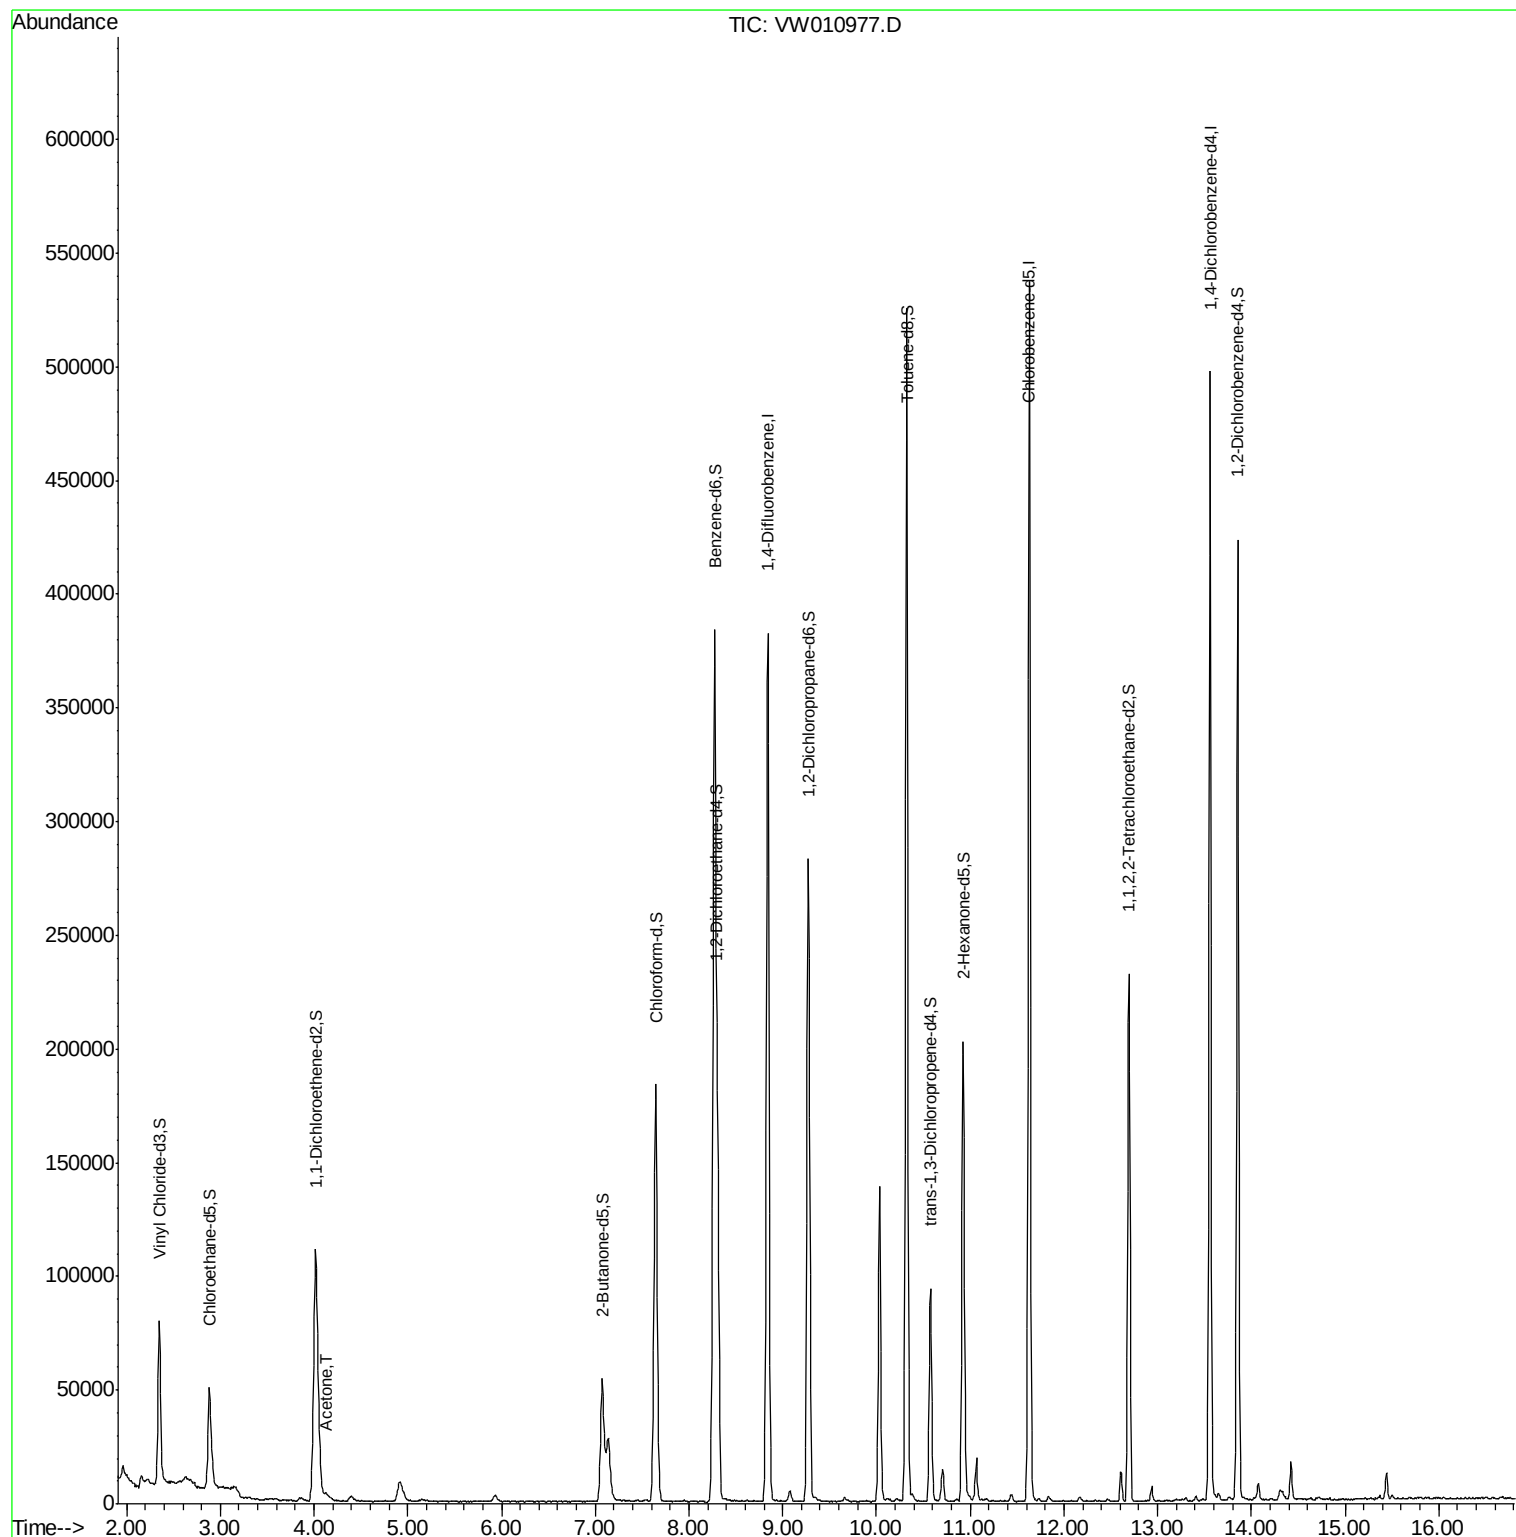

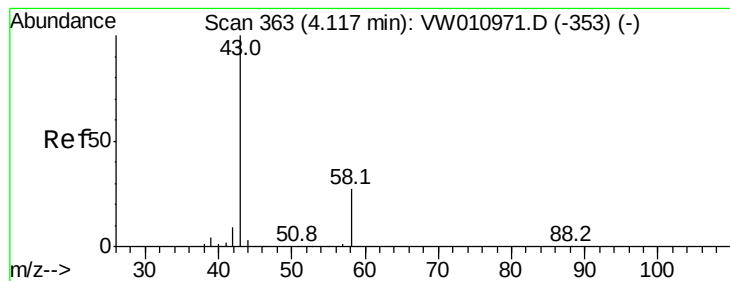

#13

Acetone

Concen: 2.278 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW010977.D

Acq: 25 Jun 2019 19:54

Instrument :
MSVOA_W
ClientSampleId :
YANT9

Tot Ion: 43 Resp: 3939

Ion Ratio Lower Upper

43 100

58 27.4 0.0 53.2

