

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062519\
 Data File : VW010978.D
 Acq On : 25 Jun 2019 20:21
 Operator : SY/VA
 Sample : K3460-06
 Misc : 3.89G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANWO

Quant Time: Jun 26 05:17:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Jun 26 04:33:18 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	319912	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	297280	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	140548	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	88557	21.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.44%
7) Chloroethane-d5	2.88	69	65938	20.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.52%
10) 1,1-Dichloroethene-d2	4.01	63	151206	15.43	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.72%
20) 2-Butanone-d5	7.07	46	107365	55.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.26%
24) Chloroform-d	7.65	84	204997	23.76	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.04%
26) 1,2-Dichloroethane-d4	8.30	65	142246	26.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.40%
29) Benzene-d6	8.27	84	423041	23.70	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.80%
33) 1,2-Dichloropropane-d6	9.27	67	147161	24.95	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.80%
37) Toluene-d8	10.32	98	372211	23.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.44%
38) trans-1,3-Dichloropropene-	10.58	79	56364	21.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.40%
39) 2-Hexanone-d5	10.92	63	73429	55.40	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.80%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	128057	26.34	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.36%
61) 1,2-Dichlorobenzene-d4	13.85	152	138891	26.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	104.72%


Target Compounds					Ovalue
13) Acetone	4.13	43	3183	1.707 ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062519\
Data File : VW010978.D
Acq On : 25 Jun 2019 20:21
Operator : SY/VA
Sample : K3460-06
Misc : 3.89G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANW0

Quant Time: Jun 26 05:17:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Wed Jun 26 04:33:18 2019
Response via : Initial Calibration

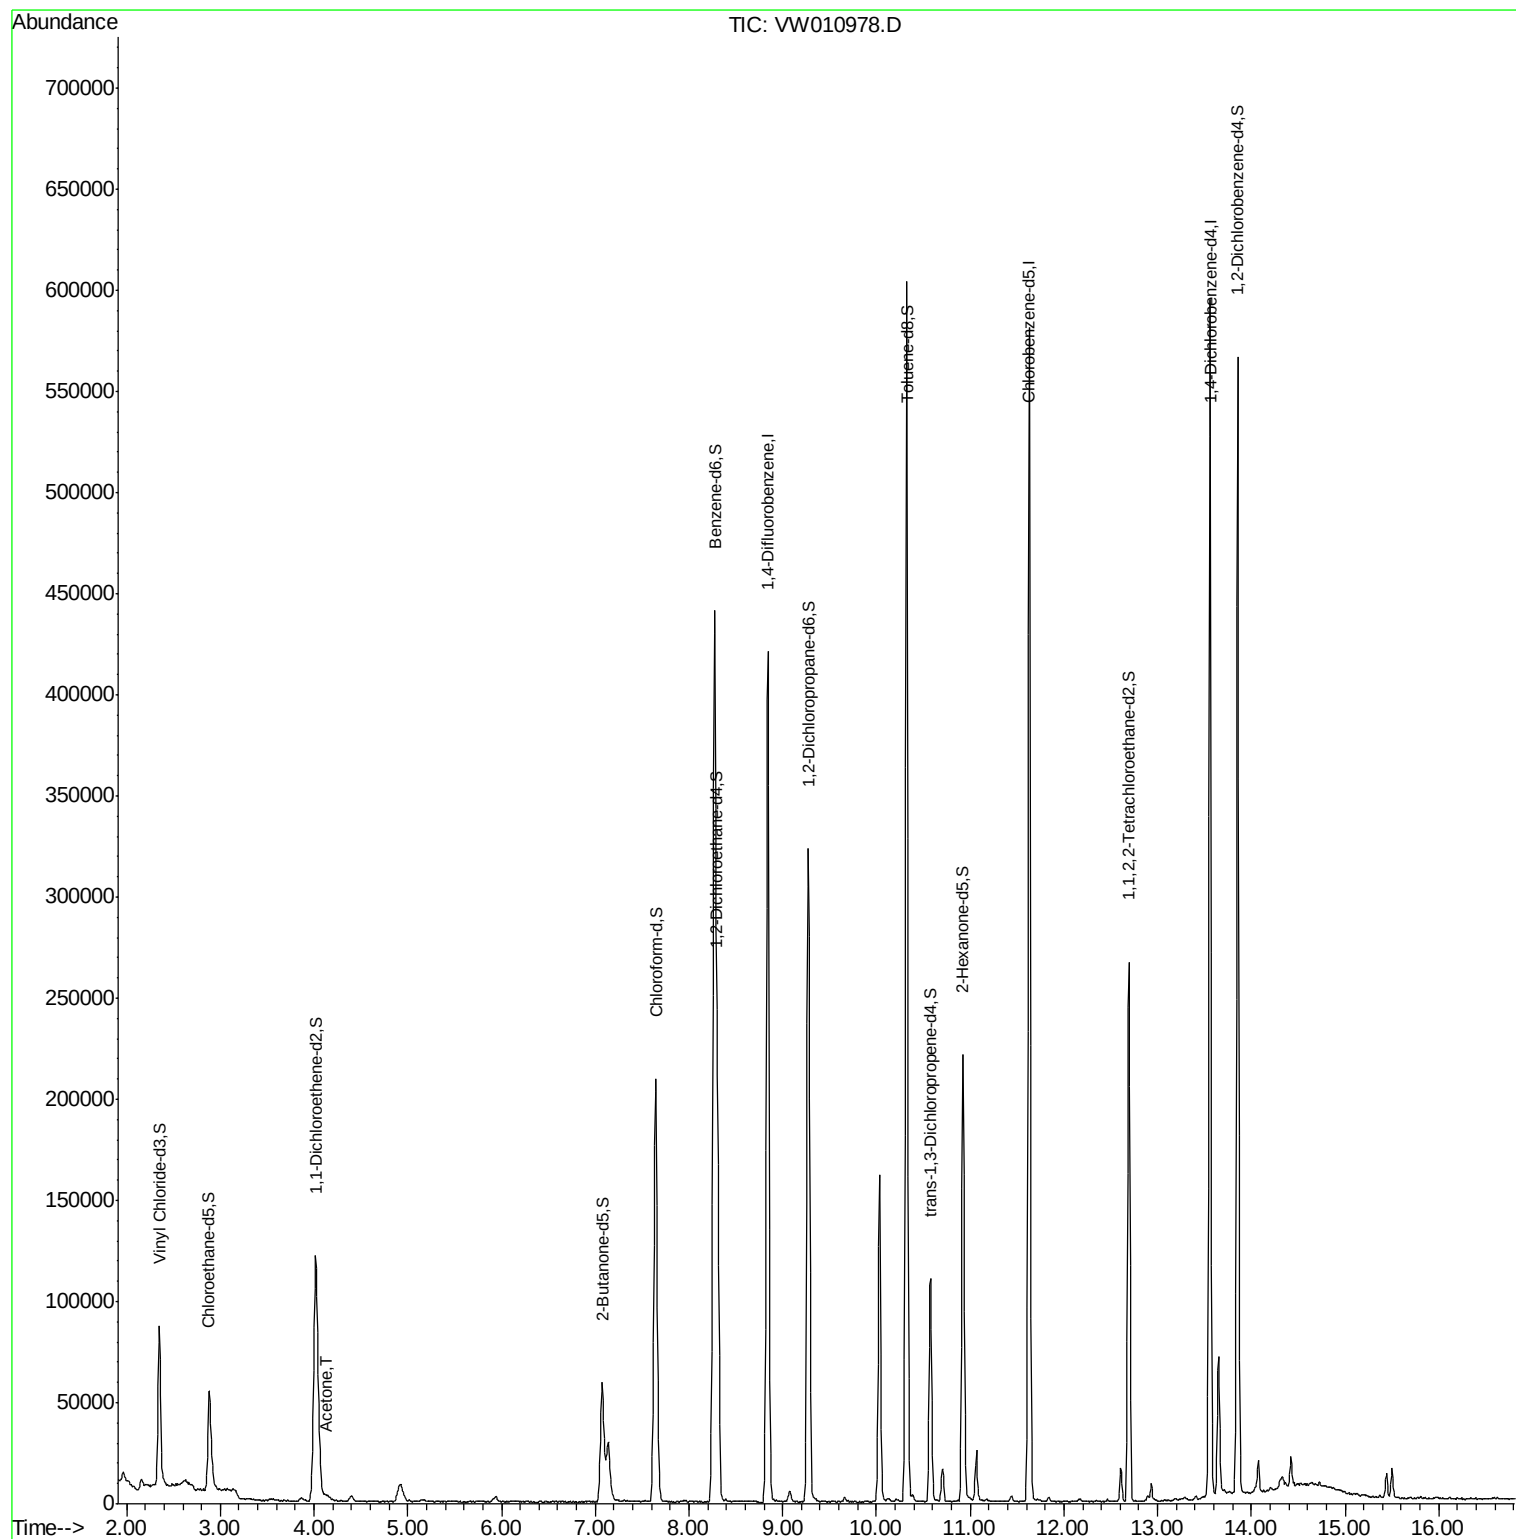

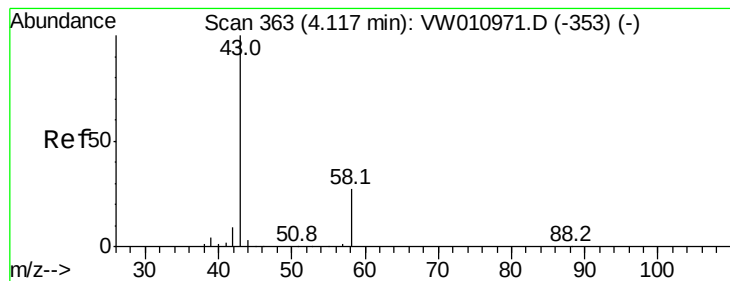

#13

Acetone

Concen: 1.707 ug/L

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW010978.D

Acq: 25 Jun 2019 20:21

Instrument :
MSVOA_W
ClientSampleId :
YANW0

Tot Ion: 43 Resp: 3183

Ion Ratio Lower Upper

43 100

58 28.9 0.0 53.2

