


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062618\
 Data File : VW003567.D
 Acq On : 26 Jun 2018 09:05
 Operator : SY/AP
 Sample : BFB90
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB90

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Title : VOC Analysis
 Last Update : Wed Jun 27 01:37:29 2018

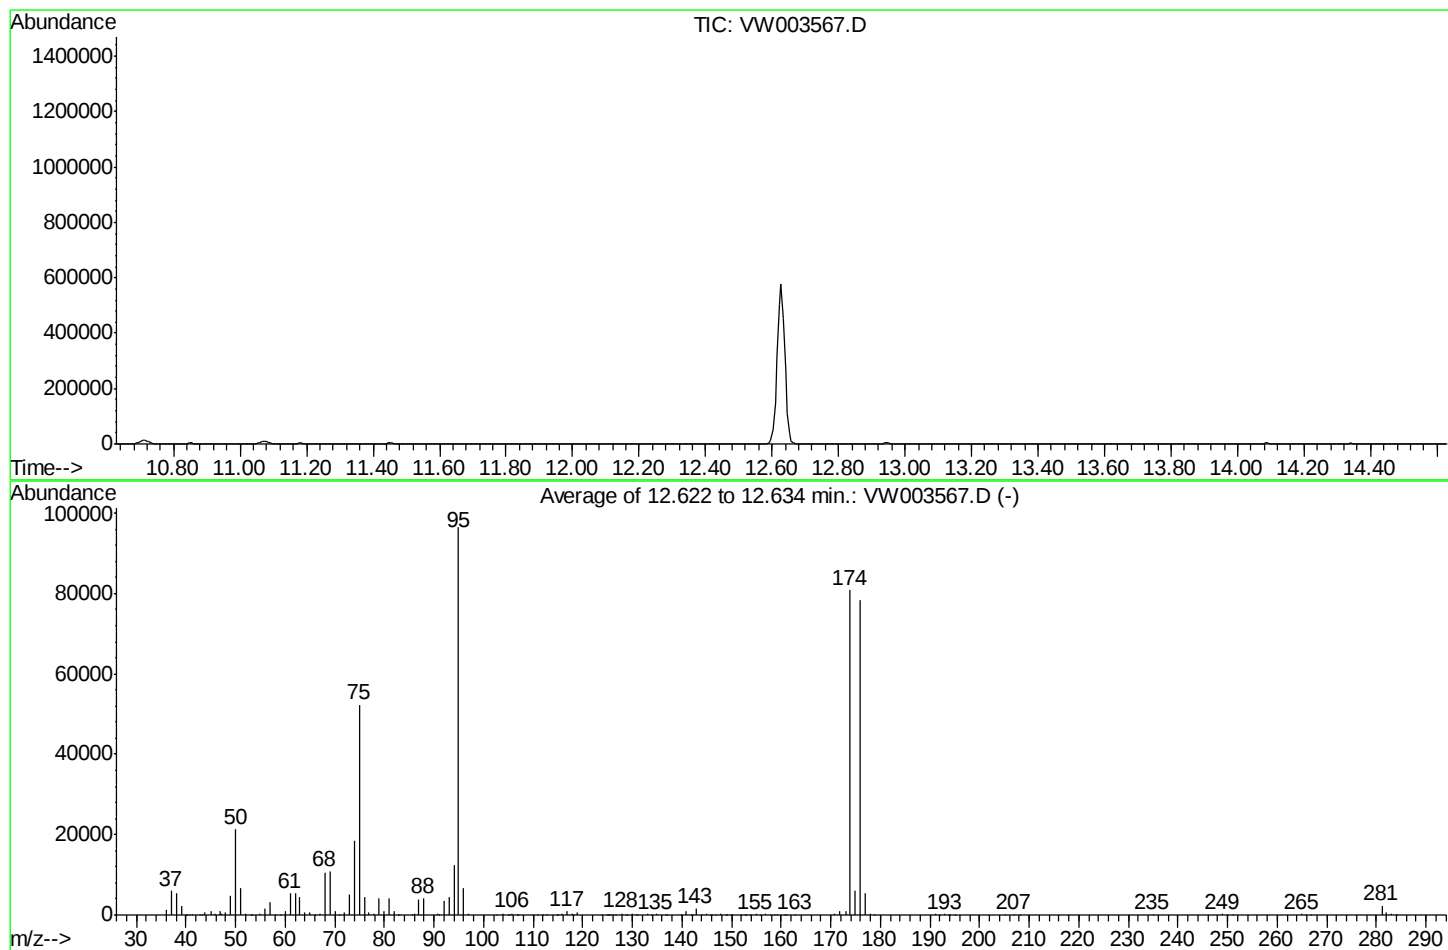

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	21248	PASS
75	95	30	80	54.3	52378	PASS
95	95	100	100	100.0	96485	PASS
96	95	5	9	6.8	6545	PASS
173	174	0.00	2	1.1	892	PASS
174	95	50	120	83.8	80853	PASS
175	174	5	9	7.6	6126	PASS
176	174	95	101	96.8	78290	PASS
177	176	5	9	7.0	5446	PASS

Scan 1802 (12.573 min): VW003567.D
BFB90

m/z	Abundance
39.10	75.0
39.90	111.0
43.90	190.0
207.00	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

m/z	Abundance
36.00	1131.0
37.00	6191.0
38.00	5349.0
39.00	2358.0
39.90	186.0
40.80	85.0
41.20	77.0
43.00	57.0
43.90	968.0
45.00	1178.0
46.00	172.0
46.90	1287.0
48.00	624.0
49.00	4810.0
50.00	22600.0
51.00	7038.0
52.10	319.0
53.30	151.0
54.90	311.0
55.90	1910.0
57.00	3425.0
58.00	136.0
59.00	93.0
60.00	1066.0
61.00	5714.0
62.00	5490.0
63.00	4722.0
63.90	711.0
64.90	657.0
65.90	137.0
67.10	315.0
68.00	10997.0
69.00	11339.0
70.00	961.0
72.00	532.0
73.00	4966.0
74.00	18832.0
75.00	52848.0
76.00	4619.0
76.90	484.0
77.90	487.0
78.90	4081.0
80.00	1200.0
80.90	4267.0
81.90	906.0
83.00	99.0
85.90	203.0
87.00	3544.0
87.90	3909.0
90.80	541.0
92.00	3349.0
93.00	4453.0
94.00	12770.0
95.00	95472.0
96.00	6858.0
97.00	266.0
102.70	123.0
103.80	392.0
104.80	216.0
105.90	438.0
106.80	150.0
109.70	103.0
110.80	148.0
111.90	87.0
112.70	87.0
114.70	83.0
115.80	370.0
116.90	773.0
117.80	441.0
118.90	751.0
124.90	125.0
125.70	116.0
126.10	86.0
126.60	70.0
127.80	385.0
128.70	176.0
129.90	334.0
131.00	169.0
133.10	348.0
133.70	112.0
134.80	236.0
136.80	120.0
139.80	65.0
140.90	1051.0
141.90	239.0
142.90	1433.0
143.90	117.0
144.90	437.0
145.70	132.0
146.10	86.0
146.80	153.0
147.80	210.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

148.80	58.0
149.80	60.0
153.80	52.0
155.00	234.0
156.80	222.0
158.80	96.0
160.70	82.0
162.80	104.0
170.80	245.0
171.90	1024.0
173.00	1312.0
173.90	74072.0
175.00	5457.0
175.90	71720.0
176.90	4931.0
178.00	212.0
178.80	209.0
191.00	197.0
191.90	74.0
192.90	423.0
193.80	72.0
194.10	63.0
195.00	86.0
205.10	72.0
207.00	314.0
208.10	109.0
234.90	54.0
249.00	190.0
249.90	58.0
250.90	125.0
265.00	288.0
265.70	76.0
266.80	127.0
281.10	2527.0
282.00	702.0
282.90	606.0
283.90	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

m/z	Abundance
36.00	1463.0
37.00	6758.0
38.00	6097.0
39.10	2459.0
39.90	279.0
41.20	63.0
42.80	112.0
44.00	931.0
45.00	1401.0
45.80	185.0
46.10	171.0
46.90	1500.0
47.90	717.0
49.00	5216.0
50.00	24040.0
51.00	7582.0
52.00	264.0
53.00	121.0
55.00	385.0
56.00	1885.0
57.00	3638.0
58.10	161.0
60.00	1062.0
61.10	6114.0
62.00	5553.0
63.00	5099.0
63.90	632.0
65.00	727.0
67.00	346.0
68.00	11760.0
69.00	12384.0
70.00	1002.0
72.00	596.0
73.00	5652.0
74.00	20688.0
75.00	58880.0
76.00	4742.0
77.00	689.0
77.80	477.0
78.90	4585.0
79.90	1242.0
80.90	4637.0
81.90	858.0
83.10	84.0
86.00	201.0
87.00	4504.0
87.90	4848.0
90.80	464.0
92.00	3742.0
93.00	4877.0
94.00	13874.0
95.00	110416.0
96.00	7183.0
97.00	204.0
102.70	114.0
103.90	535.0
104.90	202.0
105.80	518.0
107.00	133.0
109.80	112.0
110.90	162.0
111.80	142.0
112.80	83.0
114.90	153.0
115.90	453.0
116.90	1069.0
117.80	355.0
118.90	889.0
124.00	75.0
125.00	122.0
125.60	126.0
126.10	55.0
126.70	63.0
127.80	513.0
128.90	135.0
130.00	480.0
130.70	163.0
132.90	237.0
133.80	132.0
134.90	310.0
137.00	255.0
139.80	100.0
140.90	1085.0
141.80	201.0
142.90	1749.0
143.80	187.0
144.90	432.0
145.70	206.0
146.80	106.0
147.70	374.0
149.00	87.0
150.10	60.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

151.90	96.0
152.80	68.0
153.80	50.0
154.90	392.0
156.80	214.0
158.00	84.0
158.70	134.0
159.20	74.0
161.00	121.0
170.80	252.0
171.90	1038.0
172.90	1365.0
173.90	90440.0
174.90	7199.0
175.90	88144.0
176.90	6309.0
177.90	321.0
191.10	191.0
193.00	236.0
205.10	51.0
206.90	175.0
208.10	69.0
234.90	64.0
248.90	239.0
251.00	86.0
265.10	234.0
266.90	54.0
281.10	2877.0
282.00	589.0
283.00	469.0
284.10	79.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

m/z	Abundance
36.00	993.0
37.00	5122.0
38.00	4509.0
39.00	1980.0
39.90	154.0
40.10	154.0
41.20	86.0
43.20	67.0
44.00	773.0
45.00	782.0
46.00	165.0
47.10	1028.0
47.90	518.0
49.00	4317.0
50.00	17104.0
51.00	5643.0
52.00	263.0
53.00	118.0
54.90	290.0
56.00	1395.0
57.00	2422.0
57.90	88.0
60.00	944.0
61.00	4294.0
62.00	4900.0
63.00	3523.0
63.90	693.0
65.00	522.0
66.90	209.0
68.00	9200.0
69.00	9092.0
70.00	885.0
70.90	62.0
72.10	508.0
73.00	4343.0
74.00	15863.0
75.00	45408.0
76.00	3980.0
77.00	463.0
77.90	287.0
78.90	3363.0
79.90	794.0
80.90	3292.0
81.90	728.0
82.80	126.0
85.70	146.0
86.10	129.0
87.00	3690.0
87.90	3481.0
91.00	504.0
91.90	2996.0
93.00	4297.0
94.00	10682.0
95.00	83568.0
96.00	5595.0
97.10	177.0
102.70	74.0
103.80	346.0
105.10	122.0
105.90	333.0
106.90	94.0
109.80	75.0
110.80	85.0
112.00	84.0
112.70	101.0
115.00	102.0
115.80	285.0
116.90	704.0
118.00	278.0
118.90	680.0
123.80	79.0
124.70	91.0
125.30	86.0
125.80	61.0
126.80	57.0
127.80	347.0
128.90	216.0
130.00	346.0
131.00	163.0
133.00	232.0
133.70	72.0
134.90	261.0
136.90	211.0
139.60	56.0
140.90	1119.0
142.10	164.0
142.80	1195.0
144.90	375.0
145.90	131.0
146.80	59.0
147.80	189.0
150.10	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90

151.90	76.0
152.80	55.0
153.00	54.0
153.80	141.0
155.00	253.0
155.80	143.0
156.80	137.0
157.90	78.0
158.70	144.0
161.00	174.0
170.90	109.0
171.80	701.0
173.90	78048.0
174.90	5723.0
175.90	75008.0
176.90	5100.0
178.00	225.0
191.10	146.0
191.90	71.0
193.00	246.0
195.00	80.0
207.10	190.0
248.90	234.0
251.00	65.0
264.90	180.0
266.90	65.0
281.00	1508.0
282.00	401.0
283.00	302.0

Instrument :
MSVOA_W
ClientSampleId :
BFB90