

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062619\
 Data File : VW010996.D
 Acq On : 26 Jun 2019 11:28
 Operator : SY/VA
 Sample : K3497-07
 Misc : 5.03G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Quant Time: Jun 27 07:56:59 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 27 07:30:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	355407	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	322274	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	153336	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	117144	25.43	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.72%
7) Chloroethane-d5	2.88	69	83954	23.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.56%
10) 1,1-Dichloroethene-d2	4.02	63	194955	17.91	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.64%
20) 2-Butanone-d5	7.07	46	126982	58.70	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.40%
24) Chloroform-d	7.65	84	233207	24.33	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.32%
26) 1,2-Dichloroethane-d4	8.31	65	153804	25.89	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.56%
29) Benzene-d6	8.27	84	489105	25.28	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.12%
33) 1,2-Dichloropropane-d6	9.27	67	160270	25.07	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.28%
37) Toluene-d8	10.32	98	432494	24.77	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.08%
38) trans-1,3-Dichloropropene-	10.58	79	63174	22.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.32%
39) 2-Hexanone-d5	10.93	63	79092	55.05	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.10%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	141330	26.82	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.28%
61) 1,2-Dichlorobenzene-d4	13.86	152	149178	25.77	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.08%


Target Compounds					Ovalue
13) Acetone	4.12	43	9527	4.599 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062619\
Data File : VW010996.D
Acq On : 26 Jun 2019 11:28
Operator : SY/VA
Sample : K3497-07
Misc : 5.03G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Jun 27 07:56:59 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 27 07:30:59 2019
Response via : Initial Calibration

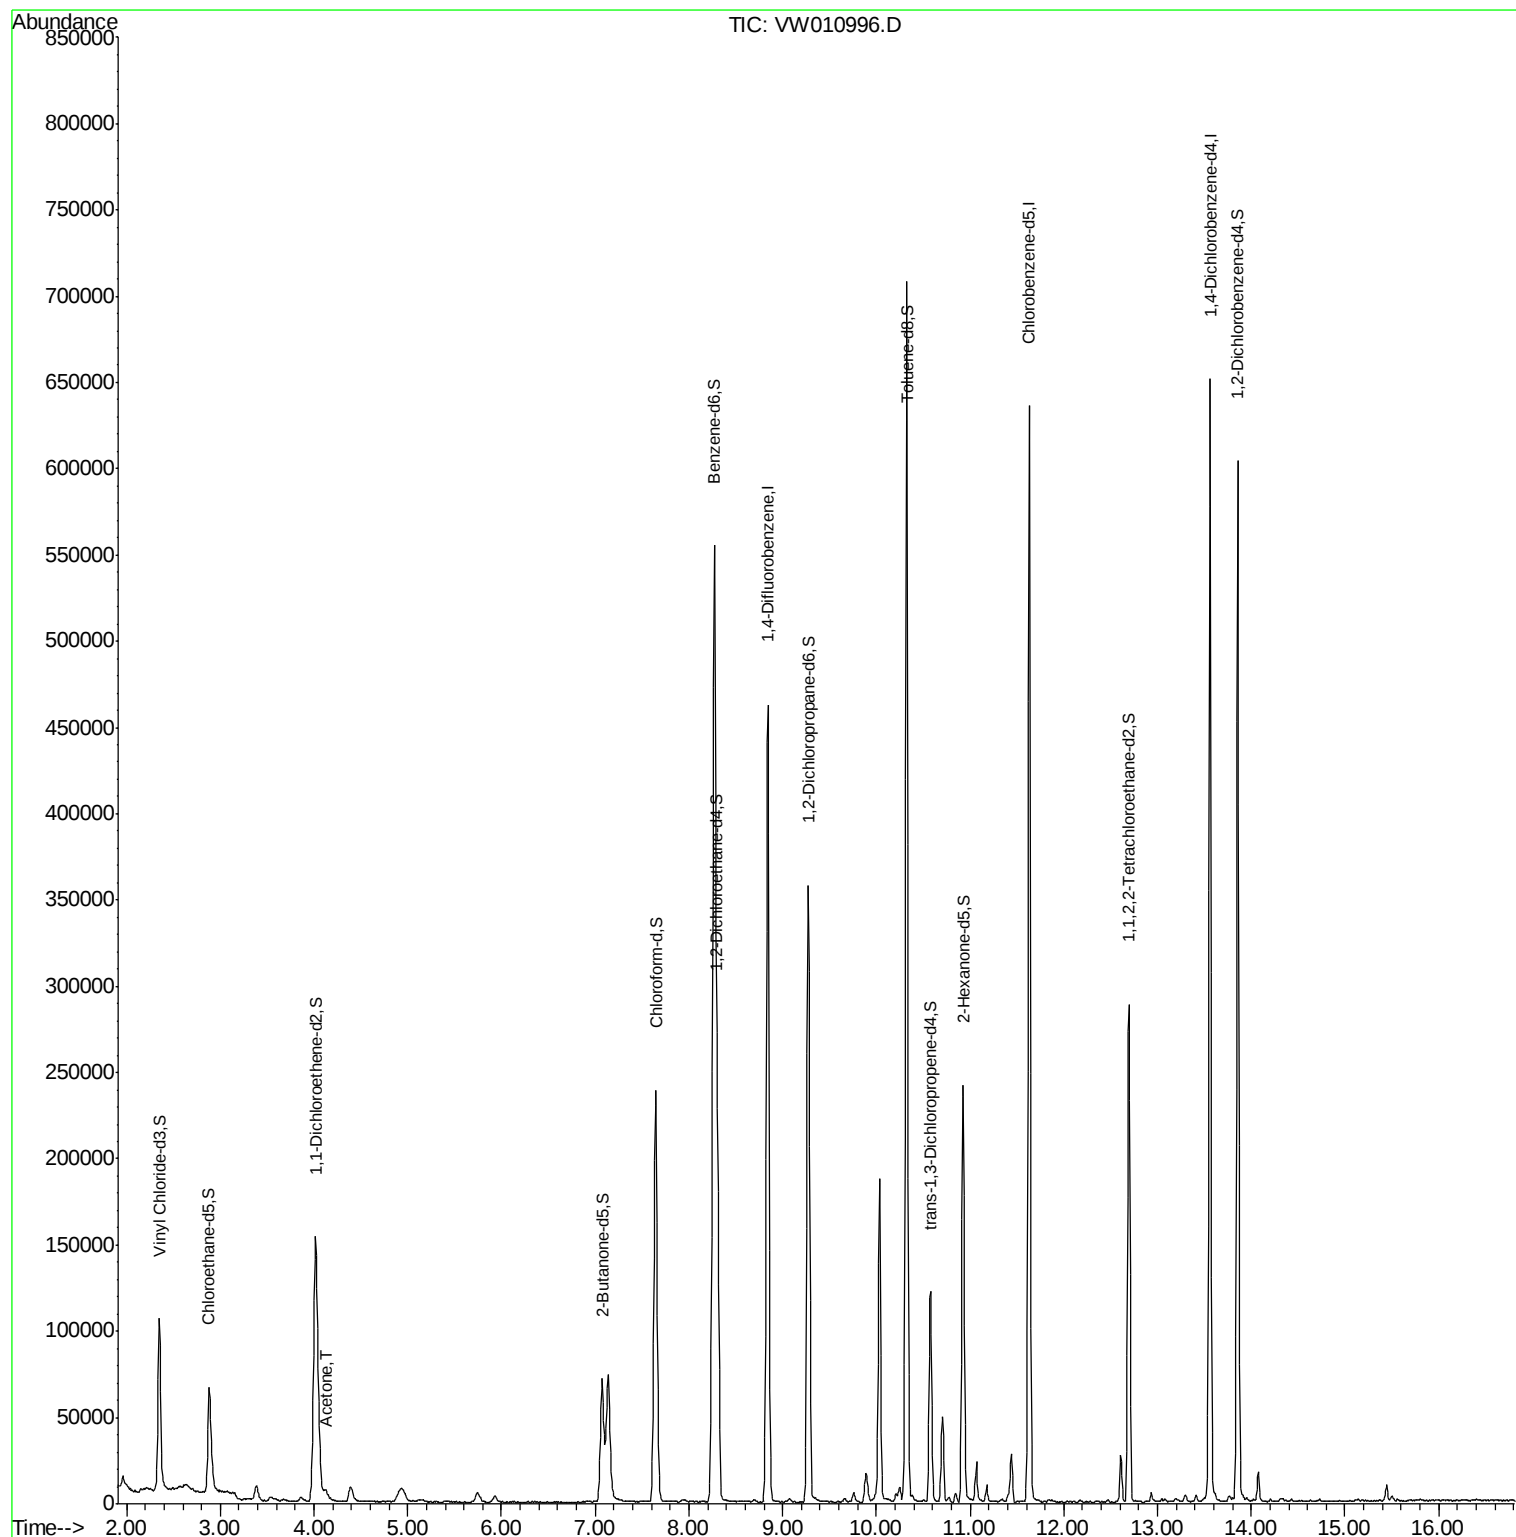

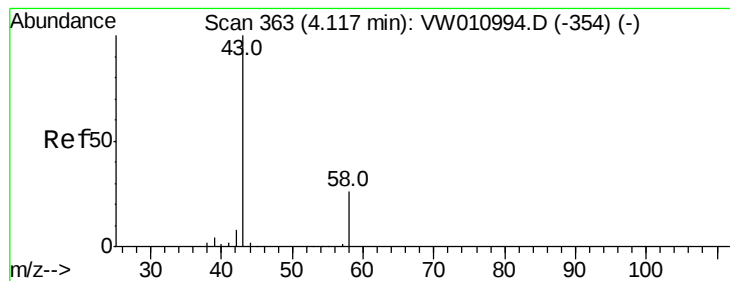

#13

Acetone

Concen: 4.599 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW010996.D

Acq: 26 Jun 2019 11:28

Instrument :

MSVOA_W

ClientSampleId :

VHBLK01

Tot Ion: 43 Resp: 9527

Ion Ratio Lower Upper

43 100

58 28.1 0.0 53.2

