

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062619\
 Data File : VW011008.D
 Acq On : 26 Jun 2019 16:53
 Operator : SY/VA
 Sample : K3461-02
 Misc : 5.70G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YANZ1

Quant Time: Jun 27 08:38:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 27 07:30:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	283487	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	246986	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	100808	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	84588	23.02	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.08%
7) Chloroethane-d5	2.88	69	63209	22.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.24%
10) 1,1-Dichloroethene-d2	4.01	63	144262	16.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.44%
20) 2-Butanone-d5	7.07	46	115671	67.03	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	134.06%
24) Chloroform-d	7.65	84	192919	25.23	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.92%
26) 1,2-Dichloroethane-d4	8.31	65	133441	28.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	112.64%
29) Benzene-d6	8.27	84	389726	26.28	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	105.12%
33) 1,2-Dichloropropane-d6	9.27	67	136537	27.87	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.48%
37) Toluene-d8	10.32	98	335011	25.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.16%
38) trans-1,3-Dichloropropene-	10.58	79	50913	23.48	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.92%
39) 2-Hexanone-d5	10.93	63	75465	68.53	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.06%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	122300	30.28	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.12%#
61) 1,2-Dichlorobenzene-d4	13.85	152	102360	26.90	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	107.60%


Target Compounds				Ovalue
13) Acetone	4.12	43	7758	4.695 ug/L 98
16) Methylene chloride	4.92	84	11253	2.680 ug/L 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062619\
Data File : VW011008.D
Acq On : 26 Jun 2019 16:53
Operator : SY/VA
Sample : K3461-02
Misc : 5.70G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YANZ1

Quant Time: Jun 27 08:38:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062419S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 27 07:30:59 2019
Response via : Initial Calibration

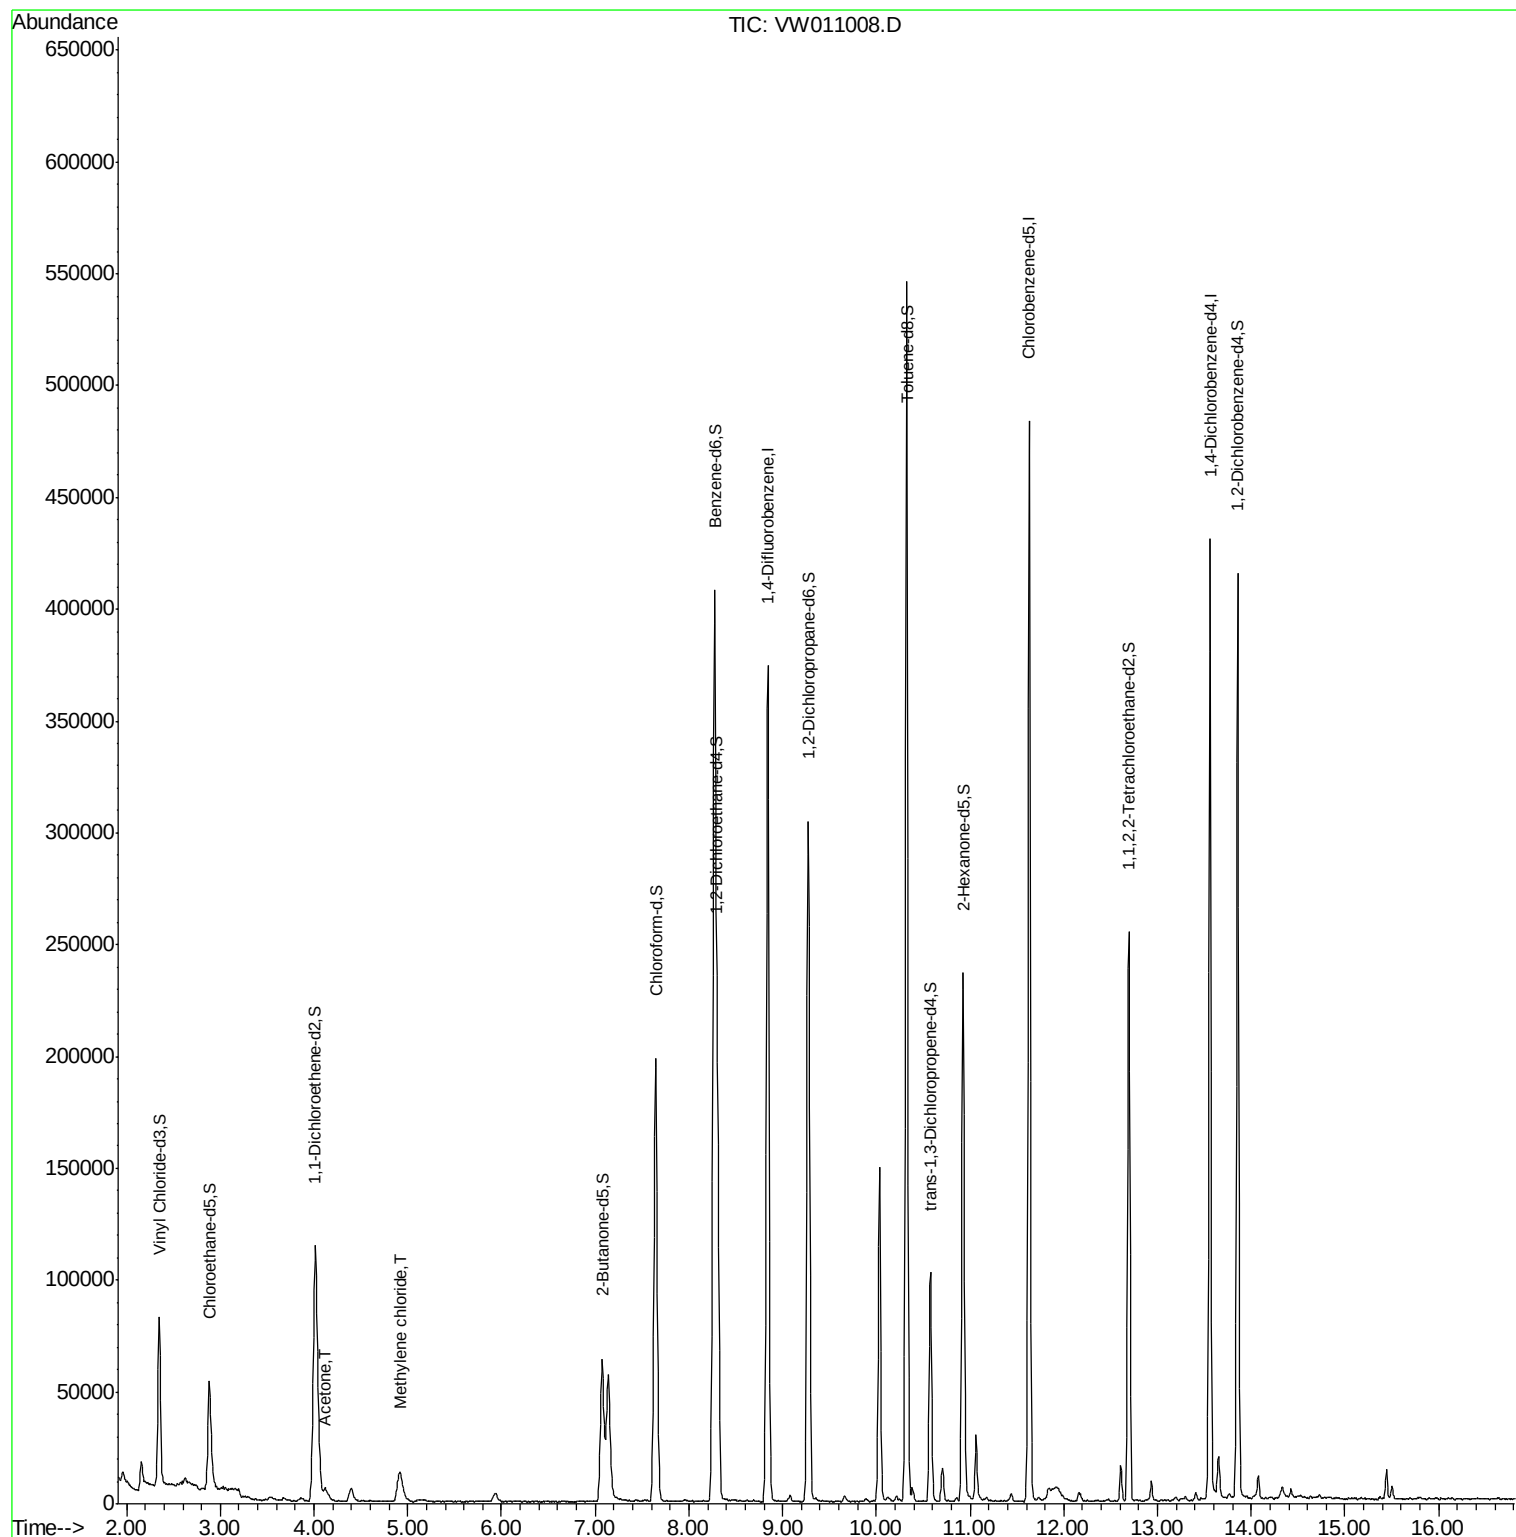

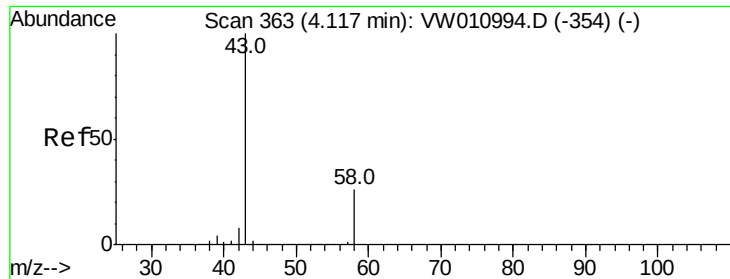

#13

Acetone

Concen: 4.695 ug/L

RT: 4.12 min Scan# 363

Delta R.T. 0.00 min

Lab File: VW011008.D

Acq: 26 Jun 2019 16:53





Instrument :
MSVOA_W
ClientSampled :
YANZ1

Tot Ion: 43 Resp: 7758

Ion Ratio Lower Upper

43 100

58 27.6 0.0 53.2

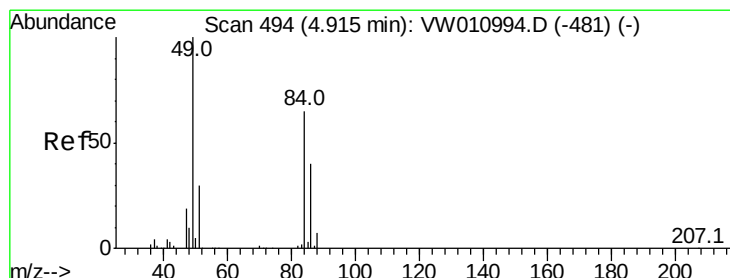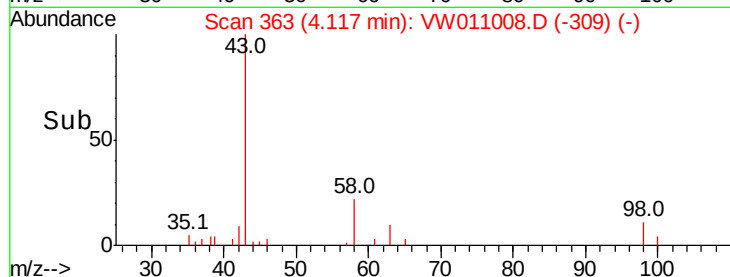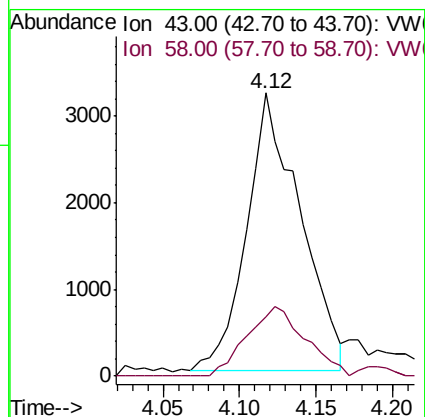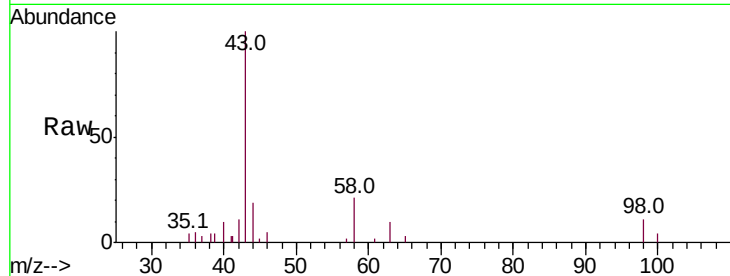

#16

Methylene chloride

Concen: 2.680 ug/L

RT: 4.92 min Scan# 494

Delta R.T. 0.00 min

Lab File: VW011008.D

Acq: 26 Jun 2019 16:53

Tgt Ion: 84 Resp: 11253

Ion Ratio Lower Upper

84 100

49 143.0 107.0 198.8

86 63.8 44.4 82.5

