


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062718\  
 Data File : VW003577.D  
 Acq On : 26 Jun 2018 18:30  
 Operator : SY/AP  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W061318S.M  
 Title : SW846 8260  
 Last Update : Sat Jun 16 05:18:54 2018

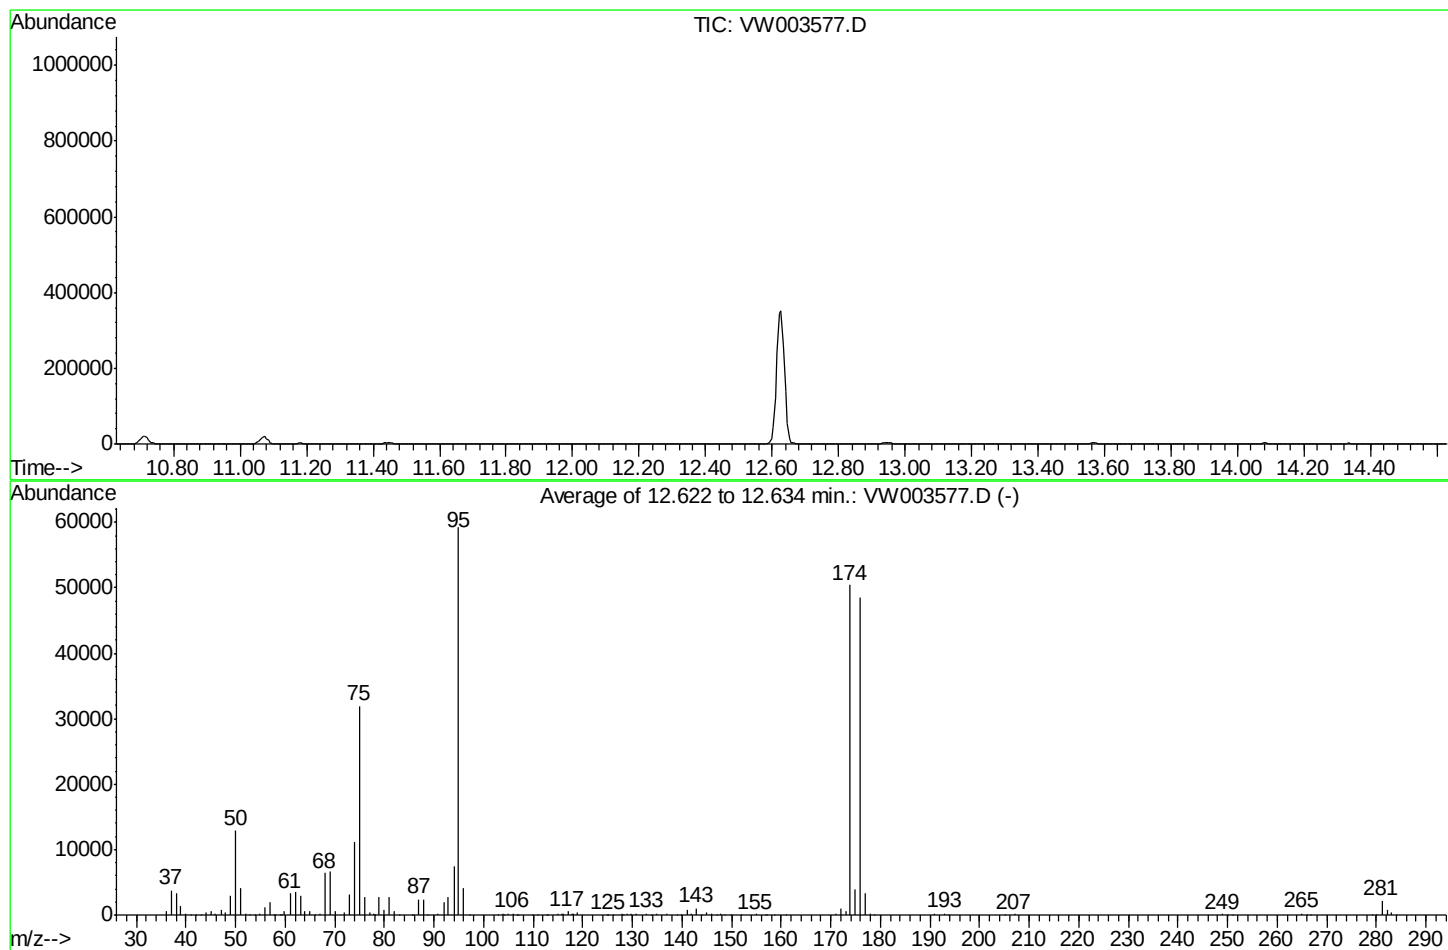

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 21.7      | 12833   | PASS             |
| 75          | 95           | 30           | 60           | 54.0      | 31973   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 59240   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 4031    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.3       | 634     | PASS             |
| 174         | 95           | 50           | 100          | 85.1      | 50386   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 4012    | PASS             |
| 176         | 174          | 95           | 101          | 96.4      | 48581   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 3392    | PASS             |