

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062818\
 Data File : VW003631.D
 Acq On : 28 Jun 2018 11:54
 Operator : SY/AP
 Sample : VW0628SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0628SBL01

Quant Time: Jun 29 06:58:32 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 16 05:18:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	200870	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	332887	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.64	117	303149	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.57	152	147421	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	123270	56.66	ug/l	0.00
Spiked Amount 50.000			Recovery	=	113.32%	
35) Dibromofluoromethane	7.88	113	107549	51.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	103.98%	
50) Toluene-d8	10.33	98	409111	49.88	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.76%	
62) 4-Bromofluorobenzene	12.63	95	136802	47.13	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.26%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062818\
Data File : VW003631.D
Acq On : 28 Jun 2018 11:54
Operator : SY/AP
Sample : VW0628SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0628SBL01

Quant Time: Jun 29 06:58:32 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
Quant Title : SW846 8260
QLast Update : Sat Jun 16 05:18:54 2018
Response via : Initial Calibration

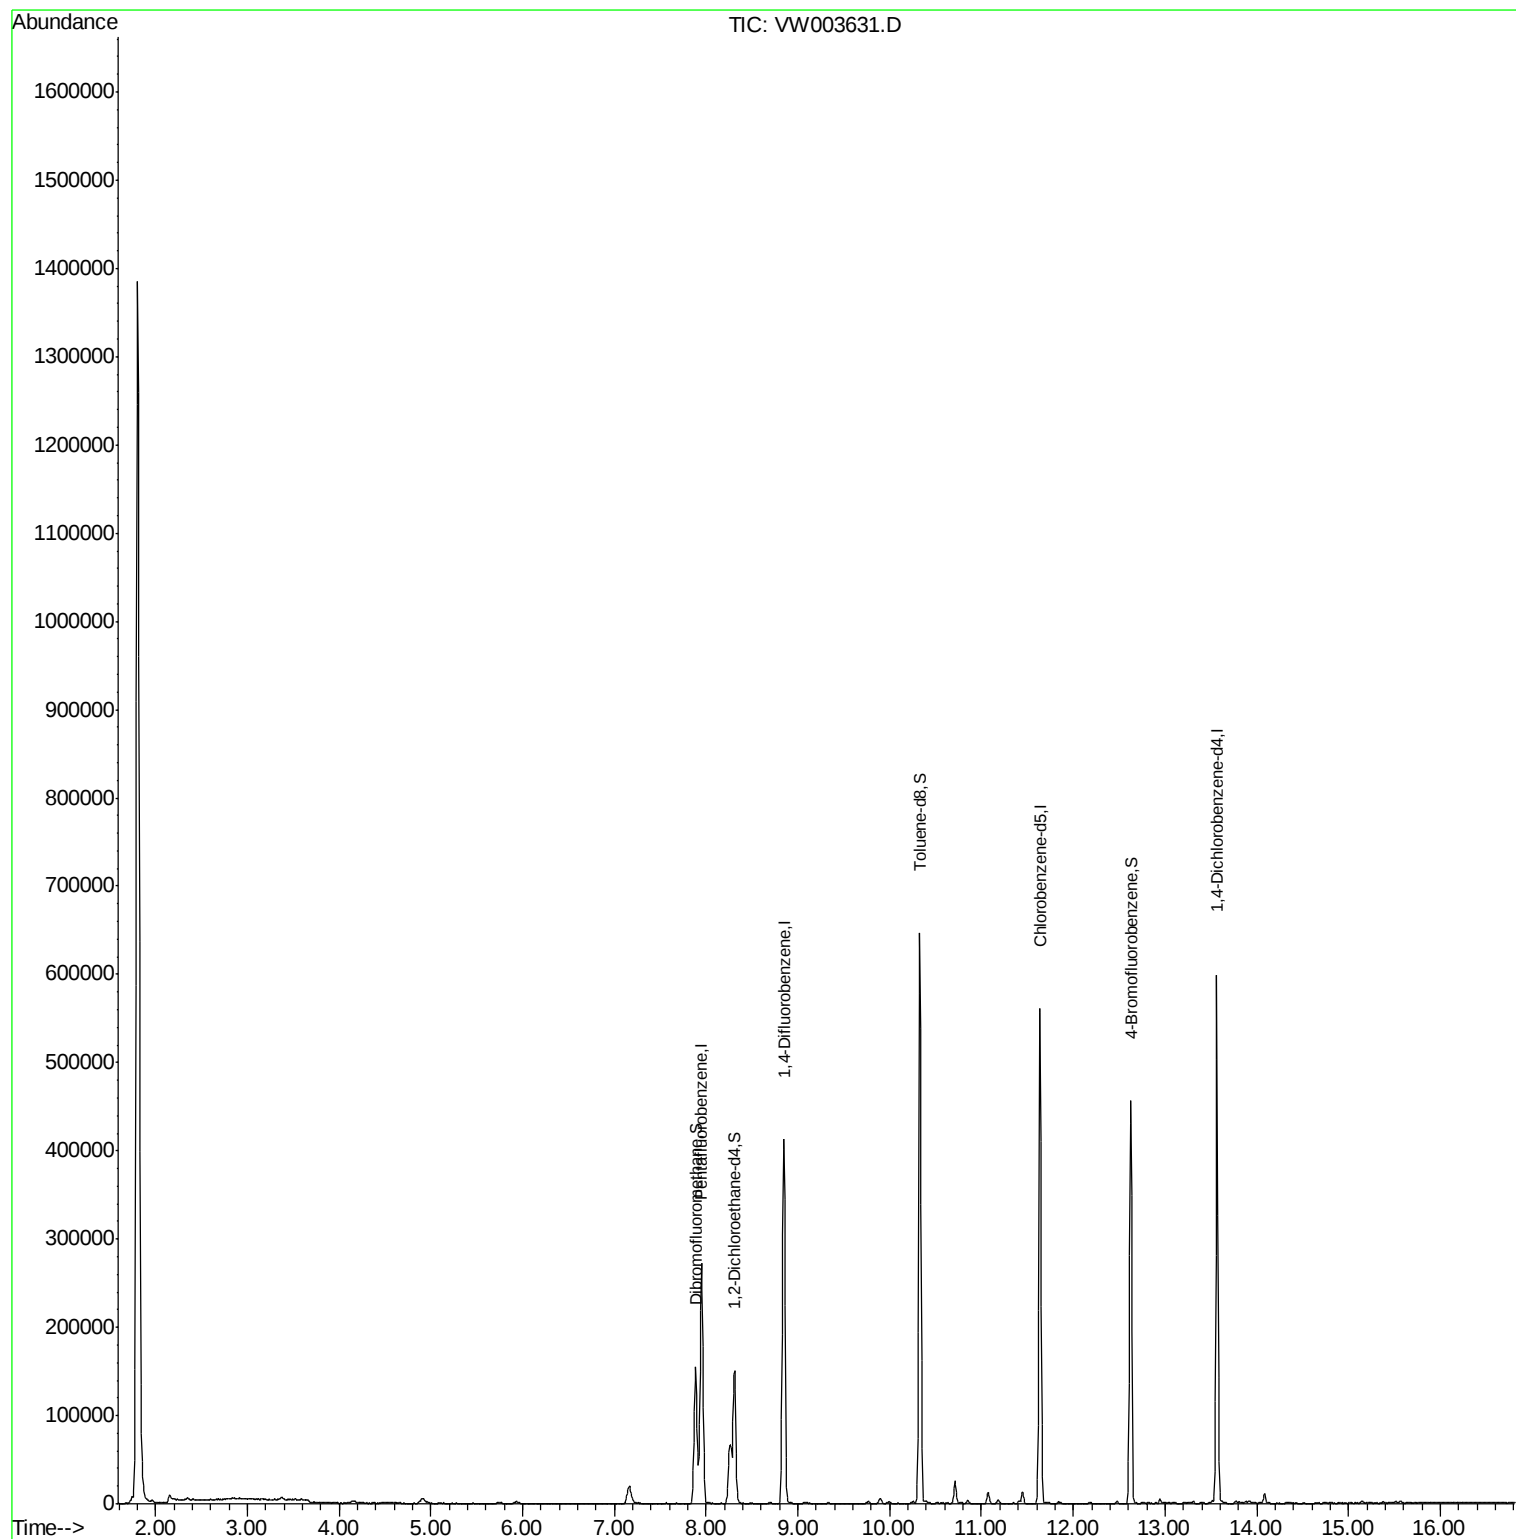

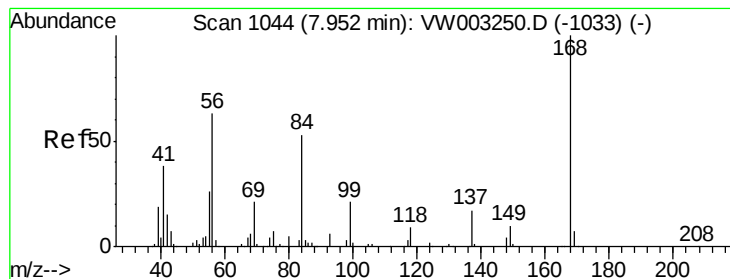

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.95 min Scan# 1044

Delta R.T. -0.00 min

Lab File: VW003631.D

Acq: 28 Jun 2018 11:54

Instrument :

MSVOA_W

ClientSampleId :


VW0628SBL01

Tot Ion:168 Resp: 200870

Ion Ratio Lower Upper

168 100

99 57.5 45.5 68.3

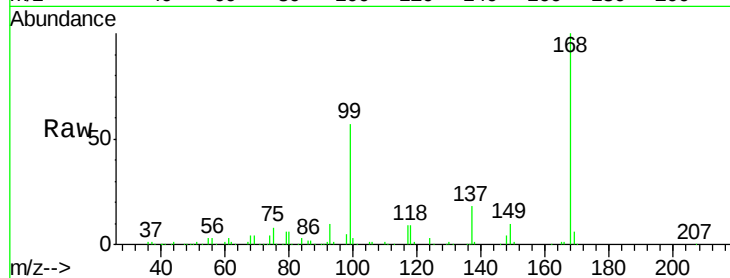

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

80000



60000

40000

20000

0

Time-->

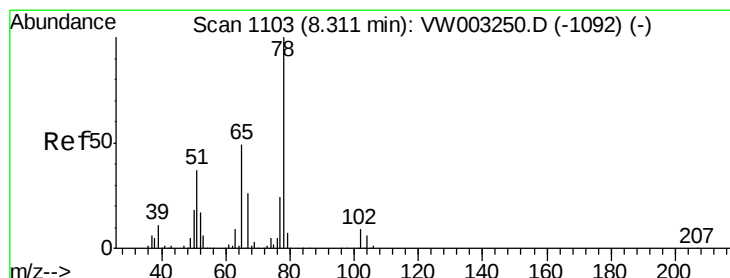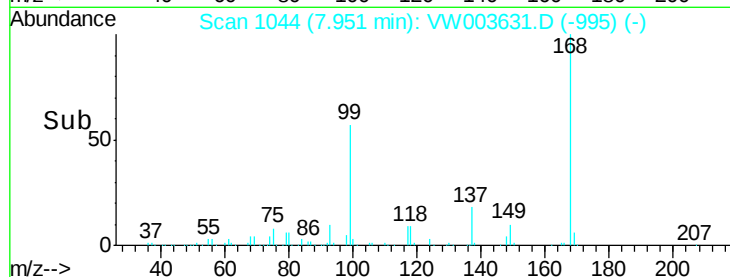

#33

1,2-Dichloroethane-d4

Concen: 56.66 ug/l

RT: 8.31 min Scan# 1103

Delta R.T. -0.00 min

Lab File: VW003631.D


Acq: 28 Jun 2018 11:54

Tgt Ion: 65 Resp: 123270

Ion Ratio Lower Upper

65 100

67 51.0 0.0 104.2

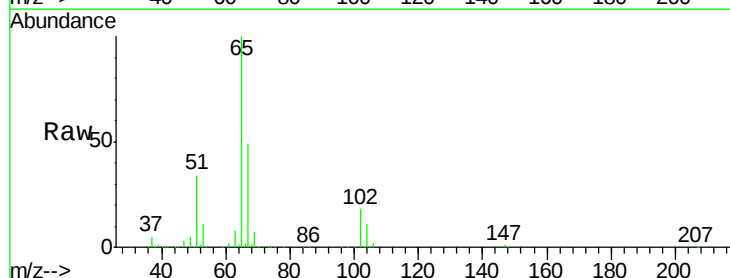

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

60000

50000

40000


30000


20000

10000

0

Time-->

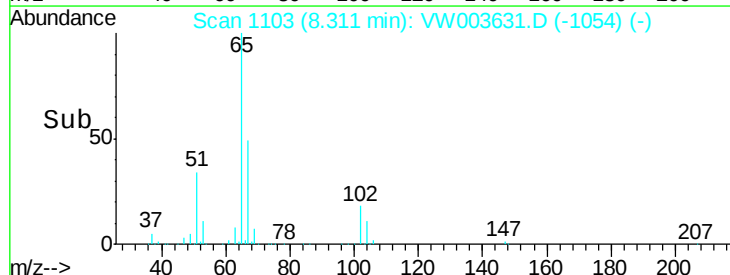

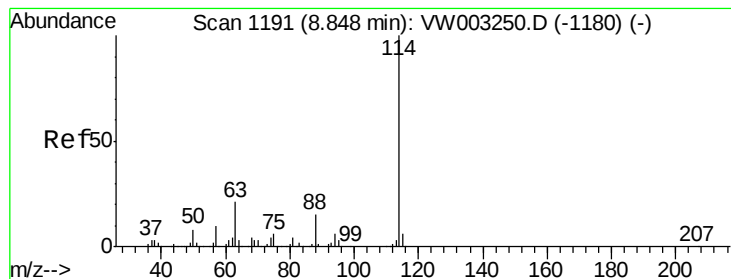

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 8.85 min Scan# 1191

Delta R.T. -0.00 min

Lab File: VW003631.D

Acq: 28 Jun 2018 11:54

Instrument :

MSVOA_W

ClientSampleId :

VW0628SBL01


Tot Ion:114 Resp: 332887

Ion Ratio Lower Upper

114 100

63 21.8 0.0 43.0




88 15.4 0.0 29.6

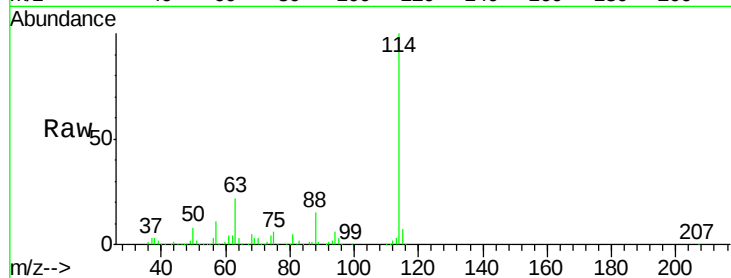

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

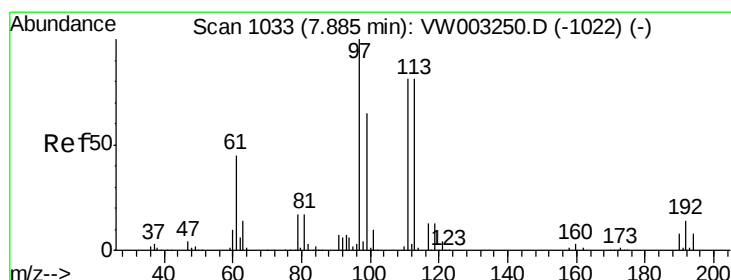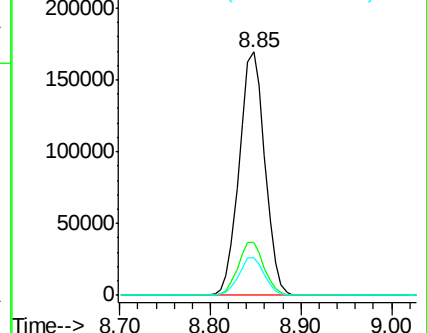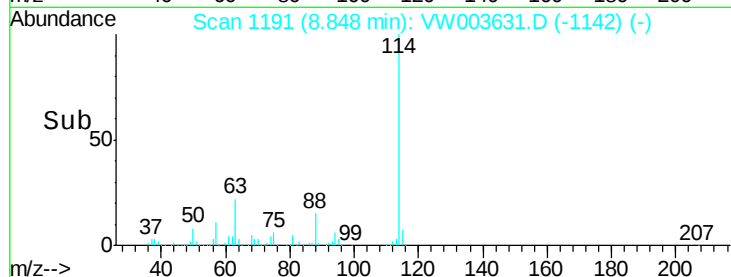

#35

Dibromofluoromethane

Concen: 51.99 ug/l

RT: 7.88 min Scan# 1033

Delta R.T. -0.00 min

Lab File: VW003631.D

Acq: 28 Jun 2018 11:54


Tgt Ion:113 Resp: 107549

Ion Ratio Lower Upper

113 100

111 102.8 82.2 123.2



192 19.6 16.2 24.2

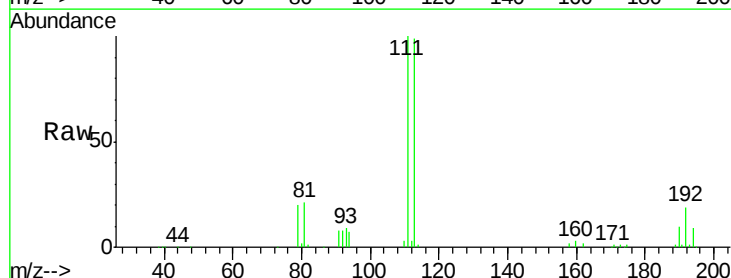


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

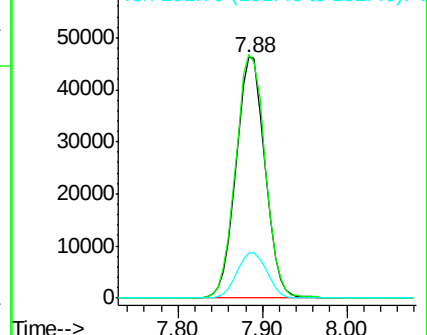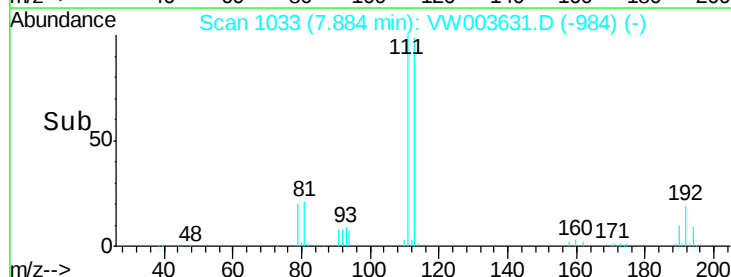

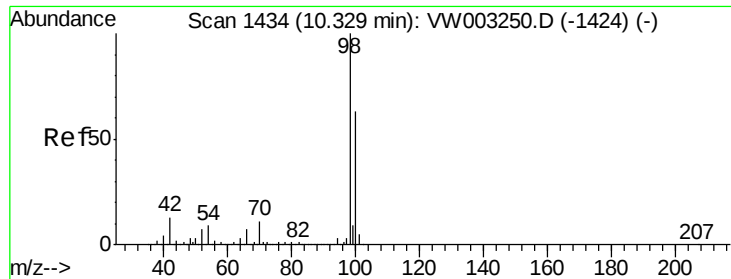

#50

Toluene-d8

Concen: 49.88 ug/l

RT: 10.33 min Scan# 1434

Delta R.T. -0.00 min

Lab File: VW003631.D

Acq: 28 Jun 2018 11:54

Instrument :

MSVOA_W

ClientSampleId :





VW0628SBL01

Tot Ion: 98 Resp: 409111

Ion Ratio Lower Upper

98 100

100 62.7 50.8 76.2

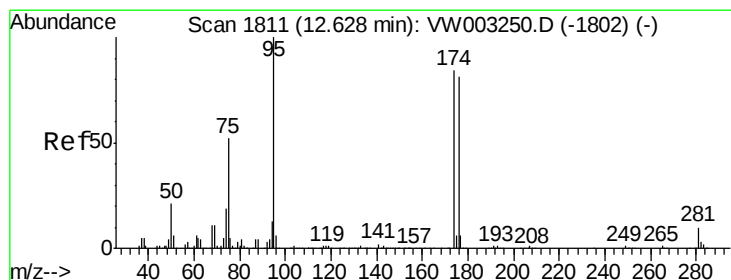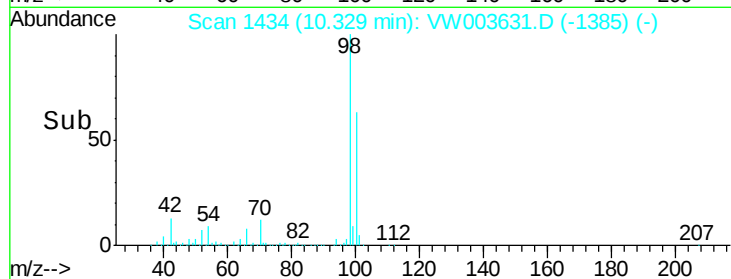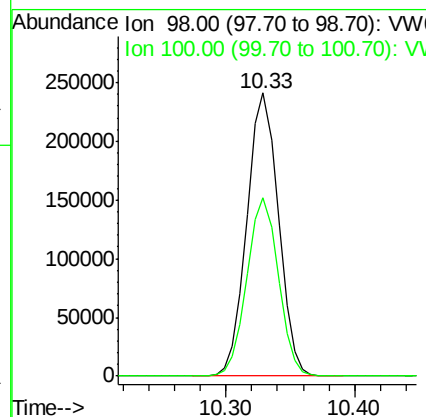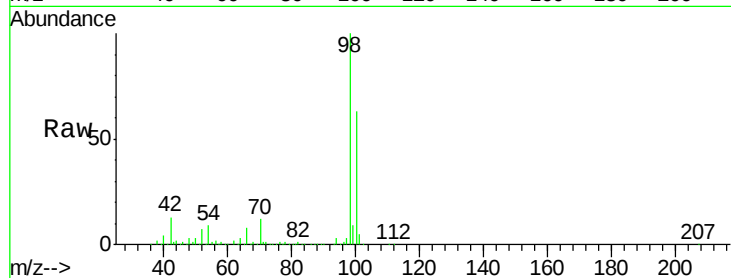

#62

4-Bromofluorobenzene

Concen: 47.13 ug/l

RT: 12.63 min Scan# 1811

Delta R.T. -0.00 min

Lab File: VW003631.D

Acq: 28 Jun 2018 11:54




Tgt Ion: 95 Resp: 136802


Ion Ratio Lower Upper

95 100

174 82.8 0.0 166.4

176 78.8 0.0 162.0


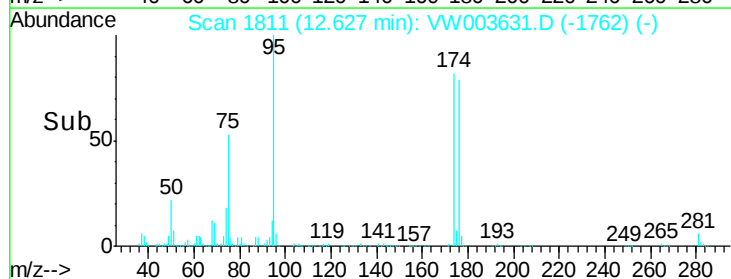
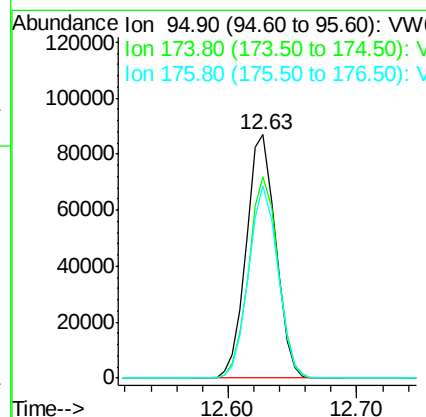
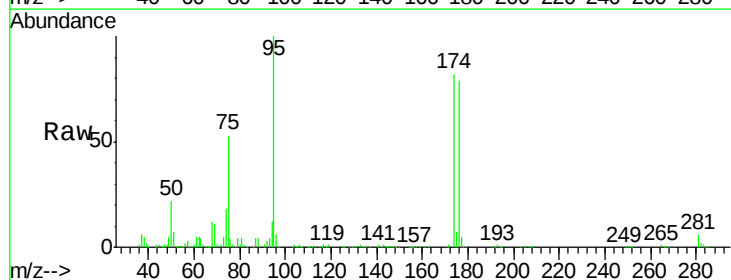


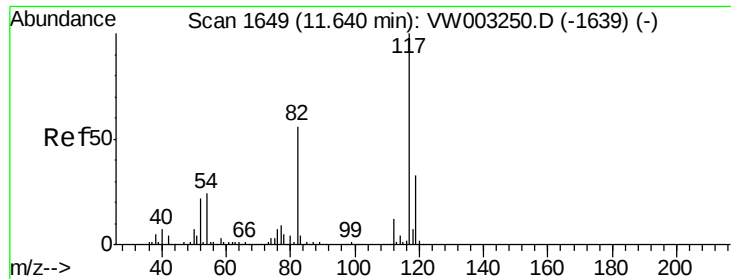

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.64 min Scan# 1649
Delta R.T. -0.00 min
Lab File: VW003631.D
Acq: 28 Jun 2018 11:54

Instrument :
MSVOA_W
ClientSampleId :
VW0628SBL01

Tot Ion:117 Resp: 303149
Ion Ratio Lower Upper
117 100
82 56.4 44.6 67.0
119 32.4 26.7 40.1

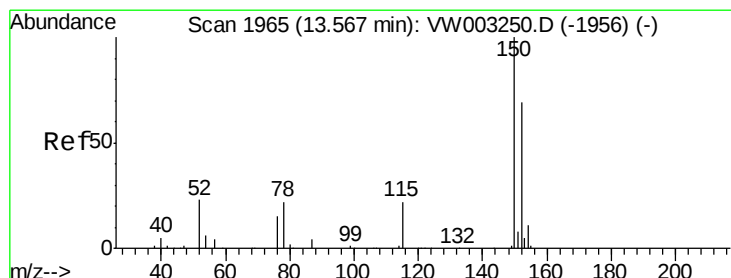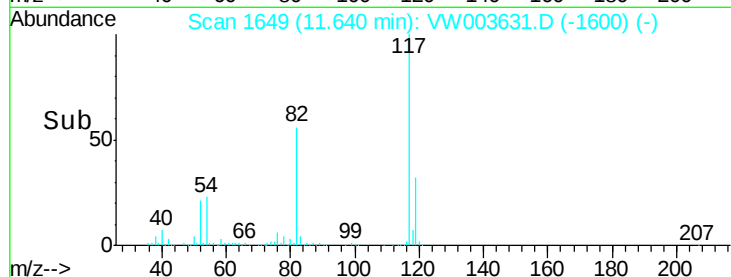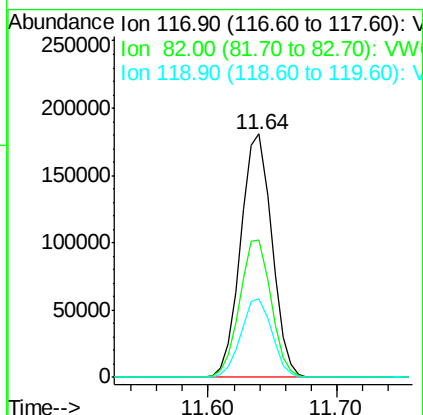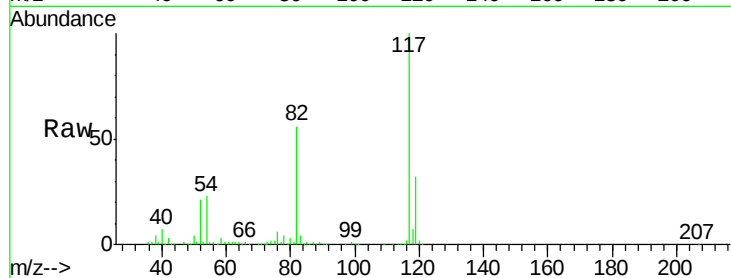

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.57 min Scan# 1965
Delta R.T. -0.00 min
Lab File: VW003631.D
Acq: 28 Jun 2018 11:54

Tgt Ion:152 Resp: 147421
Ion Ratio Lower Upper
152 100
115 58.5 29.3 88.0
150 158.0 0.0 349.6

