


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062818\
 Data File : VW003629.D
 Acq On : 28 Jun 2018 09:48
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
 Title : SW846 8260
 Last Update : Sat Jun 16 05:18:54 2018

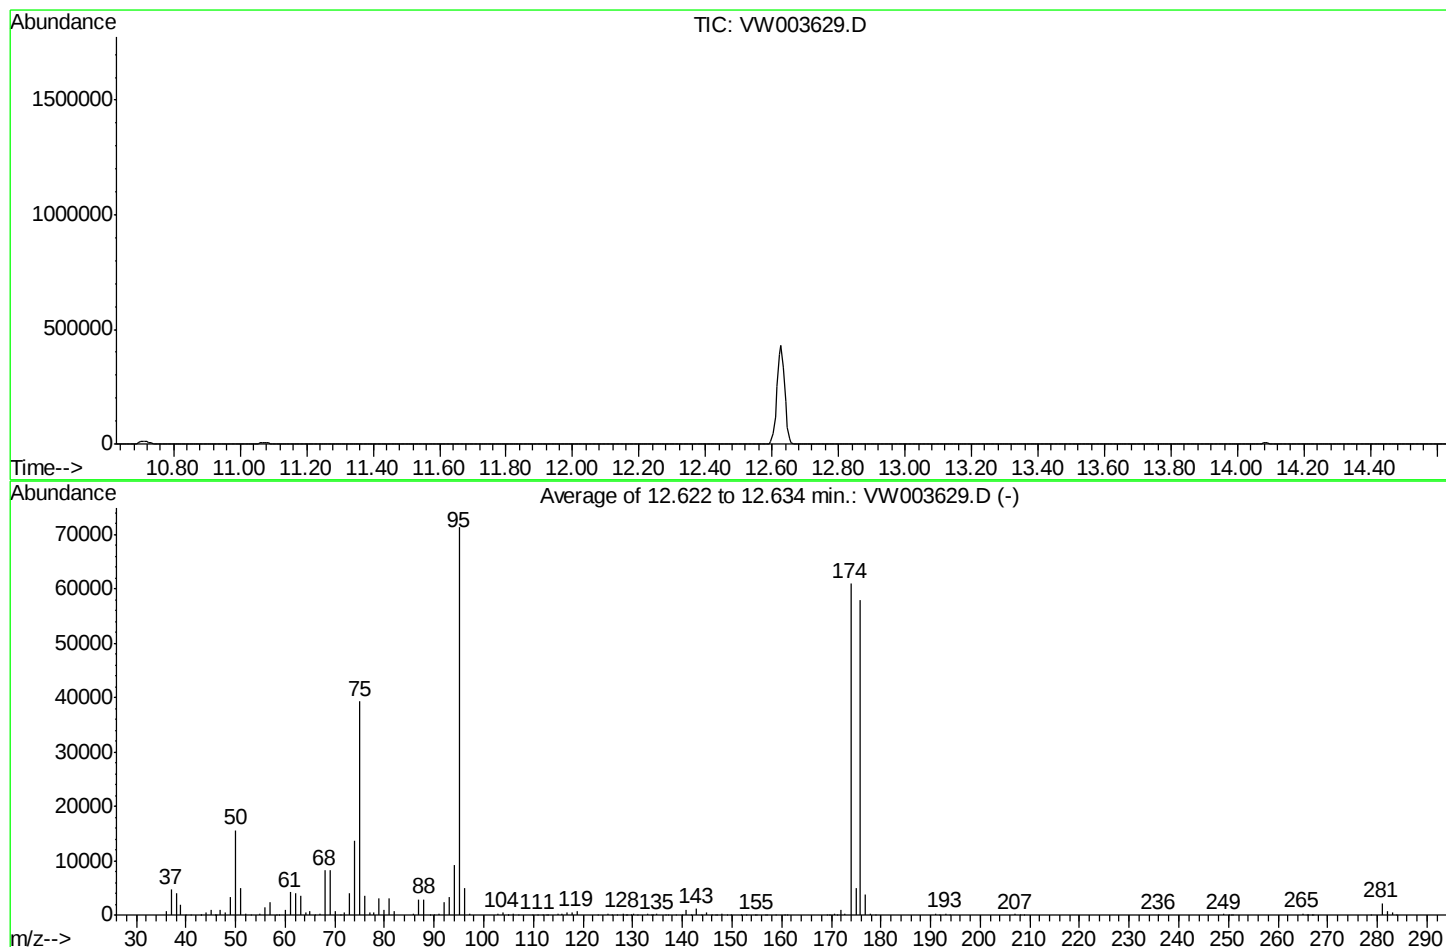

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	15586	PASS
75	95	30	60	55.1	39264	PASS
95	95	100	100	100.0	71301	PASS
96	95	5	9	7.0	5017	PASS
173	174	0.00	2	0.5	314	PASS
174	95	50	100	85.5	60960	PASS
175	174	5	9	8.0	4857	PASS
176	174	95	101	95.1	57994	PASS
177	176	5	9	6.4	3735	PASS