




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026393.D
 Acq On : 28 Jun 2023 13:09
 Operator : SY/MD
 Sample : 03420-06RE
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4645RE

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:50:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

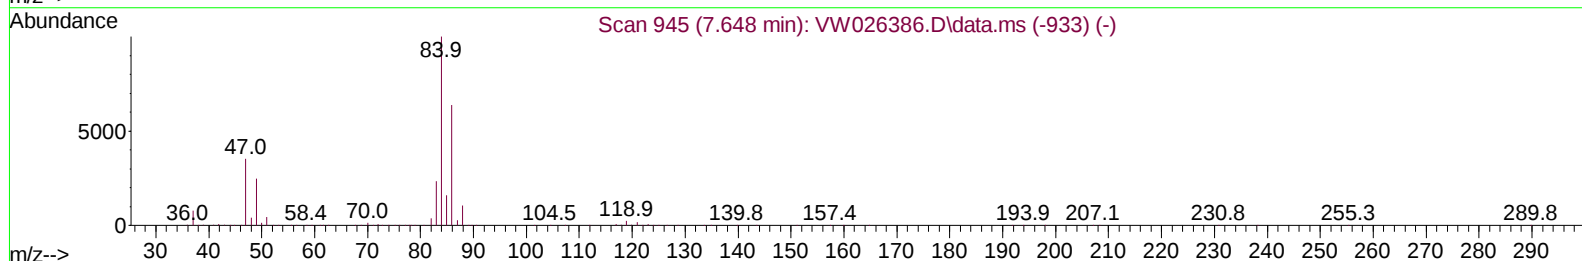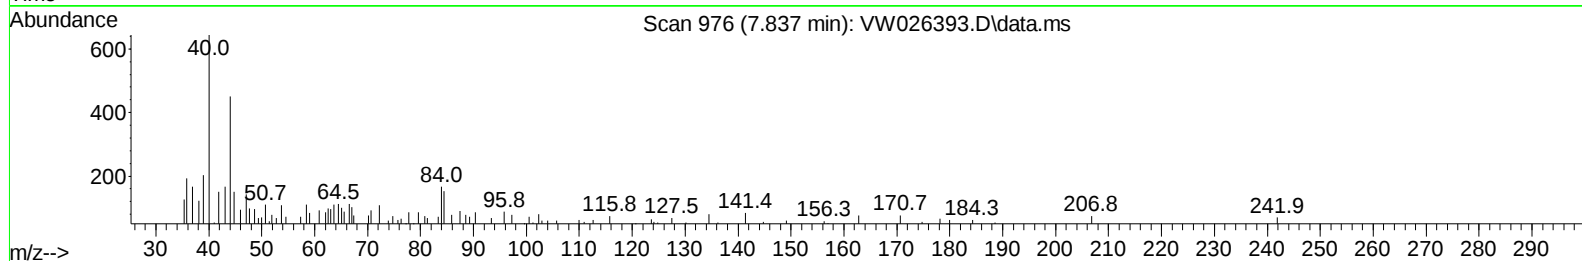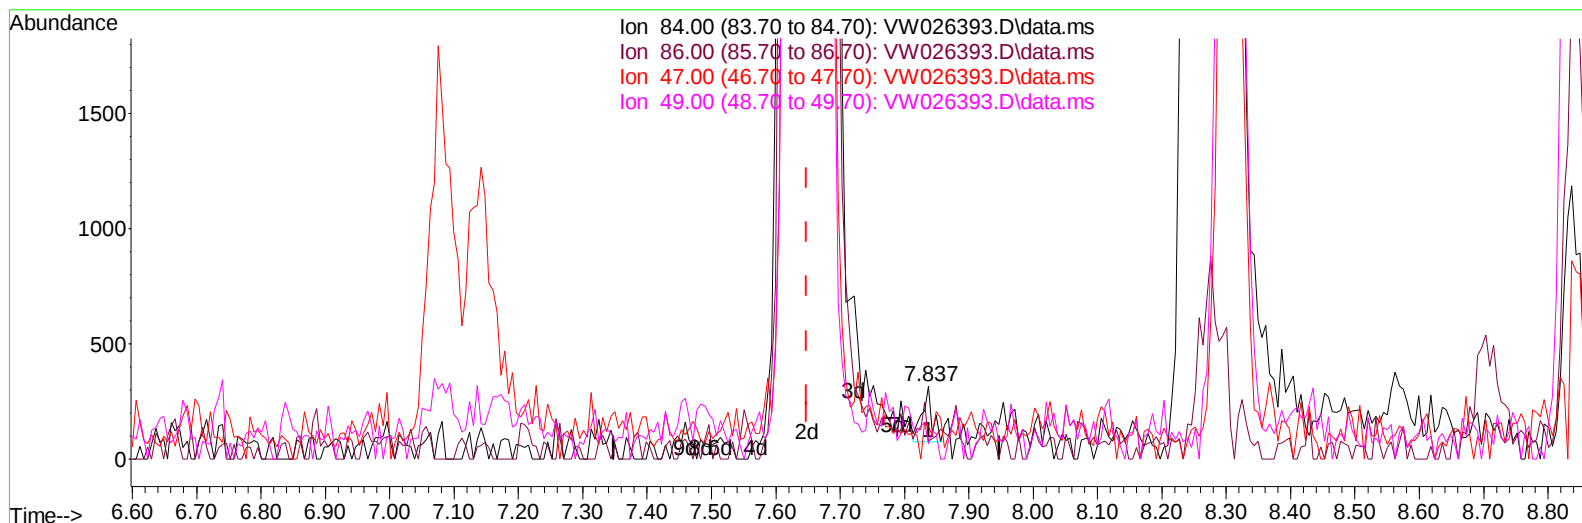

TIC: VW026393.D\data.ms

(24) Chloroform-d (S)

7.837min (+ 0.189) 0.01 ug/L

response 267

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.50	74.16
47.00	52.30	49.81
49.00	29.40	32.21




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026393.D
 Acq On : 28 Jun 2023 13:09
 Operator : SY/MD
 Sample : 03420-06RE
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4645RE

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:50:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

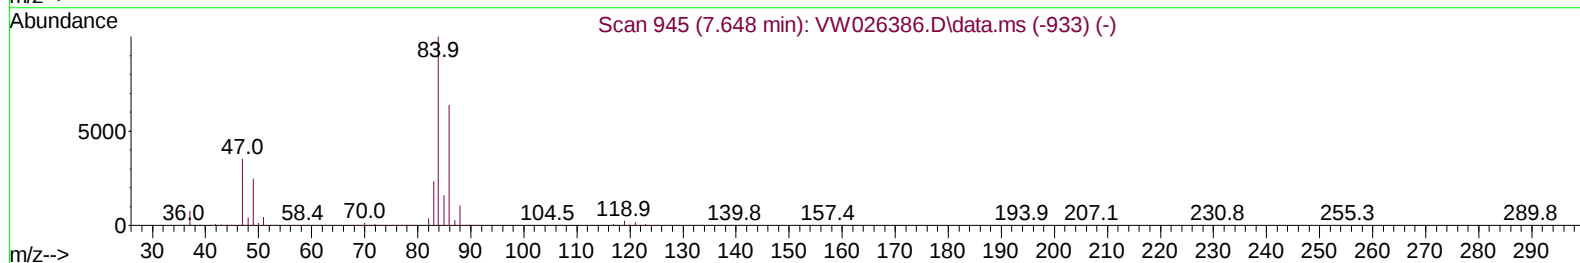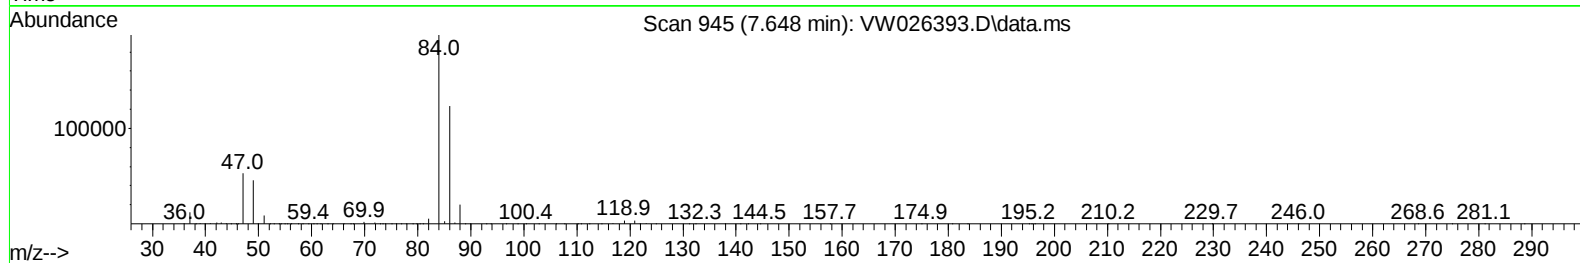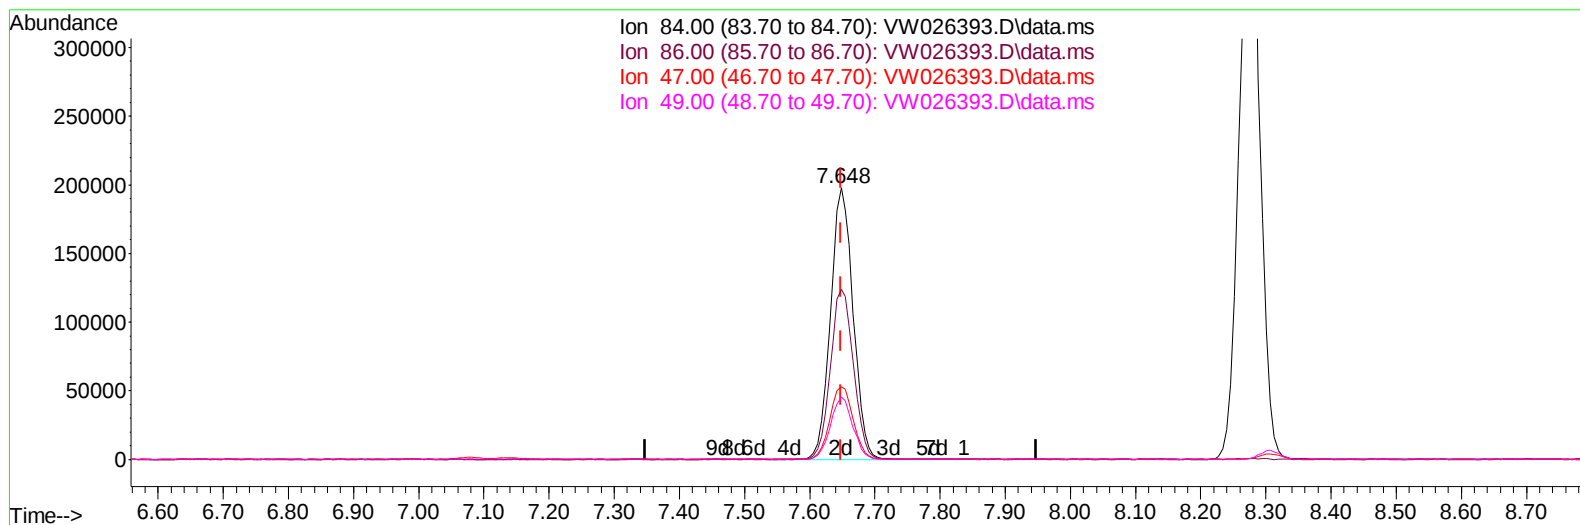

TIC: VW026393.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 22.37 ug/L m

response 474851

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.50	0.04#
47.00	52.30	0.03#
49.00	29.40	0.02#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026393.D
 Acq On : 28 Jun 2023 13:09
 Operator : SY/MD
 Sample : 03420-06RE
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4645RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 23:50:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

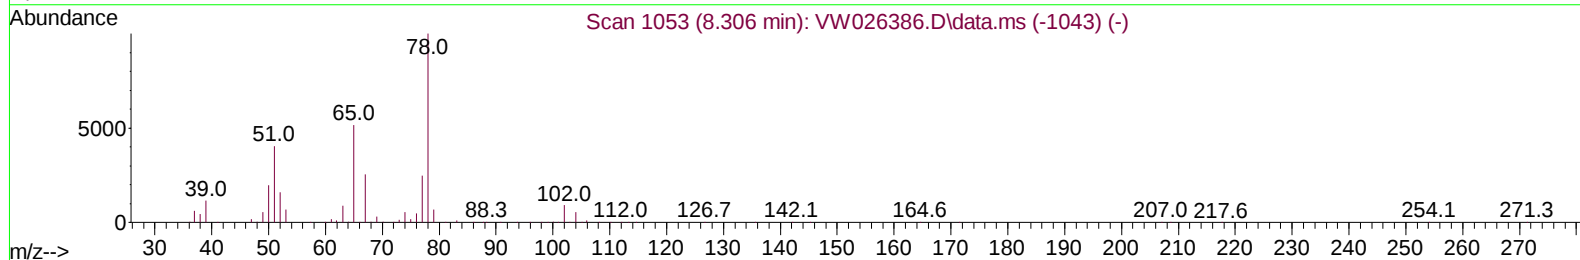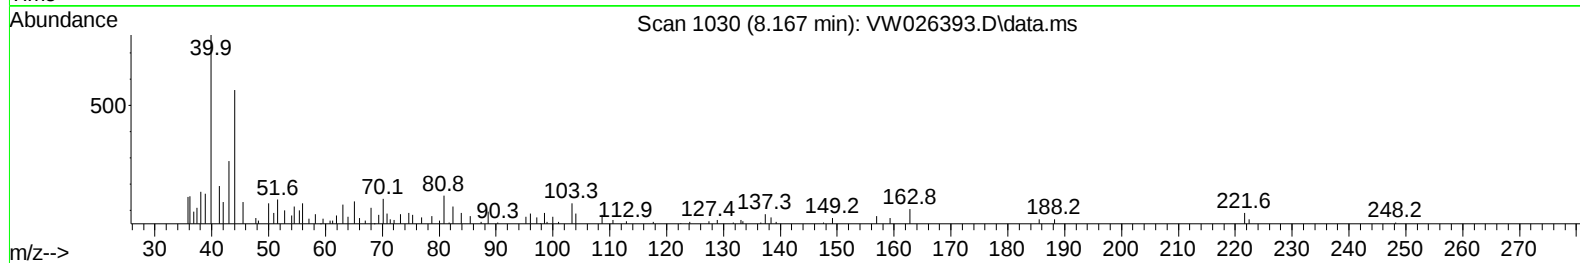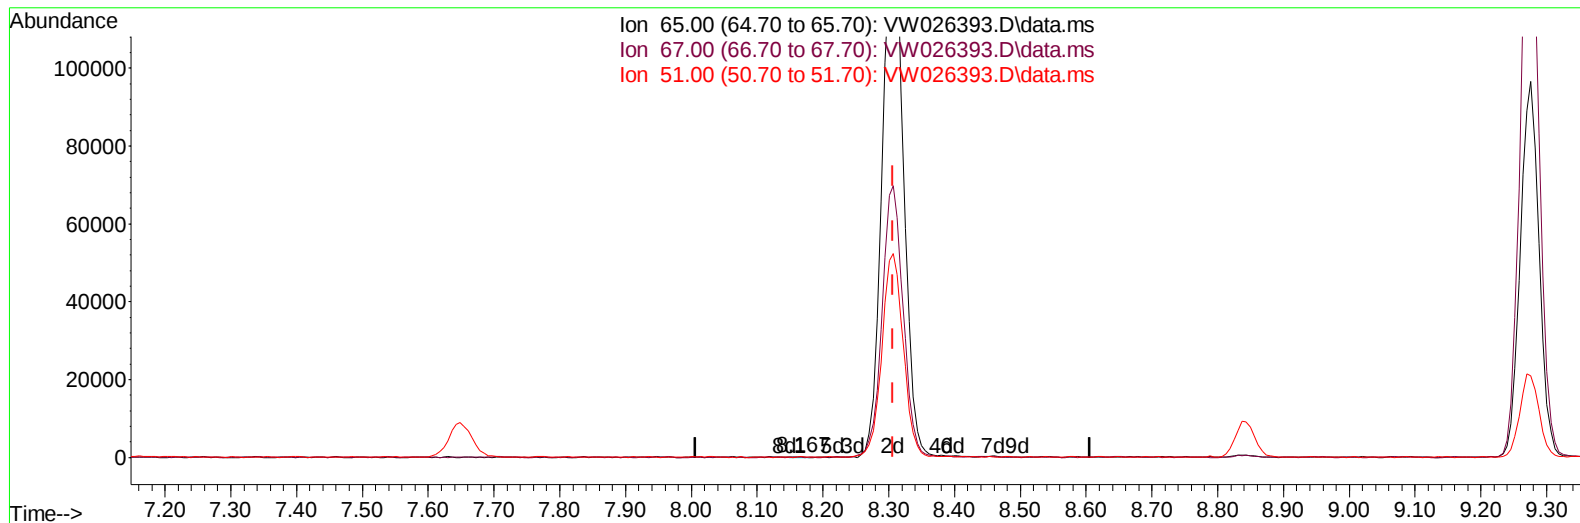

TIC: VW026393.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.167min (-0.140) 0.01 ug/L

response 142

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.20	55.63
51.00	117.60	120.42
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026393.D
 Acq On : 28 Jun 2023 13:09
 Operator : SY/MD
 Sample : 03420-06RE
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4645RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 23:50:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

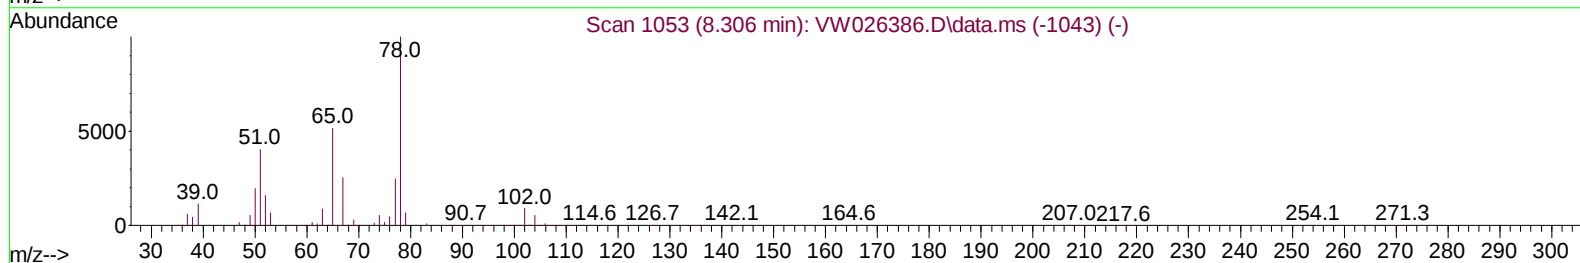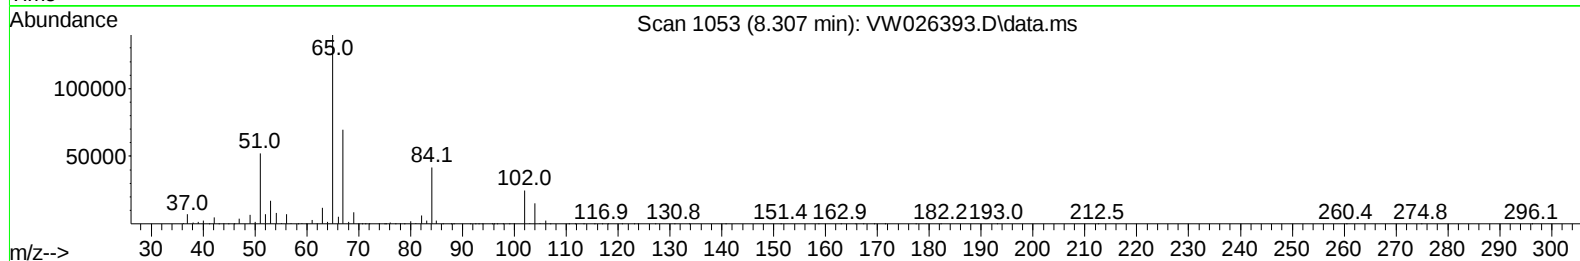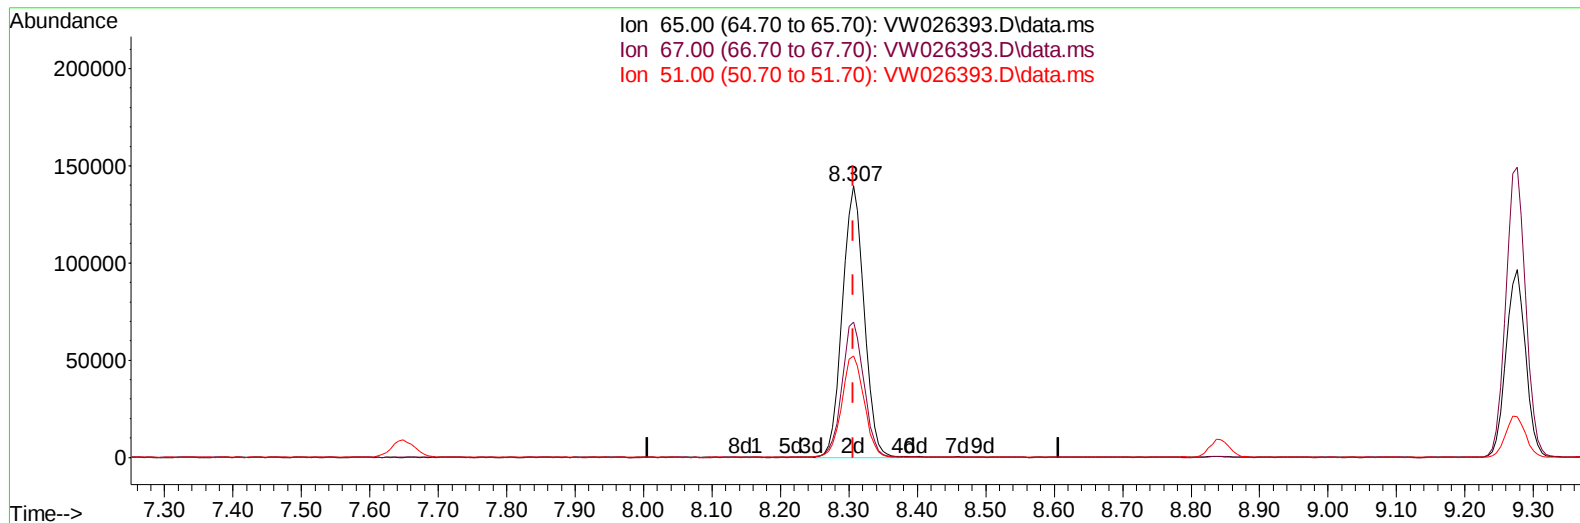

TIC: VW026393.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.61 ug/L m

response 305486

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	53.20	0.03#
51.00	117.60	0.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026393.D
 Acq On : 28 Jun 2023 13:09
 Operator : SY/MD
 Sample : 03420-06RE
 Misc : 4.72g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4645RE

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:50:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		749095	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		500379	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		129611	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		232322	21.348	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	85.400%	
7) Chloroethane-d5	2.893	69		245150	31.689	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	126.760%	
11) 1,1-Dichloroethene-d2	4.027	65		113393	23.015	ug/L	0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	92.040%	
21) 2-Butanone-d5	7.081	46		161854	47.323	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	94.640%	
24) Chloroform-d	7.648	84		474851m	22.370	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	89.480%	
26) 1,2-Dichloroethane-d4	8.307	65		305486m	25.613	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	102.440%	
32) Benzene-d6	8.276	84		936865	30.248	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	121.000%	
36) 1,2-Dichloropropane-d6	9.276	67		301672	29.975	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	119.880%	
41) Toluene-d8	10.325	98		714729	26.364	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	105.440%	
43) trans-1,3-Dichloroprop...	10.575	79		101756	25.182	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	100.720%	
47) 2-Hexanone-d5	10.922	63		94577	61.189	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	122.380%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		184023	23.225	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	92.880%	
66) 1,2-Dichlorobenzene-d4	13.855	152		99644	22.080	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	88.320%	
Target Compounds							
						Qvalue	
13) Acetone	4.125	43		277292	101.292	ug/L	98
22) 2-Butanone	7.173	43		113762	27.159	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026393.D
Acq On : 28 Jun 2023 13:09
Operator : SY/MD
Sample : 03420-06RE
Misc : 4.72g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4645RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2023
Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 23:50:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 23:48:01 2023
Response via : Initial Calibration

