




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026394.D
 Acq On : 28 Jun 2023 13:32
 Operator : SY/MD
 Sample : 03420-11RE
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46E5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:50:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

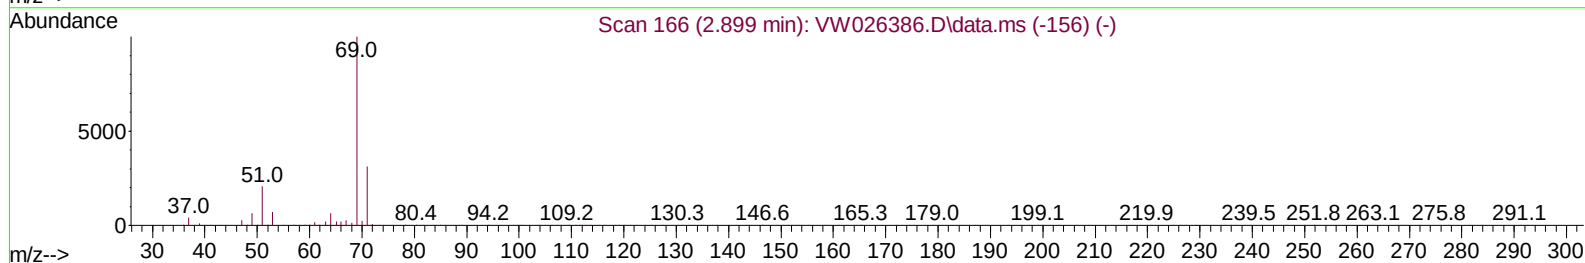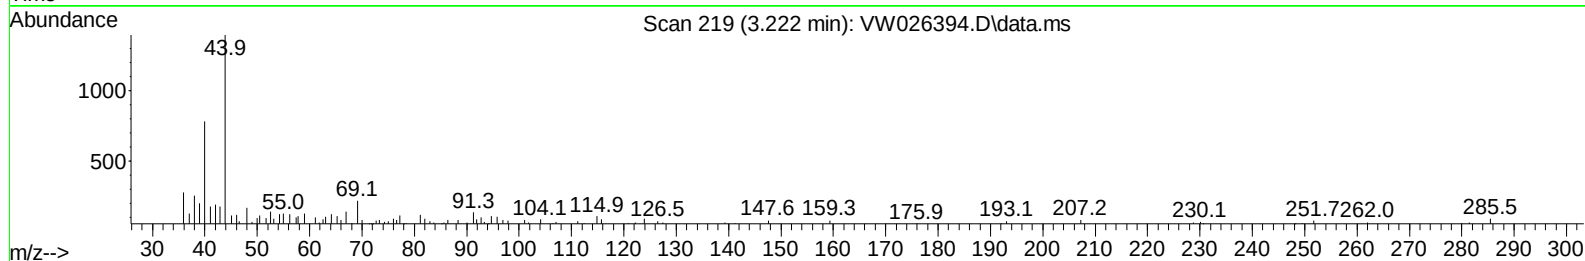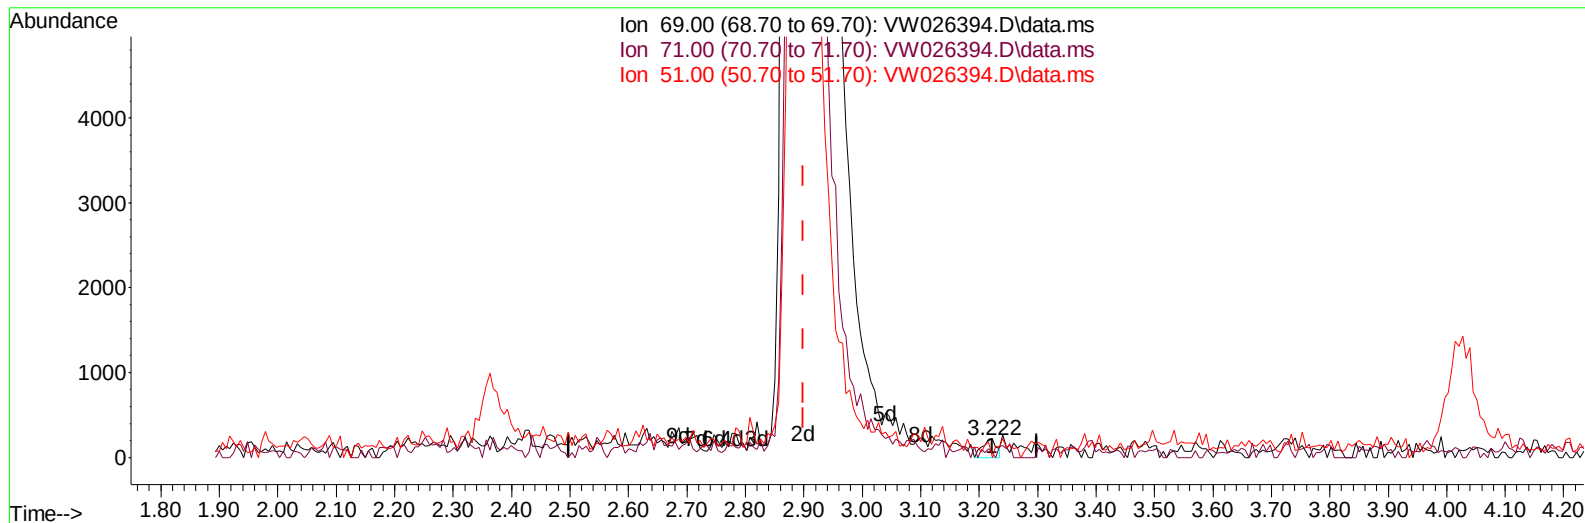

TIC: VW026394.D\data.ms

(7) Chloroethane-d5 (S)

3.222min (+ 0.324) 0.04 ug/L

response	371	
Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	29.92
51.00	28.50	32.35
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026394.D
 Acq On : 28 Jun 2023 13:32
 Operator : SY/MD
 Sample : 03420-11RE
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46E5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:50:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

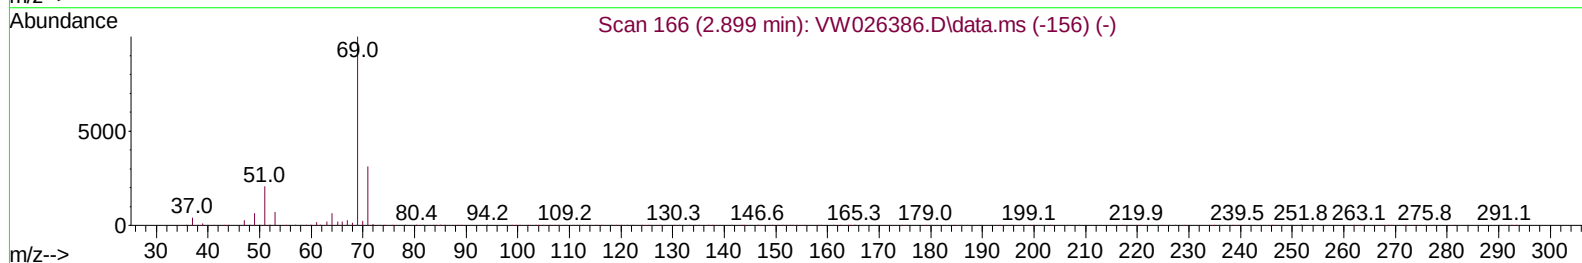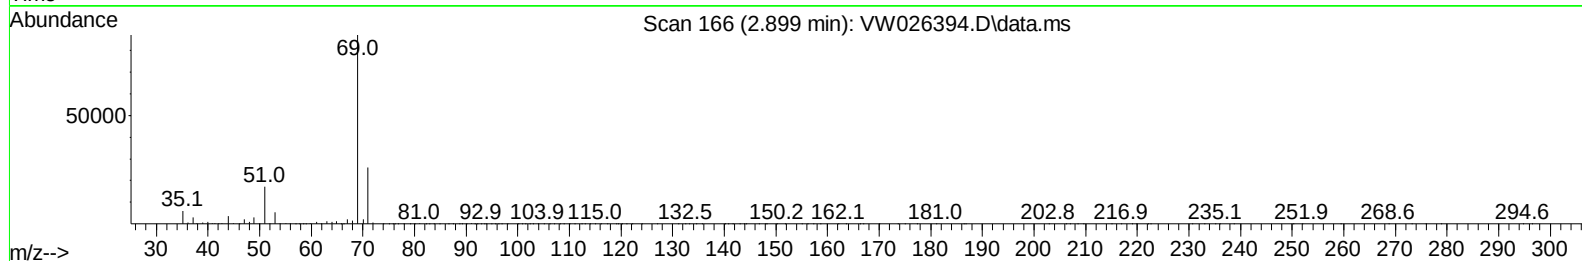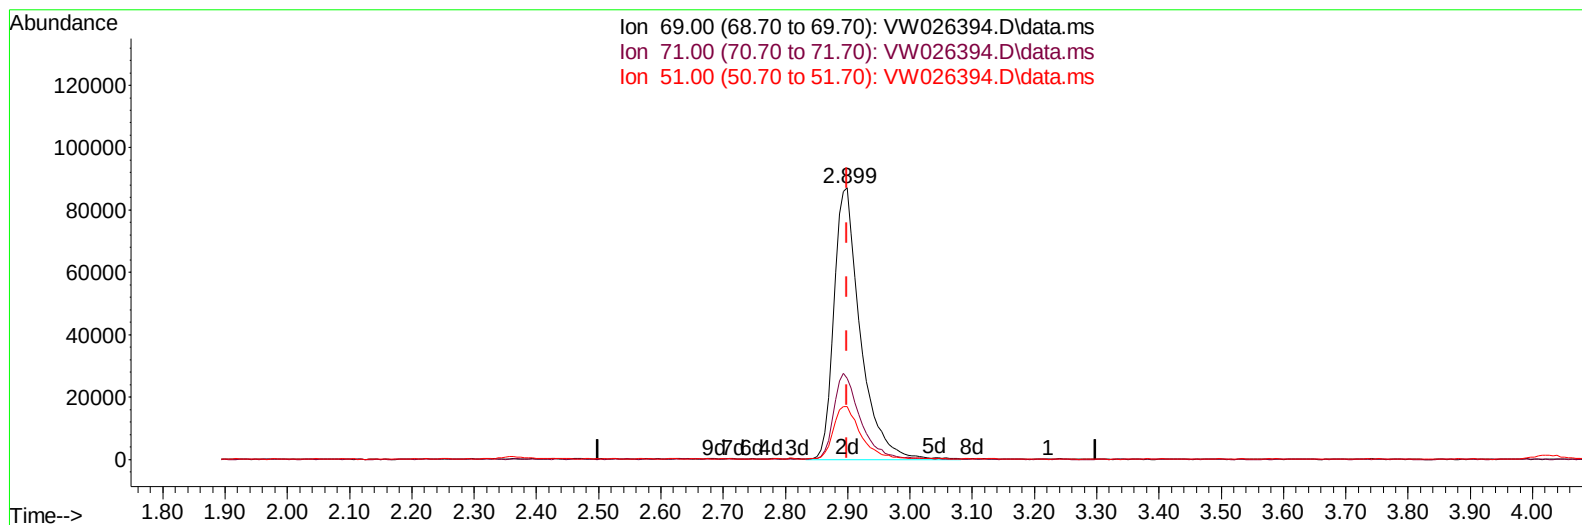

TIC: VW026394.D\data.ms

(7) Chloroethane-d5 (S)

2.899min (+ 0.000) 29.39 ug/L m

response 256357

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	31.70	0.04#
51.00	28.50	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026394.D
 Acq On : 28 Jun 2023 13:32
 Operator : SY/MD
 Sample : 03420-11RE
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46E5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:50:41 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 28 23:48:01 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		844738	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		607094	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		206619	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		223446	18.208	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	72.840%	
7) Chloroethane-d5	2.899	69		256357m	29.385	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	117.560%	
11) 1,1-Dichloroethene-d2	4.021	65		120295	21.651	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	86.600%	
21) 2-Butanone-d5	7.075	46		160131	41.518	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	83.040%	
24) Chloroform-d	7.648	84		502841	21.007	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	84.040%	
26) 1,2-Dichloroethane-d4	8.307	65		327645	24.360	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	97.440%	
32) Benzene-d6	8.276	84		1003915	26.716	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	106.880%	
36) 1,2-Dichloropropane-d6	9.276	67		321559	26.334	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	105.320%	
41) Toluene-d8	10.319	98		797671	24.251	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	97.000%	
43) trans-1,3-Dichloroprop...	10.575	79		108852	22.203	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	88.800%	
47) 2-Hexanone-d5	10.922	63		102049	54.418	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	108.840%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84		267227	27.797	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	111.200%	
66) 1,2-Dichlorobenzene-d4	13.855	152		162042	22.524	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	90.080%	
Target Compounds							
13) Acetone	4.125	43		52519	17.012	ug/L	Qvalue 100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026394.D
Acq On : 28 Jun 2023 13:32
Operator : SY/MD
Sample : 03420-11RE
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46E5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2023
Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 28 23:50:41 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 28 23:48:01 2023
Response via : Initial Calibration

