




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026425.D
 Acq On : 29 Jun 2023 04:00
 Operator : SY/MD
 Sample : 03458-11
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 06:30:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 29 02:27:38 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

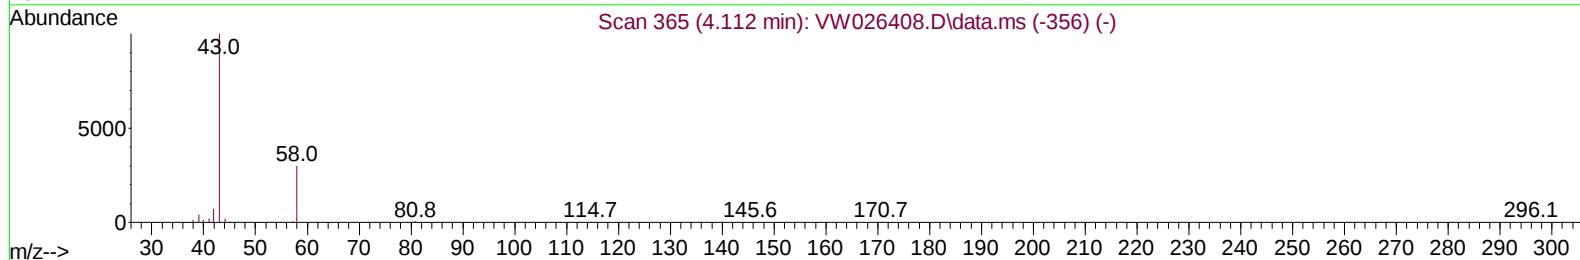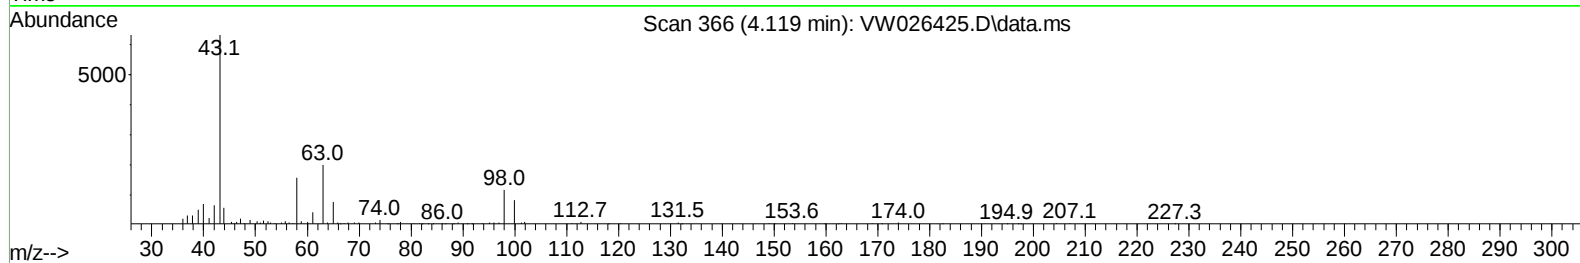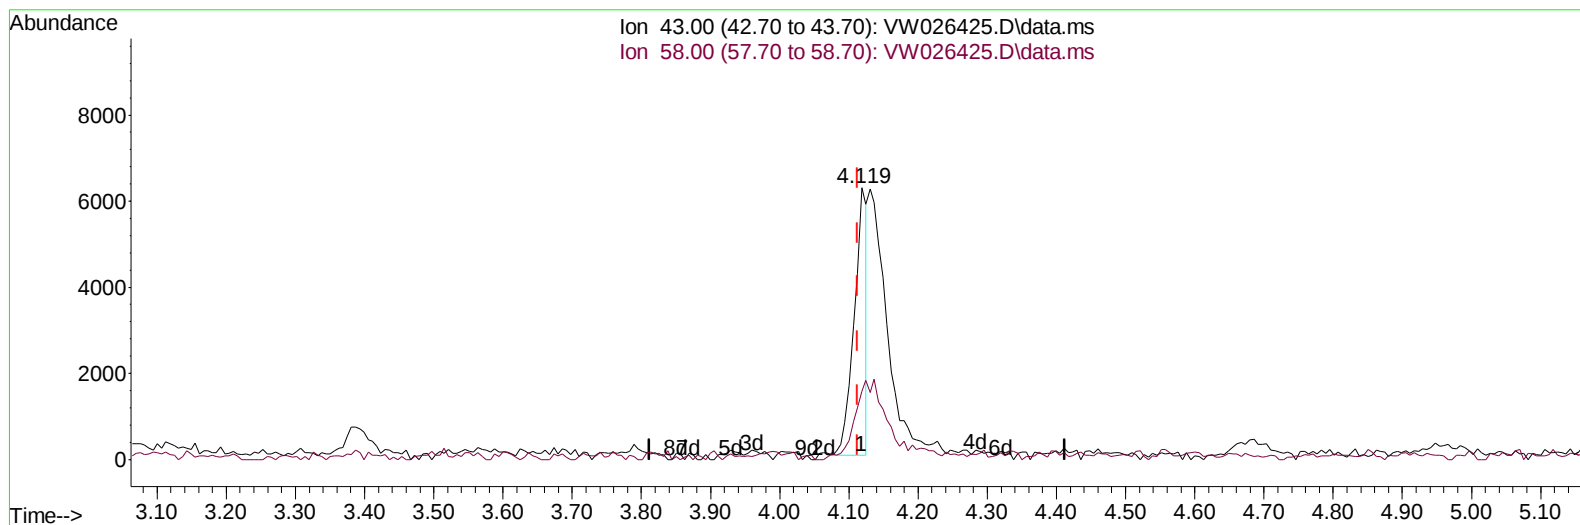

TIC: VW026425.D\data.ms

(13) Acetone (T)

4.119min (+ 0.006) 1.88 ug/L

response 8058

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	27.90	32.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026425.D
Acq On : 29 Jun 2023 04:00
Operator : SY/MD
Sample : 03458-11
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2023
Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 29 06:30:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 29 02:27:38 2023
Response via : Initial Calibration

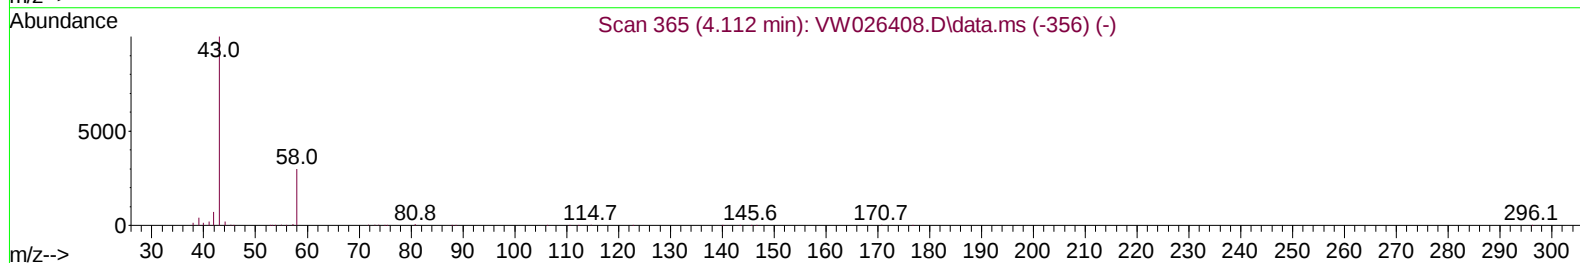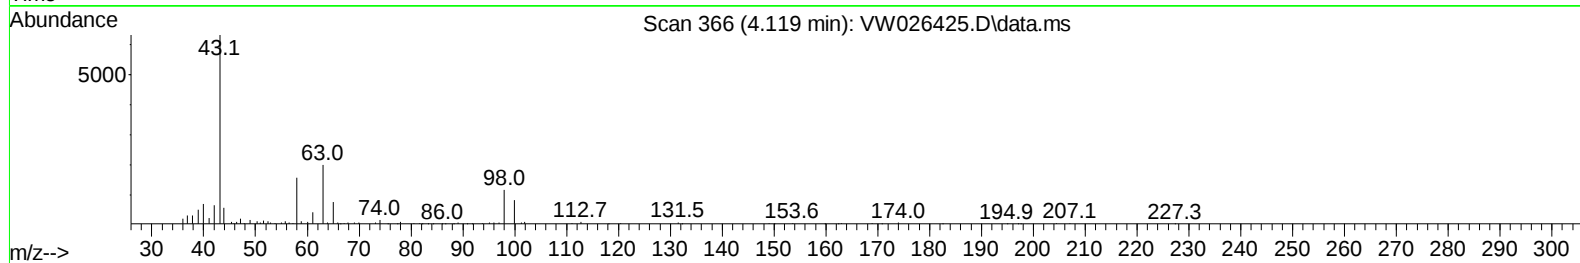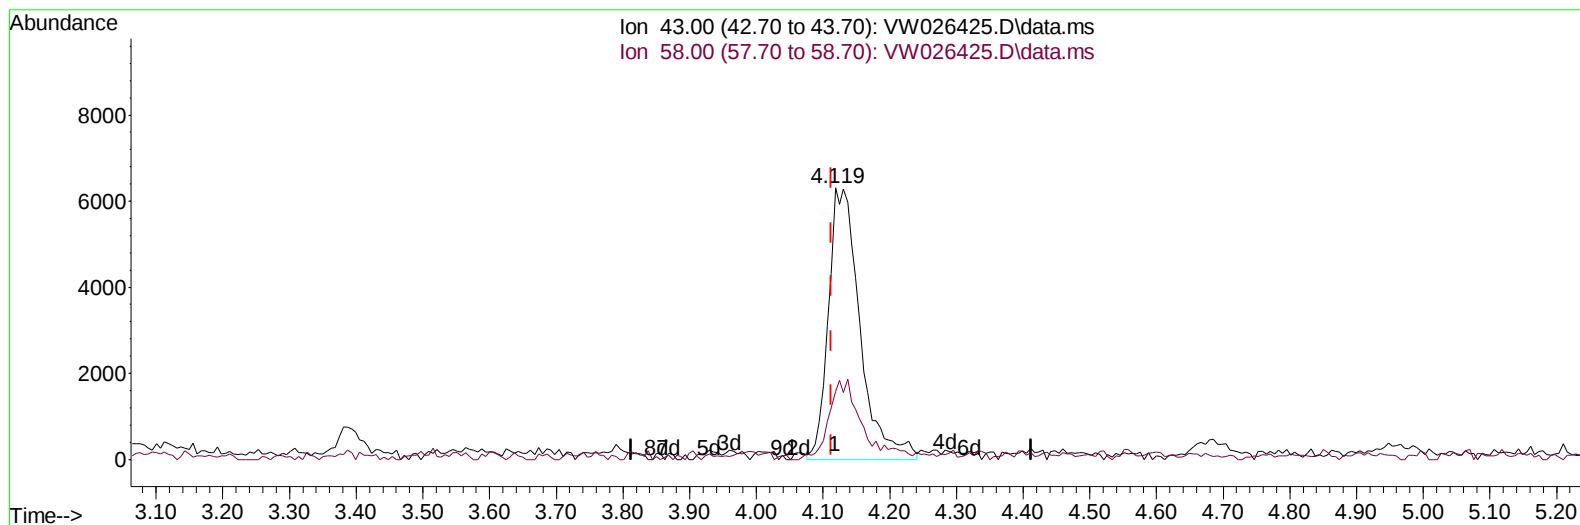

TIC: VW026425.D\data.ms

(13) Acetone (T)

4.119min (+ 0.006) 4.85 ug/L m

response 20761

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	27.90	12.54
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026425.D
 Acq On : 29 Jun 2023 04:00
 Operator : SY/MD
 Sample : 03458-11
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46M4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 06:30:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 29 02:27:38 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/29/2023
 Supervised By :Mahesh Dadoda 06/29/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		1170893	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		987811	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		450880	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.369	65		268393	15.778	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	63.120%		
7) Chloroethane-d5	2.893	69		257560	21.299	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	85.200%		
11) 1,1-Dichloroethene-d2	4.021	65		118911	15.441	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	61.760%		
21) 2-Butanone-d5	7.081	46		160197	29.965	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	59.940%		
24) Chloroform-d	7.648	84		694981	20.946	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	83.800%		
26) 1,2-Dichloroethane-d4	8.307	65		400211	21.467	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	85.880%		
32) Benzene-d6	8.276	84		1395880	22.830	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	91.320%		
36) 1,2-Dichloropropane-d6	9.276	67		443128	22.304	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	89.200%		
41) Toluene-d8	10.319	98		1165745	21.782	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	87.120%		
43) trans-1,3-Dichloroprop...	10.575	79		149797	18.778	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	75.120%		
47) 2-Hexanone-d5	10.922	63		106033	34.750	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	69.500%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		337316	21.565	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	86.240%		
66) 1,2-Dichlorobenzene-d4	13.849	152		349965	22.292	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	89.160%		
Target Compounds							
13) Acetone	4.119	43		20761m	4.852	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026425.D
Acq On : 29 Jun 2023 04:00
Operator : SY/MD
Sample : 03458-11
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46M4

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/29/2023
Supervised By :Mahesh Dadoda 06/29/2023

Quant Time: Jun 29 06:30:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 29 02:27:38 2023
Response via : Initial Calibration

