

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026417.D
 Acq On : 29 Jun 2023 00:48
 Operator : SY/MD
 Sample : VIBLK479
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK479

Quant Time: Jun 29 04:14:23 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 29 02:27:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	874030	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	775485	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	371082	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	203989	16.065	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	64.240%		
7) Chloroethane-d5	2.899	69	172393	19.099	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	76.400%		
11) 1,1-Dichloroethene-d2	4.021	65	106194	18.473	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	73.880%		
21) 2-Butanone-d5	7.075	46	172494	43.225	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.440%		
24) Chloroform-d	7.648	84	474305	19.151	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	76.600%		
26) 1,2-Dichloroethane-d4	8.307	65	271630	19.519	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.080%		
32) Benzene-d6	8.276	84	1018652	21.222	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	84.880%		
36) 1,2-Dichloropropane-d6	9.276	67	330970	21.219	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.880%		
41) Toluene-d8	10.325	98	893734	21.272	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	85.080%		
43) trans-1,3-Dichloroprop...	10.575	79	120824	19.293	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	77.160%		
47) 2-Hexanone-d5	10.922	63	111582	46.581	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.160%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	251677	20.495	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	82.000%		
66) 1,2-Dichlorobenzene-d4	13.849	152	283806	21.966	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.880%		
Target Compounds						Qvalue
16) Methylene chloride	4.917	84	60924	4.119	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026417.D
Acq On : 29 Jun 2023 00:48
Operator : SY/MD
Sample : VIBLK479
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK479

Quant Time: Jun 29 04:14:23 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 29 02:27:38 2023
Response via : Initial Calibration

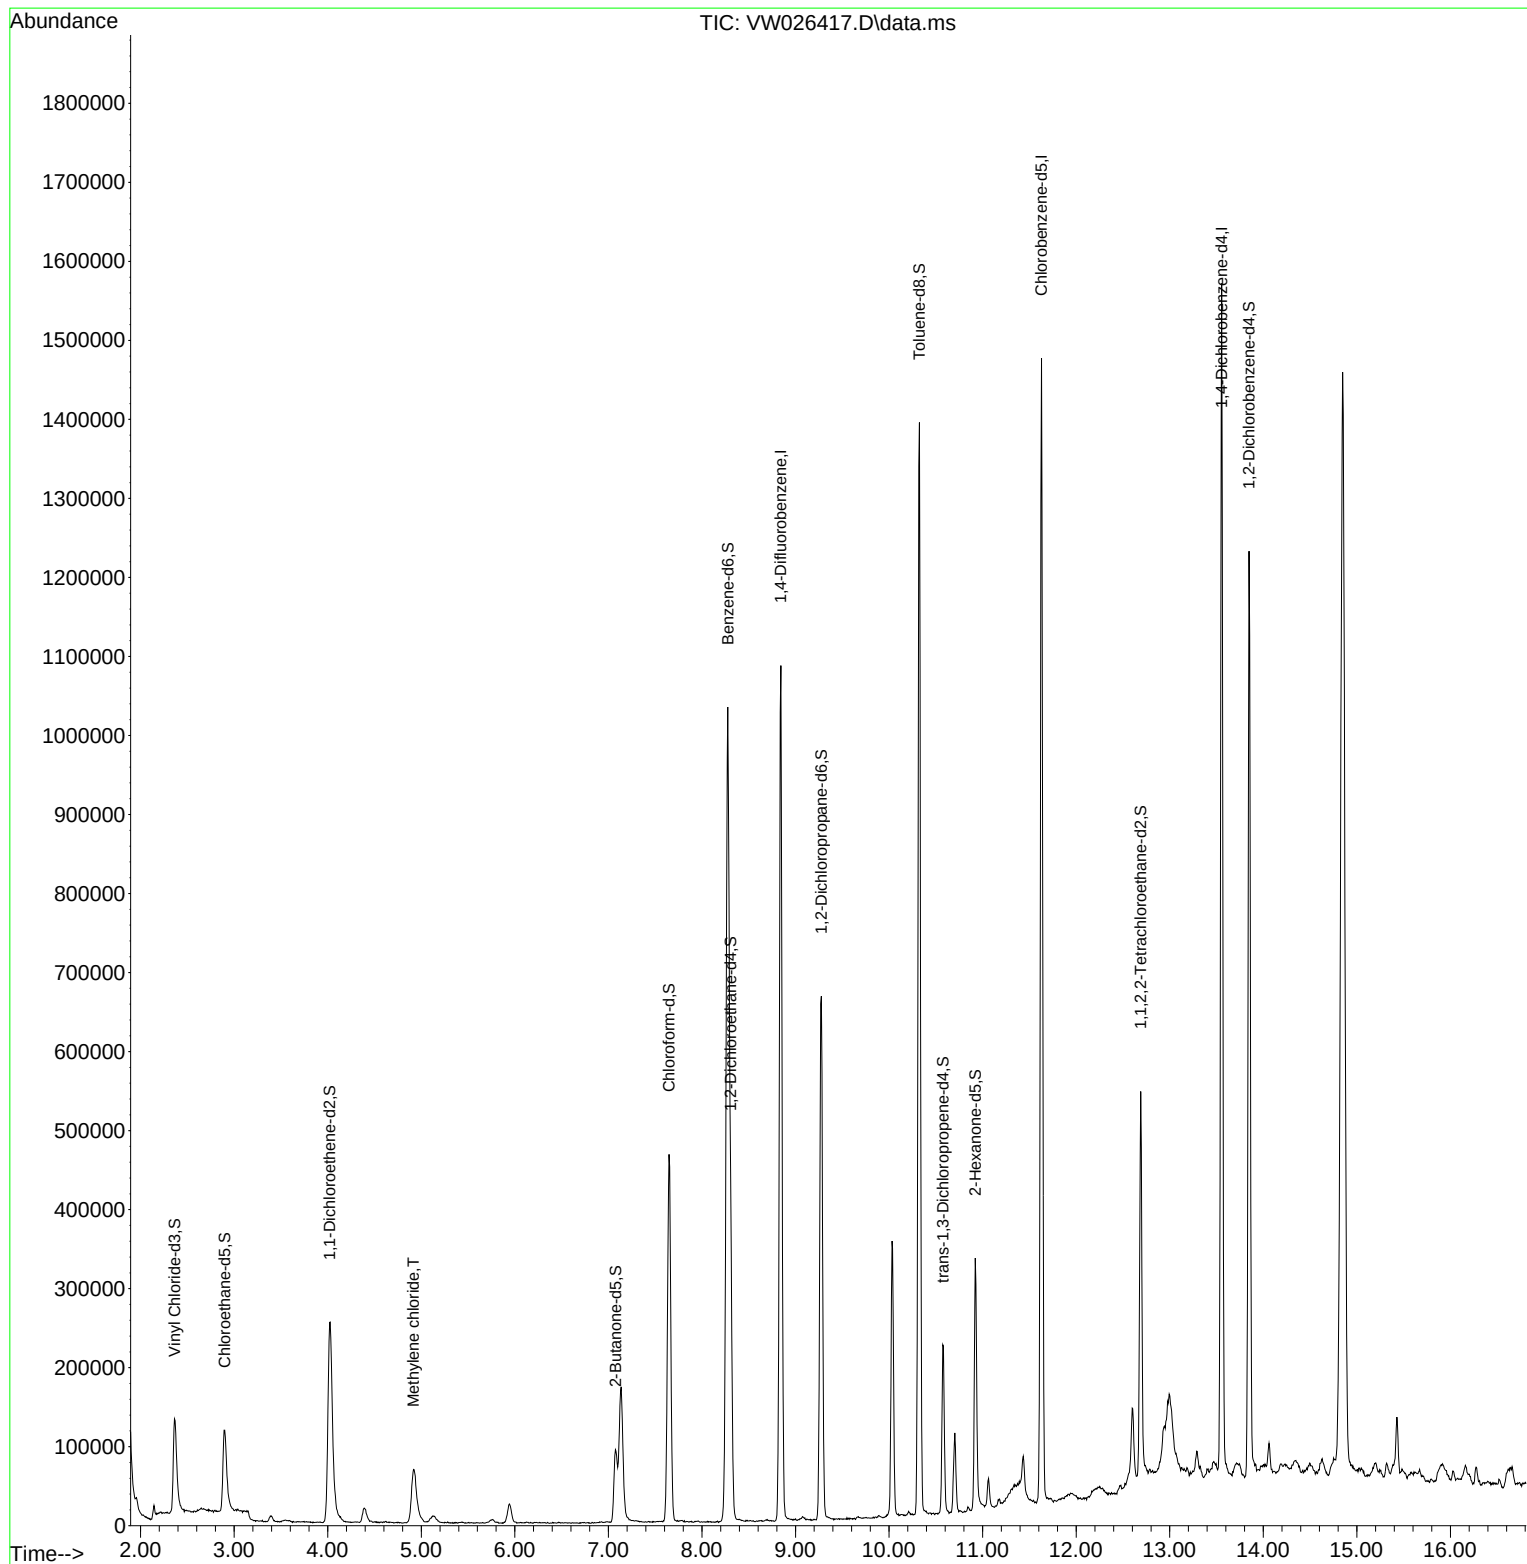

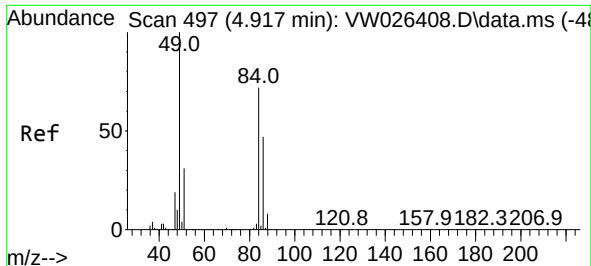

#16
Methylene chloride
Concen: 4.119 ug/L
RT: 4.917 min Scan# 49
Delta R.T. 0.000 min
Lab File: VW026417.D
Acq: 29 Jun 2023 00:48

Instrument :
MSVOA_W
ClientSampleId :
VIBLK479

Tgt Ion: 84 Resp: 60924
Ion Ratio Lower Upper
84 100
86 60.3 43.9 81.5
49 130.7 100.4 186.4

