

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026419.D
 Acq On : 29 Jun 2023 01:36
 Operator : SY/MD
 Sample : 03458-05
 Misc : 4.81g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46L8

Quant Time: Jun 29 04:14:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 29 02:27:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1239683	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1086448	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	514063	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.369	65	262309	14.565	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.240%		
7) Chloroethane-d5	2.899	69	253970	19.837	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	79.360%		
11) 1,1-Dichloroethene-d2	4.021	65	127115	15.590	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	62.360%		
21) 2-Butanone-d5	7.075	46	279273	49.340	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.680%		
24) Chloroform-d	7.648	84	668963	19.043	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	76.160%		
26) 1,2-Dichloroethane-d4	8.307	65	411269	20.836	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.360%		
32) Benzene-d6	8.276	84	1448399	21.538	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	86.160%		
36) 1,2-Dichloropropane-d6	9.270	67	449751	20.582	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	82.320%		
41) Toluene-d8	10.319	98	1196482	20.327	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	81.320%		
43) trans-1,3-Dichloroprop...	10.575	79	174721	19.914	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	79.640%		
47) 2-Hexanone-d5	10.922	63	192374	57.323	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	114.640%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	406226	23.612	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	94.440%		
66) 1,2-Dichlorobenzene-d4	13.848	152	410196	22.917	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.680%		
Target Compounds					Qvalue	
13) Acetone	4.125	43	23201	5.121	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026419.D
Acq On : 29 Jun 2023 01:36
Operator : SY/MD
Sample : 03458-05
Misc : 4.81g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46L8

Quant Time: Jun 29 04:14:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 29 02:27:38 2023
Response via : Initial Calibration

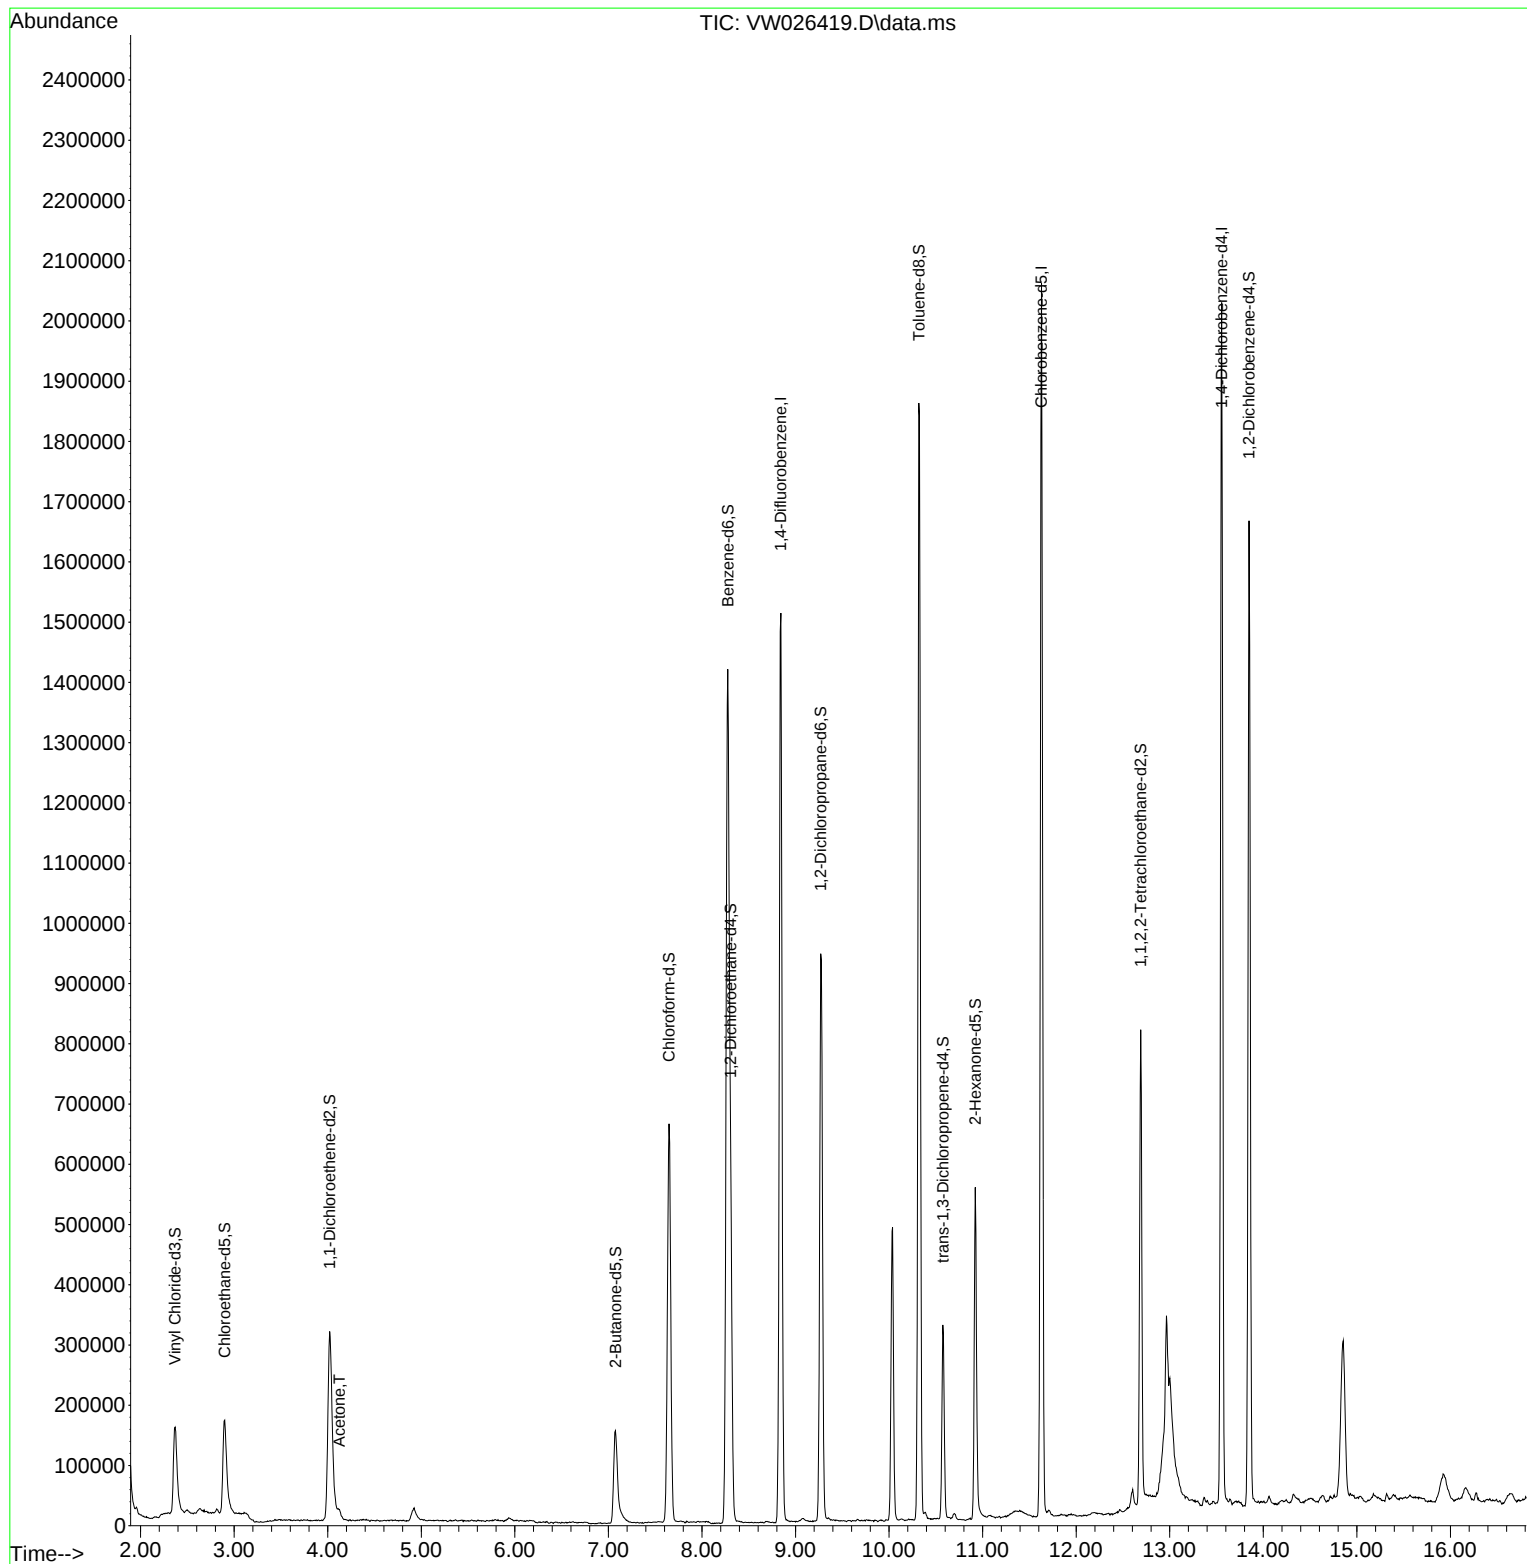

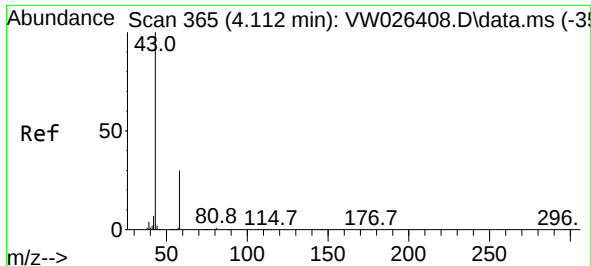

#13
 Acetone
 Concen: 5.121 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW026419.D
 Acq: 29 Jun 2023 01:36

Instrument :
 MSVOA_W
 ClientSampleId :
 A46L8

Tgt Ion: 43 Resp: 23201
 Ion Ratio Lower Upper
 43 100
 58 27.6 0.0 55.8

