

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
 Data File : VW026421.D
 Acq On : 29 Jun 2023 02:24
 Operator : SY/MD
 Sample : 03458-07
 Misc : 4.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A46M0

Quant Time: Jun 29 04:15:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 29 02:27:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1326263	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	1177386	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	546208	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	318140	16.512	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.040%
7) Chloroethane-d5	2.893	69	264291	19.296	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.200%
11) 1,1-Dichloroethene-d2	4.021	65	164297	18.835	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	75.320%
21) 2-Butanone-d5	7.075	46	264569	43.691	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.380%
24) Chloroform-d	7.648	84	751885	20.007	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.040%
26) 1,2-Dichloroethane-d4	8.307	65	427152	20.228	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.920%
32) Benzene-d6	8.276	84	1588165	21.792	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	87.160%
36) 1,2-Dichloropropane-d6	9.270	67	515513	21.769	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	87.080%
41) Toluene-d8	10.318	98	1378753	21.614	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.440%
43) trans-1,3-Dichloroprop...	10.581	79	189143	19.893	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	79.560%
47) 2-Hexanone-d5	10.922	63	173852	47.803	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.600%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	397334	21.312	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.240%
66) 1,2-Dichlorobenzene-d4	13.848	152	436066	22.929	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.720%
Target Compounds						
13) Acetone	4.118	43	17320	3.573	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062823\
Data File : VW026421.D
Acq On : 29 Jun 2023 02:24
Operator : SY/MD
Sample : 03458-07
Misc : 4.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A46M0

Quant Time: Jun 29 04:15:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 29 02:27:38 2023
Response via : Initial Calibration

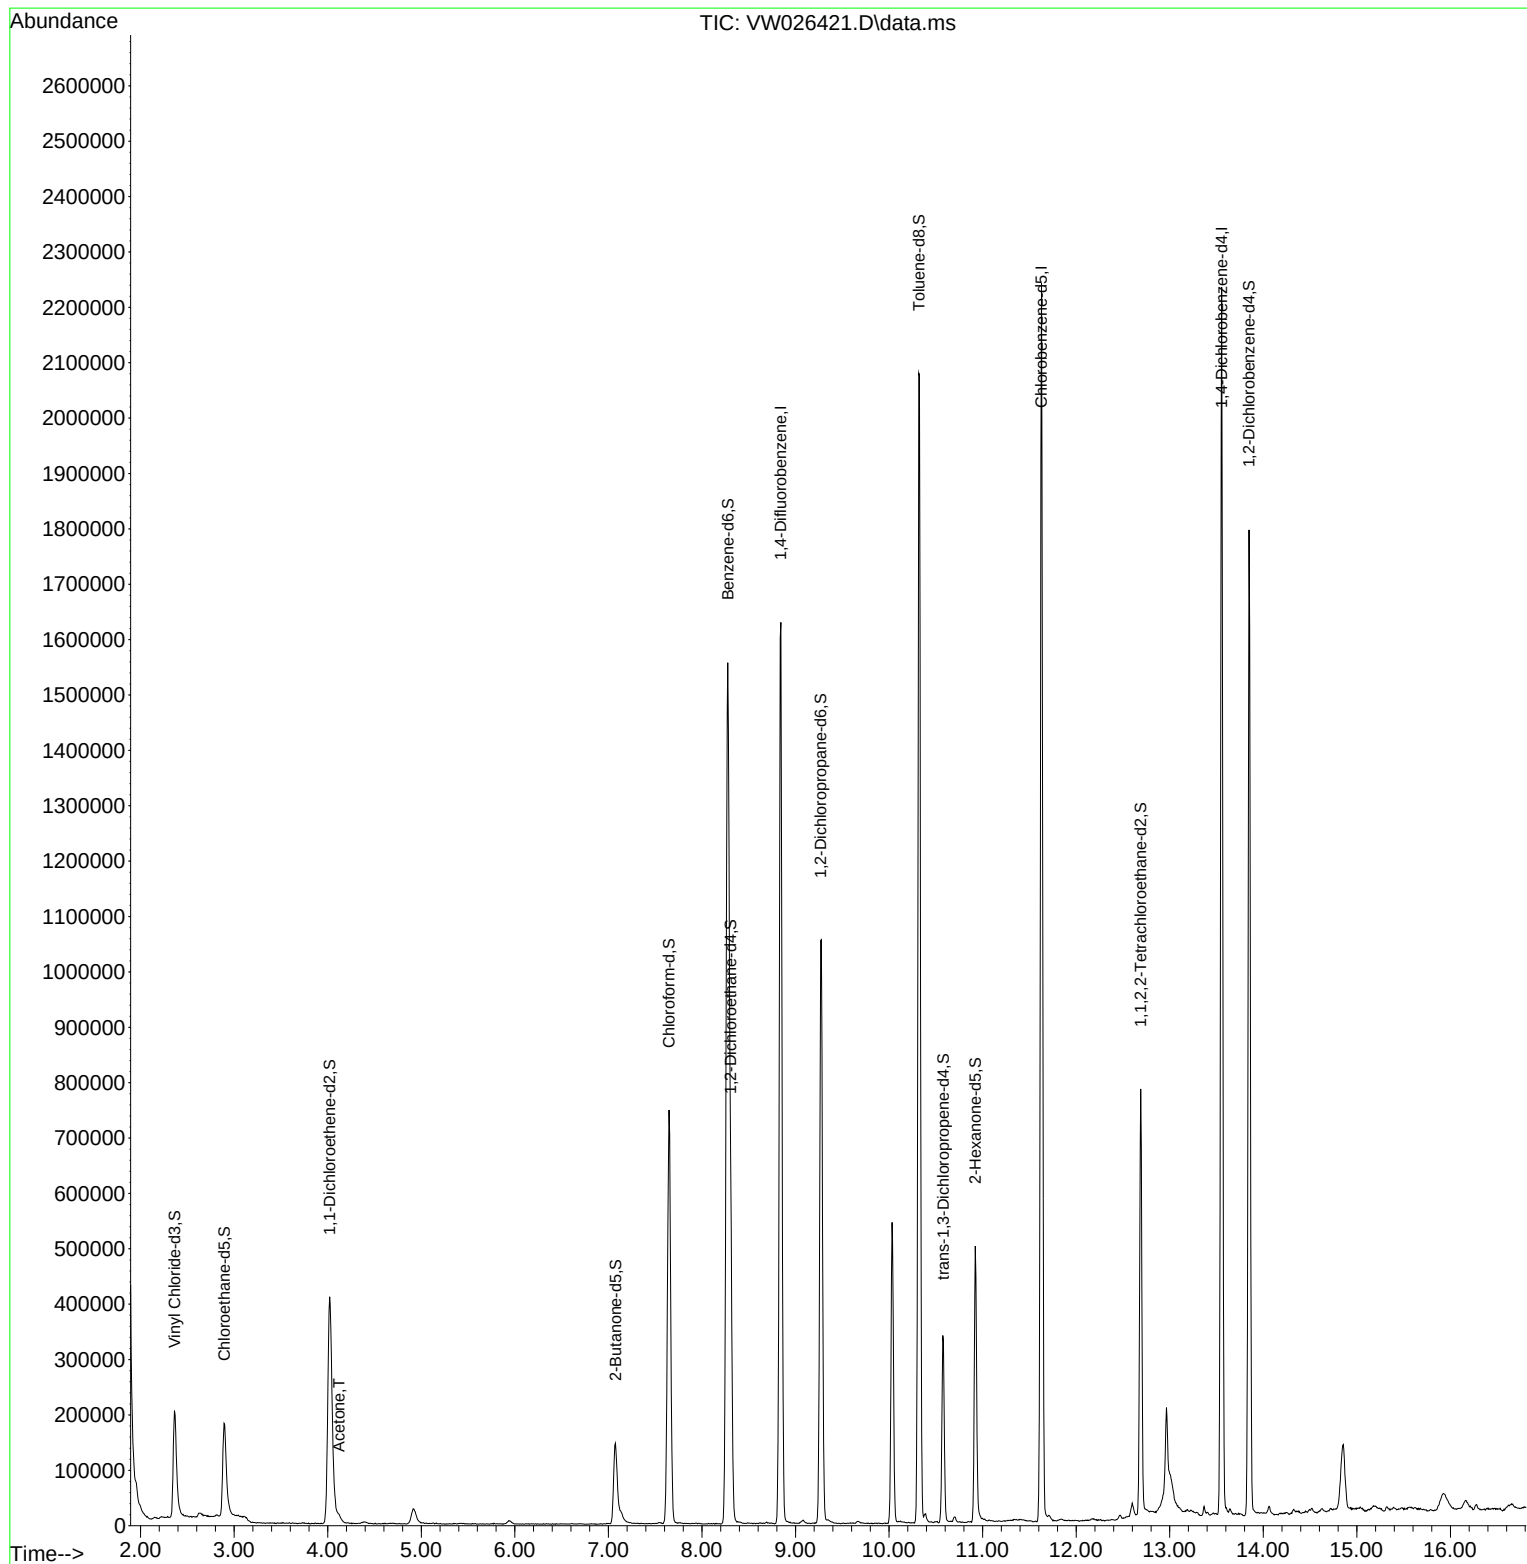

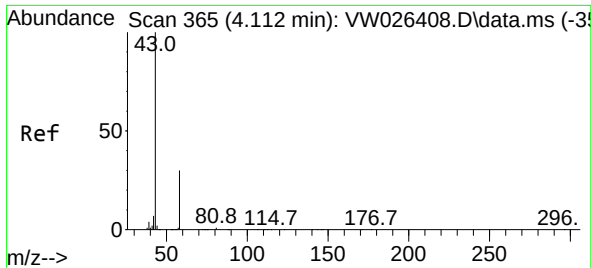

#13
 Acetone
 Concen: 3.573 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW026421.D
 Acq: 29 Jun 2023 02:24

Instrument :
 MSVOA_W
 ClientSampleId :
 A46M0

Tgt Ion: 43 Resp: 17320
 Ion Ratio Lower Upper
 43 100
 58 29.8 0.0 55.8

