

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062918\
 Data File : VW003673.D
 Acq On : 29 Jun 2018 20:43
 Operator : SY/AP
 Sample : J3774-04RE
 Misc : 5.40G/5ML/MSVOA W/SOIL
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-4(8-10)RE

Quant Time: Jun 30 03:43:36 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
 Quant Title : SW846 8260
 QLast Update : Sat Jun 16 05:18:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	0.00	168	0	0.00	ug/l	-7.95
34) 1,4-Difluorobenzene	0.00	114	0	0.00	ug/l	-8.85
63) Chlorobenzene-d5	0.00	117	0	0.00	ug/l	-11.64
72) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ug/l	-13.57

System Monitoring Compounds		R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4		0.00	65	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
35) Dibromofluoromethane		0.00	113	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
50) Toluene-d8		0.00	98	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	
62) 4-Bromofluorobenzene		0.00	95	0	0.00	ug/l	
Spiked Amount	50.000			Recovery	=	0.00%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062918\
Data File : VW003673.D
Acq On : 29 Jun 2018 20:43
Operator : SY/AP
Sample : J3774-04RE
Misc : 5.40G/5ML/MSVOA W/SOIL
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-4(8-10)RE

Quant Time: Jun 30 03:43:36 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
Quant Title : SW846 8260
QLast Update : Sat Jun 16 05:18:54 2018
Response via : Initial Calibration

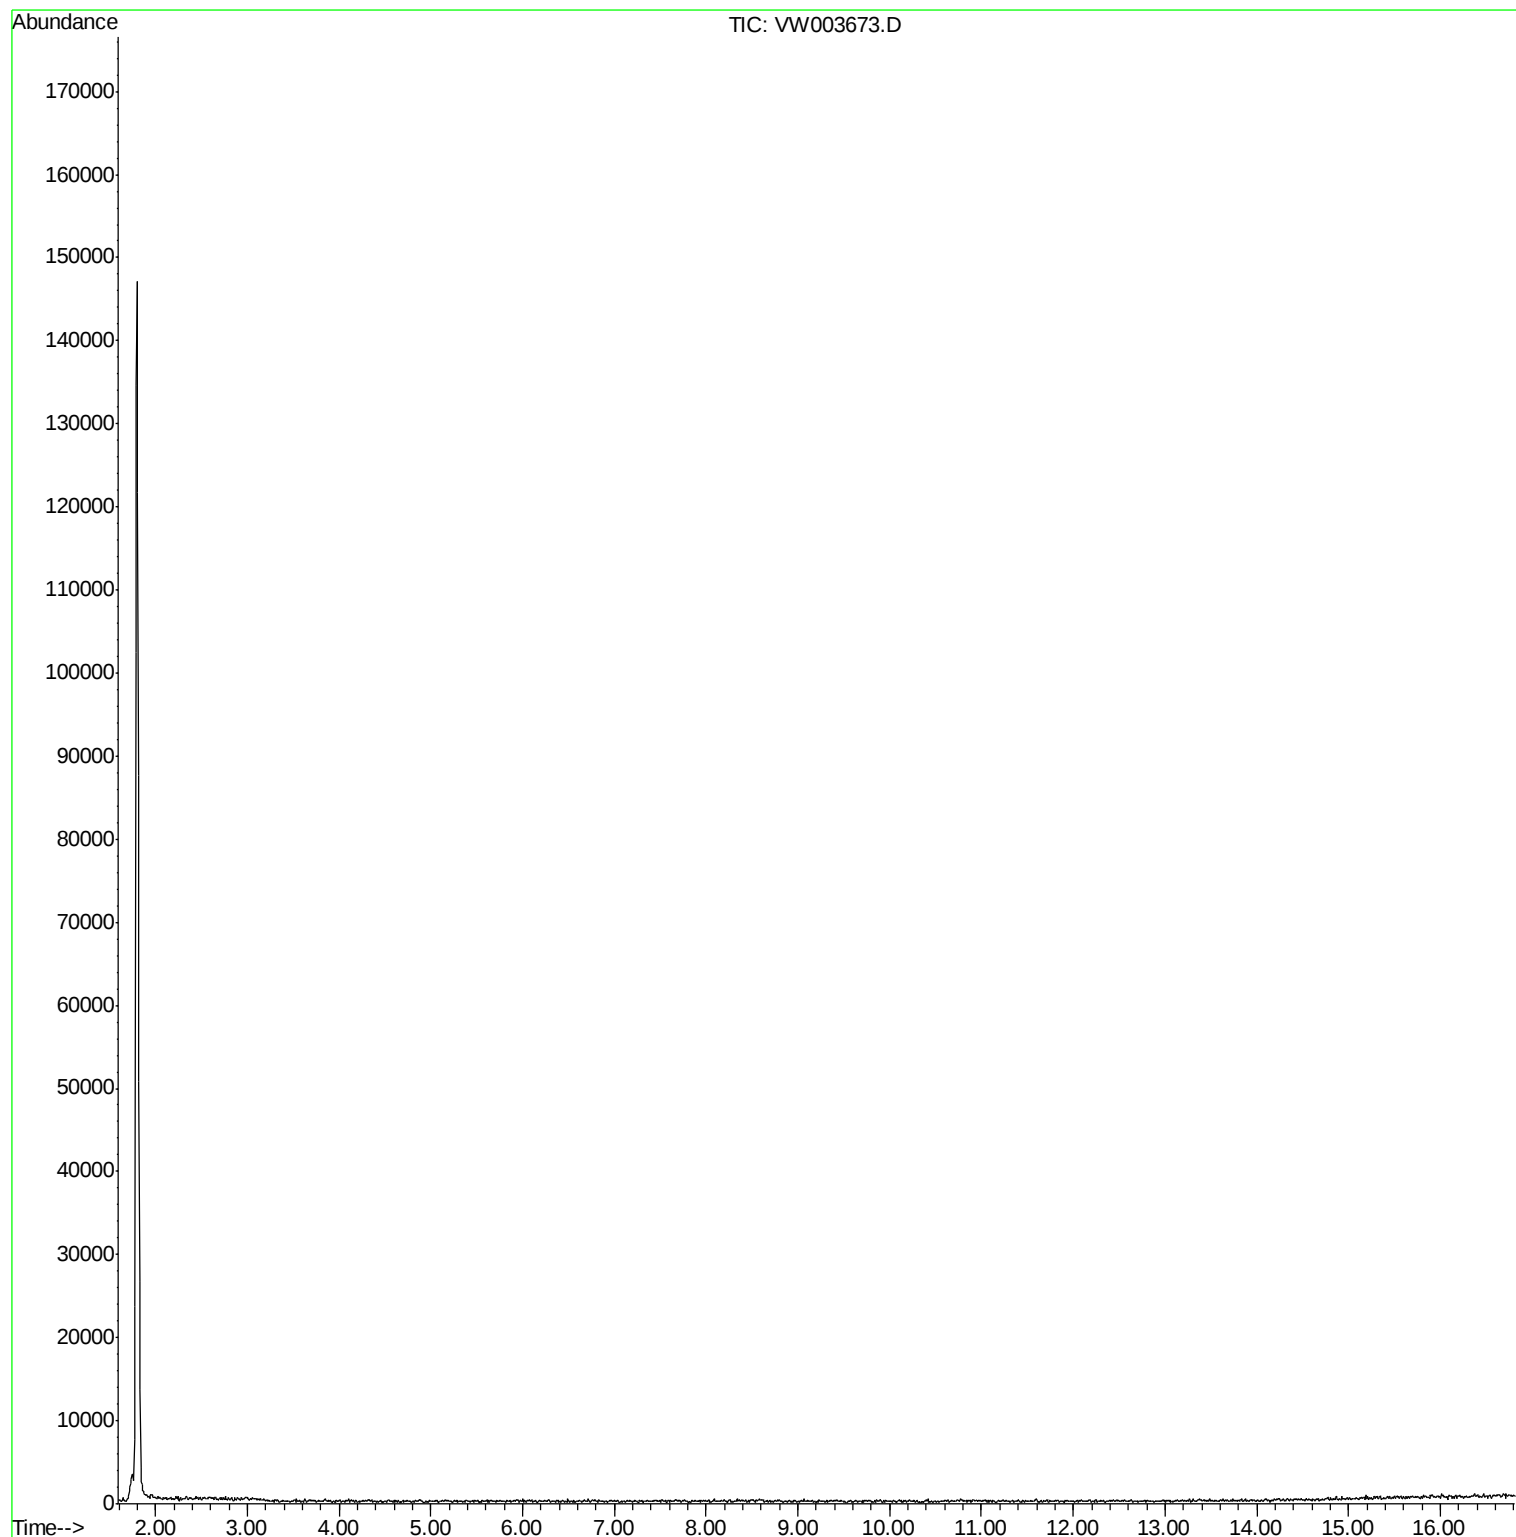

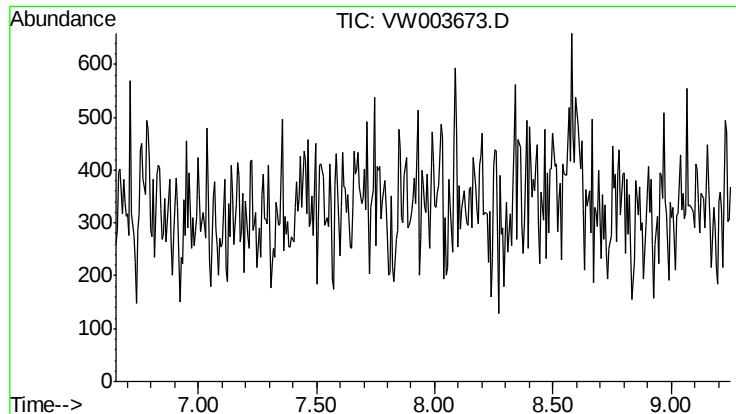

#1

Pentafluorobenzene

Concen: 0.00 ug/l

Expected RT: 7.95 min

Lab File: VW003673.D

Acq: 29 Jun 2018 20:43

Tot Ion: 168

Sig Exp Ratio

168 100



99 56.9

Instrument :

MSVOA_W

ClientSampleId :

SB-4(8-10)RE

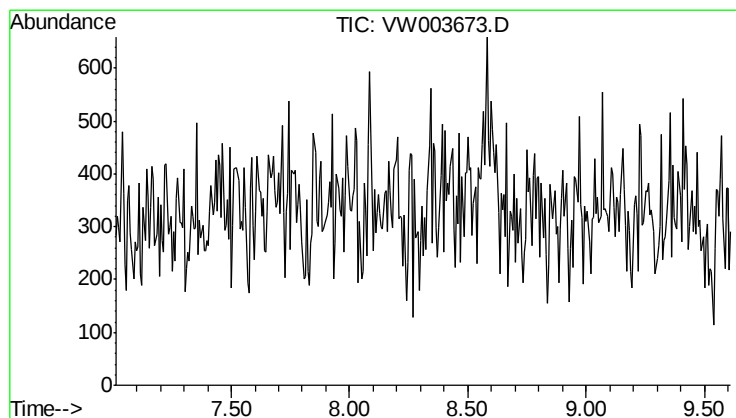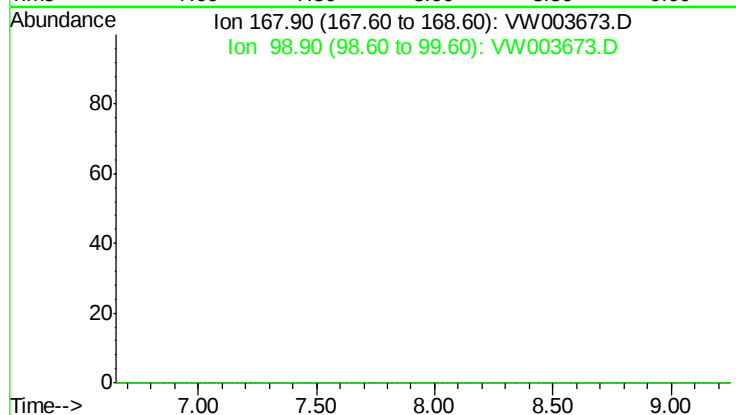

#33

1,2-Dichloroethane-d4

Concen: 0.00 ug/l

Expected RT: 8.31 min

Lab File: VW003673.D


Acq: 29 Jun 2018 20:43


Tgt Ion: 65

Sig Exp Ratio

65 100

67 52.1


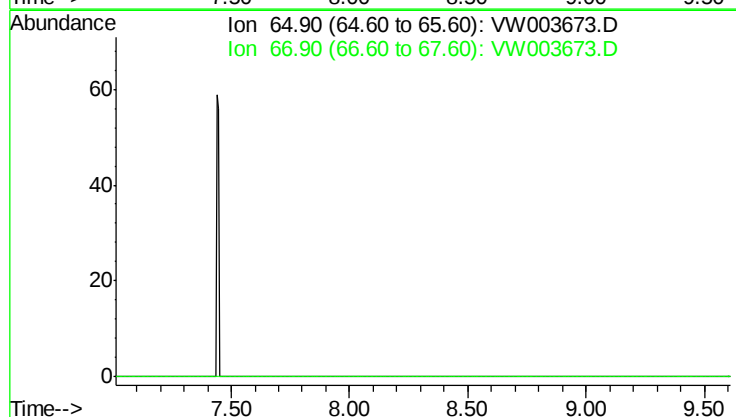


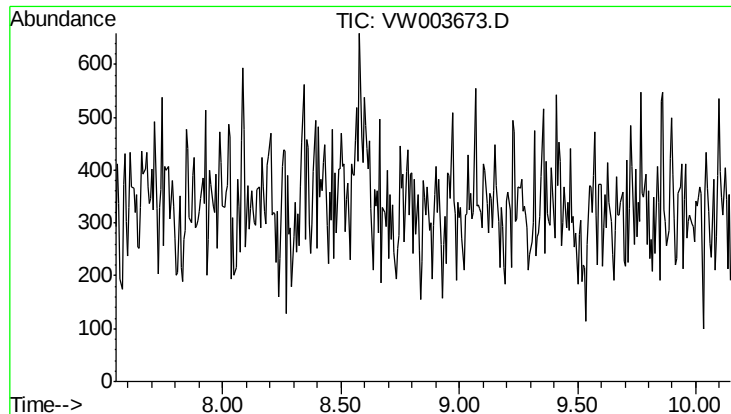

#34
 1,4-Difluorobenzene
 Concen: 0.00 ug/l
 Expected RT: 8.85 min
 Lab File: VW003673.D
 Acq: 29 Jun 2018 20:43


Instrument :
 MSVOA_W
 ClientSampleId :
 SB-4(8-10)RE


Tot Ion	114
Sig	Exp Ratio
114	100
63	21.5
88	14.8

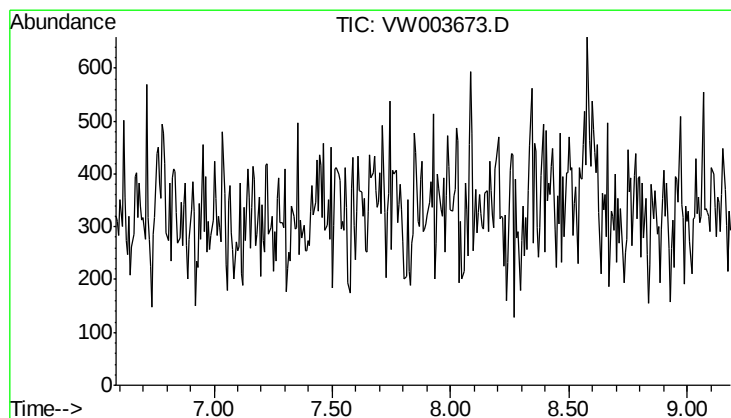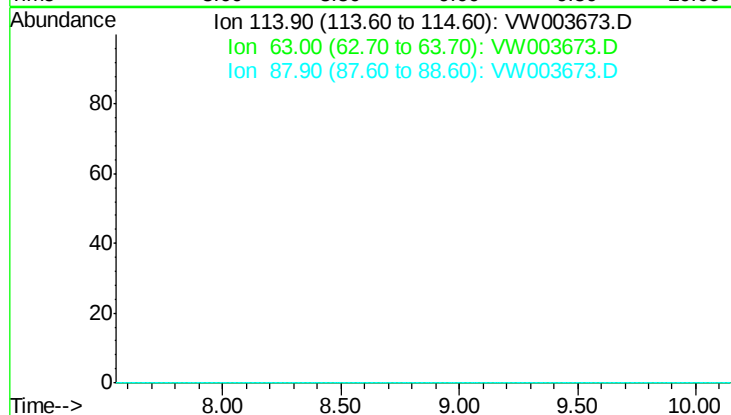

#35
 Dibromofluoromethane
 Concen: 0.00 ug/l
 Expected RT: 7.88 min
 Lab File: VW003673.D
 Acq: 29 Jun 2018 20:43

Tgt Ion	113
Sig	Exp Ratio
113	100
111	102.7
192	20.2


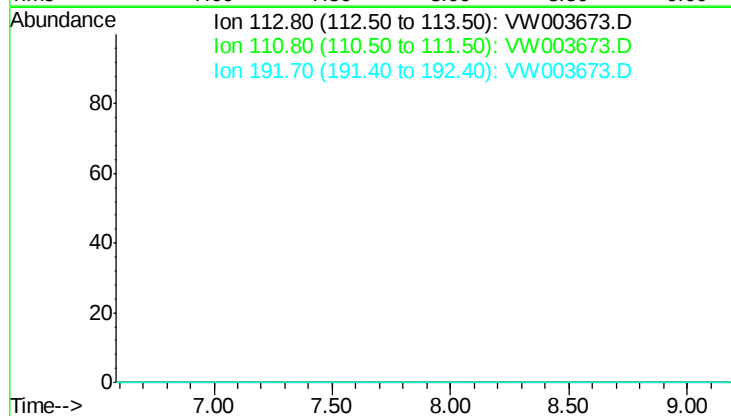


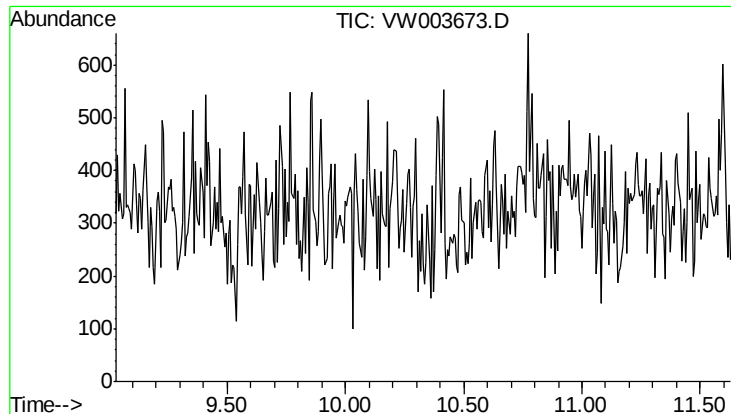

#50
Toluene-d8
Concen: 0.00 ug/l
Expected RT: 10.33 min
Lab File: VW003673.D
Acq: 29 Jun 2018 20:43


Instrument :
MSVOA_W
ClientSampleId :
SB-4(8-10)RE


Tot Ion: 98
Sig Exp Ratio
98 100
100 63.5

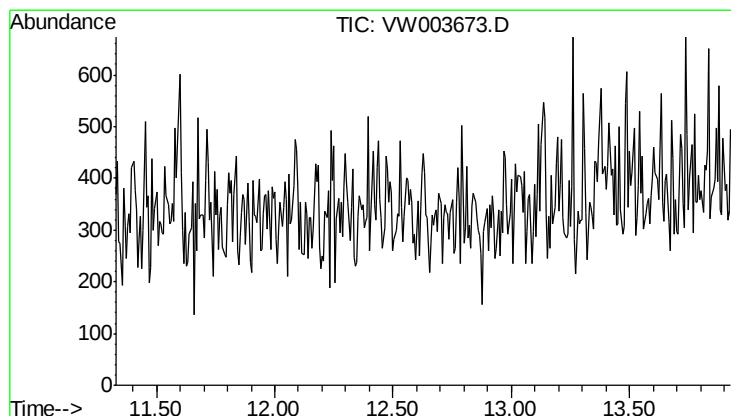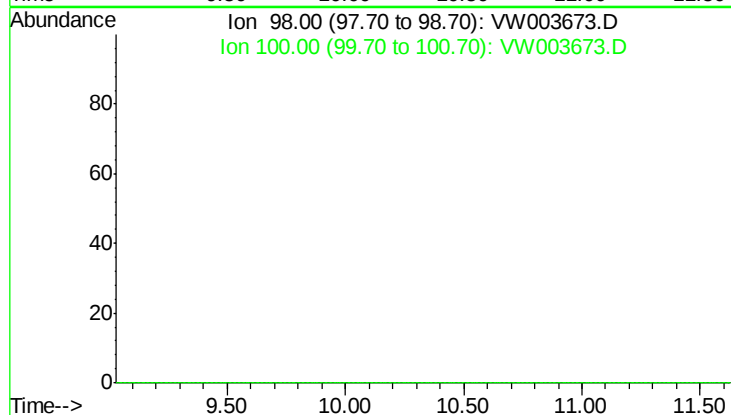

#62
4-Bromofluorobenzene
Concen: 0.00 ug/l
Expected RT: 12.63 min
Lab File: VW003673.D
Acq: 29 Jun 2018 20:43

Tgt Ion: 95
Sig Exp Ratio
95 100
174 83.2
176 81.0


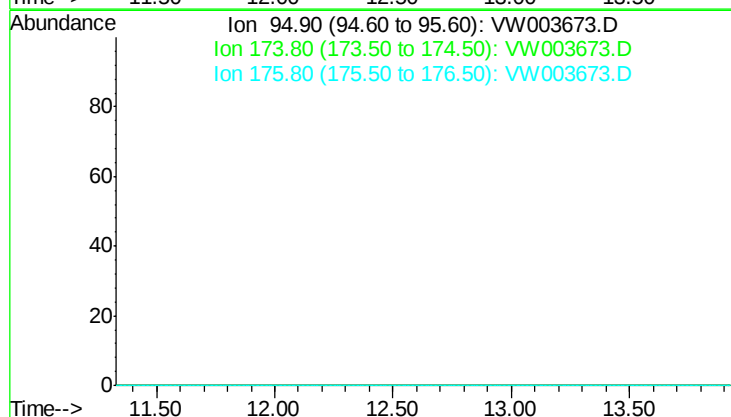


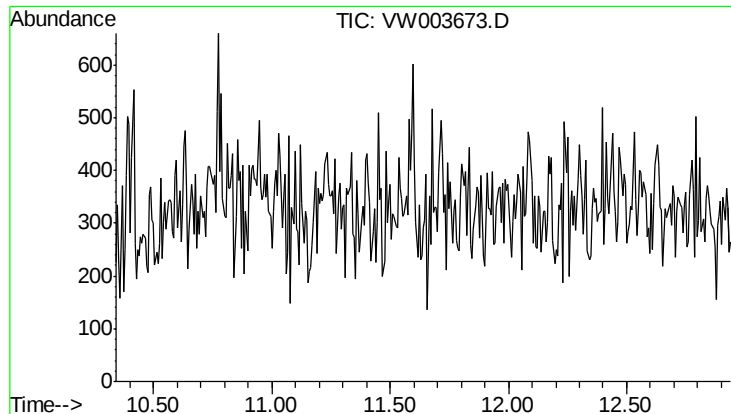

#63
Chlorobenzene-d5
Concen: 0.00 ug/l
Expected RT: 11.64 min
Lab File: VW003673.D
Acq: 29 Jun 2018 20:43

Instrument :
MSVOA_W
ClientSampleId :
SB-4(8-10)RE

Tot Ion: 117	
Sig	Exp Ratio
117	100
82	55.8
119	33.4

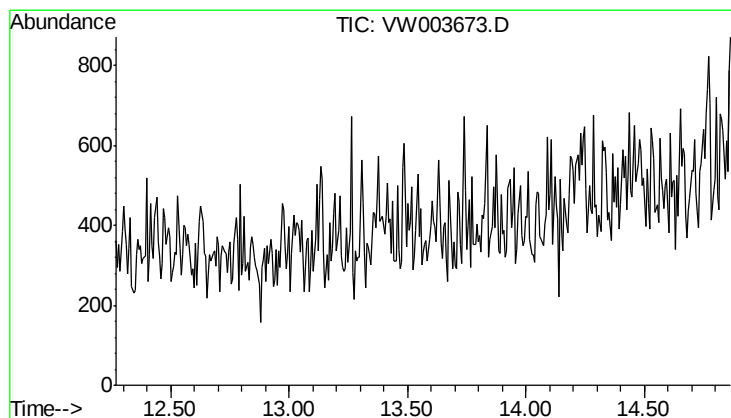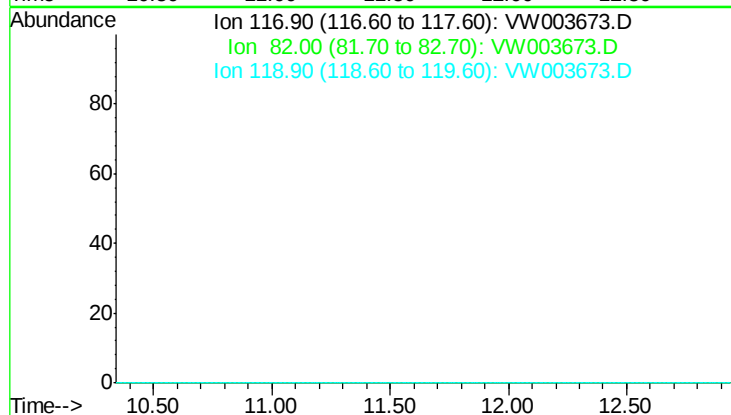

#72
1,4-Dichlorobenzene-d4
Concen: 0.00 ug/l
Expected RT: 13.57 min
Lab File: VW003673.D
Acq: 29 Jun 2018 20:43

Tgt Ion: 152	
Sig	Exp Ratio
152	100
115	58.7
150	174.8

