


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062918\
Data File : VW003653.D
Acq On : 29 Jun 2018 11:34
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
Title : SW846 8260
Last Update : Sat Jun 16 05:18:54 2018

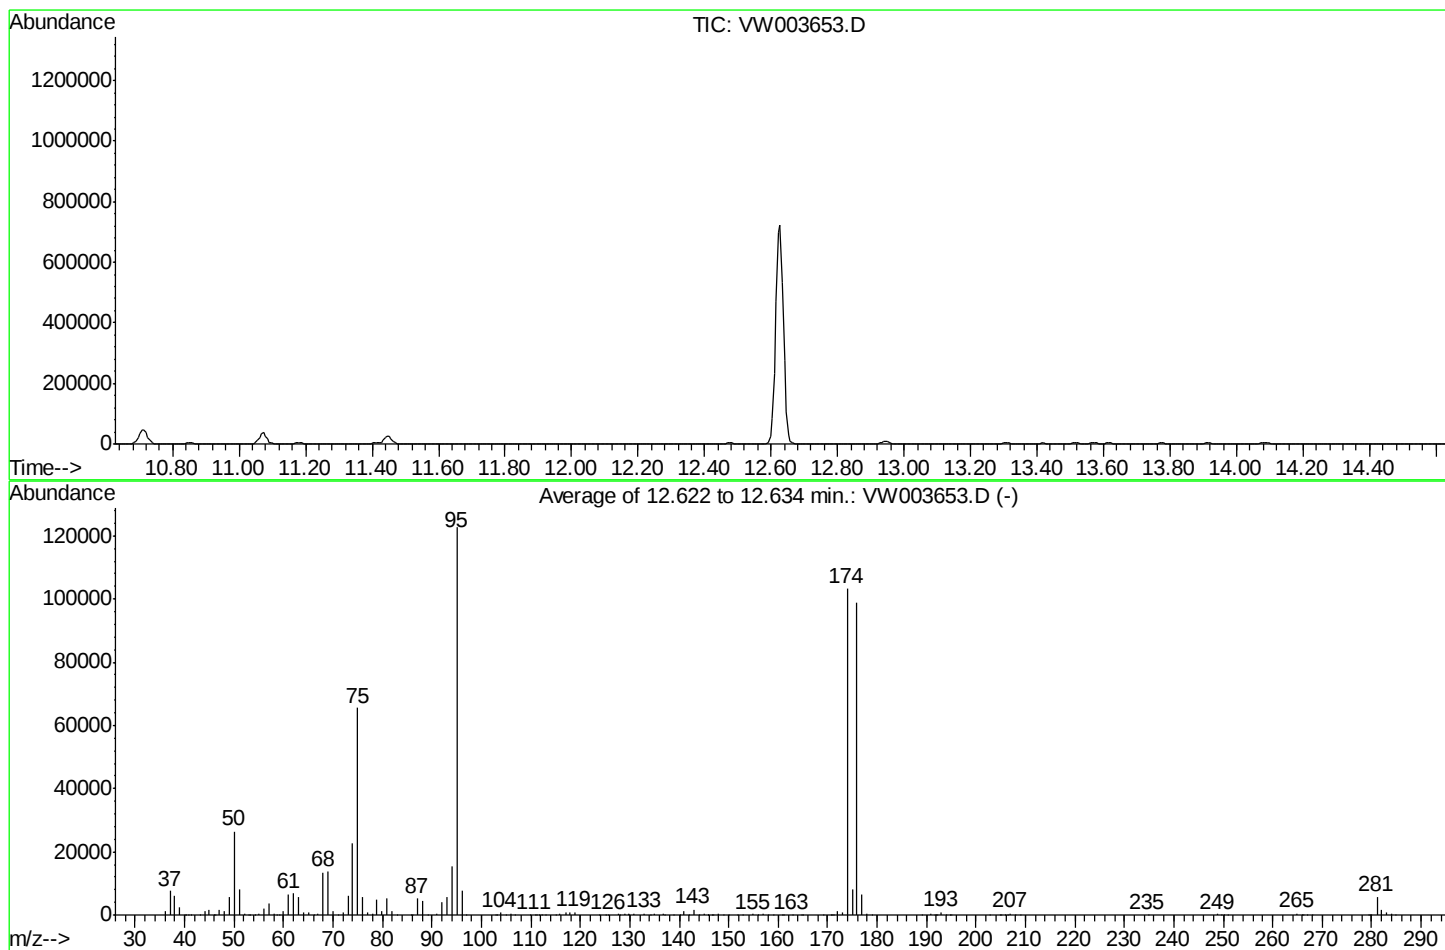

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	26362	PASS
75	95	30	60	53.3	65434	PASS
95	95	100	100	100.0	122674	PASS
96	95	5	9	6.3	7760	PASS
173	174	0.00	2	0.7	746	PASS
174	95	50	100	84.1	103128	PASS
175	174	5	9	8.0	8254	PASS
176	174	95	101	95.8	98821	PASS
177	176	5	9	6.7	6641	PASS