

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062919\
 Data File : VW011057.D
 Acq On : 28 Jun 2019 13:25
 Operator : SY/VA
 Sample : K3552-10
 Misc : 5.08G/5ML/MSVOA W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 M-5A

Quant Time: Jun 29 02:18:02 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 01:55:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	191853	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	328035	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	276805	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	116586	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	123470	49.23	ug/l	0.00
Spiked Amount			Recovery	=	98.46%	
35) Dibromofluoromethane	7.88	113	97331	48.59	ug/l	0.00
Spiked Amount			Recovery	=	97.18%	
50) Toluene-d8	10.32	98	409514	49.67	ug/l	0.00
Spiked Amount			Recovery	=	99.34%	
62) 4-Bromofluorobenzene	12.62	95	131946	43.75	ug/l	0.00
Spiked Amount			Recovery	=	87.50%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062919\
Data File : VW011057.D
Acq On : 28 Jun 2019 13:25
Operator : SY/VA
Sample : K3552-10
Misc : 5.08G/5ML/MSVOA W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
M-5A

Quant Time: Jun 29 02:18:02 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 01:55:46 2019
Response via : Initial Calibration

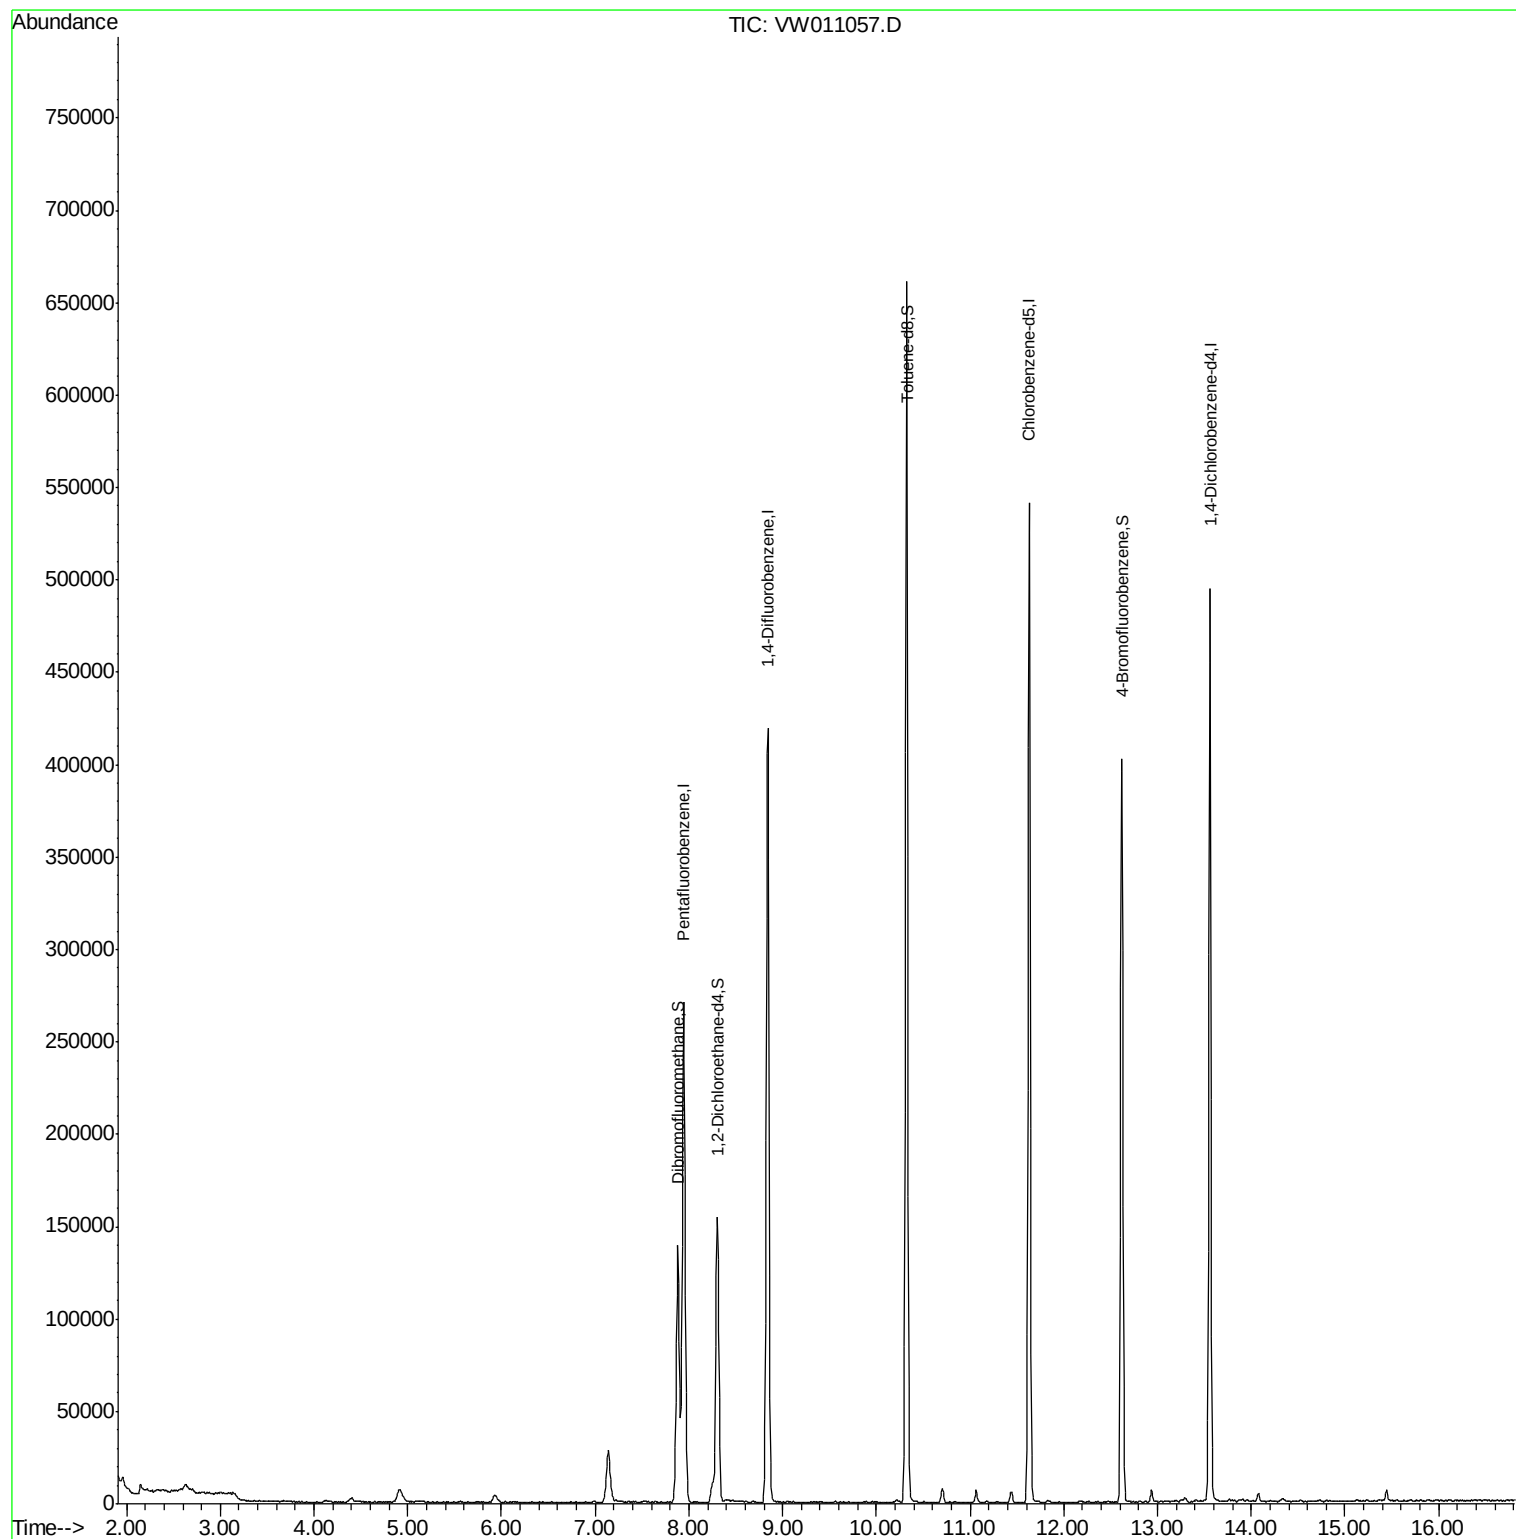

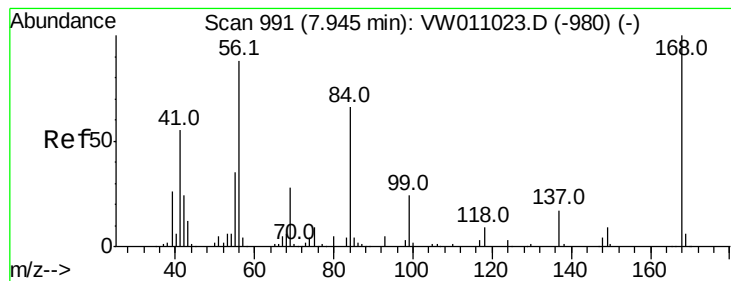

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011057.D

Acq: 28 Jun 2019 13:25

Instrument :

MSVOA_W

ClientSampleId :


M-5A

Tot Ion:168 Resp: 191853

Ion Ratio Lower Upper

168 100

99 62.4 47.8 71.6

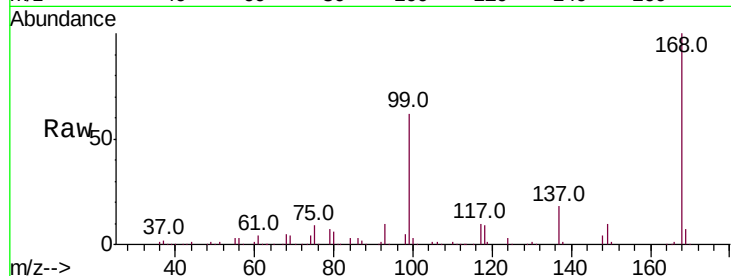

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

100000

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

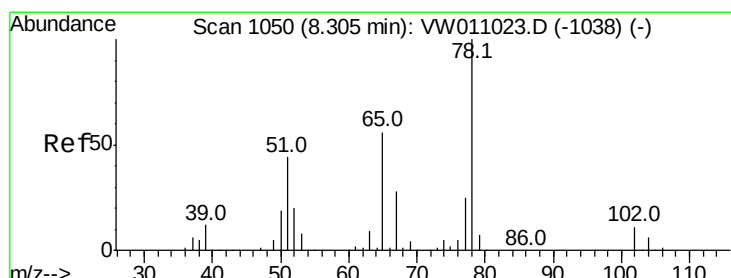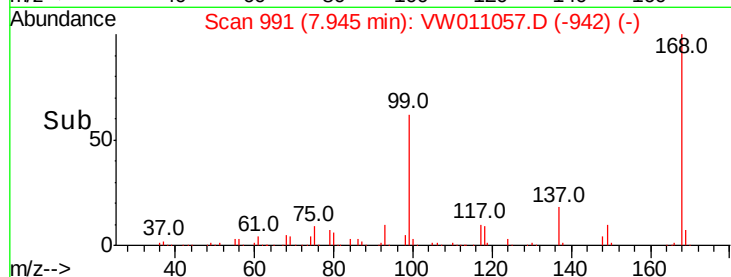

#33

1,2-Dichloroethane-d4

Concen: 49.230 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW011057.D


Acq: 28 Jun 2019 13:25

Tgt Ion: 65 Resp: 123470

Ion Ratio Lower Upper

65 100

67 51.2 0.0 102.4

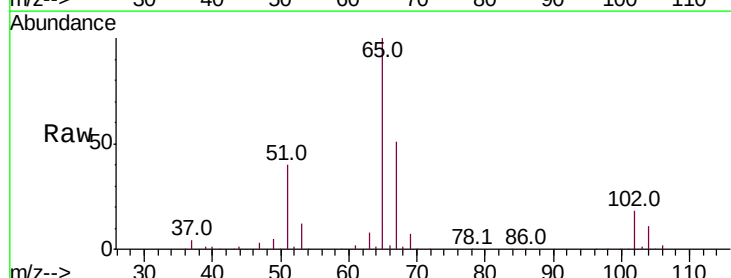

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

60000

50000

40000


30000


20000

10000

0

Time--> 8.20 8.30 8.40




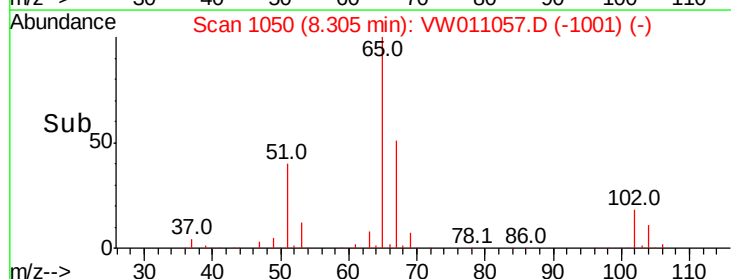


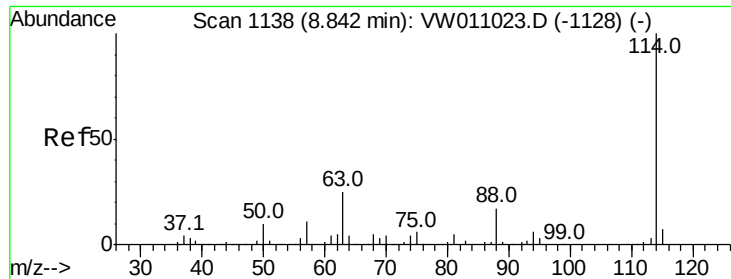

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW011057.D
 Acq: 28 Jun 2019 13:25




Instrument :
 MSVOA_W
 ClientSampleId :
 M-5A


Tot Ion	Ratio	Lower	Upper
114	100		
63	24.9	0.0	50.6
88	16.9	0.0	34.0

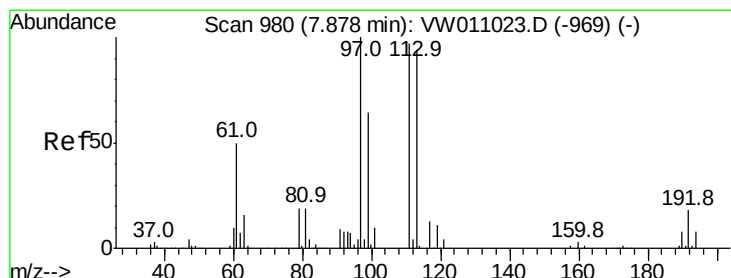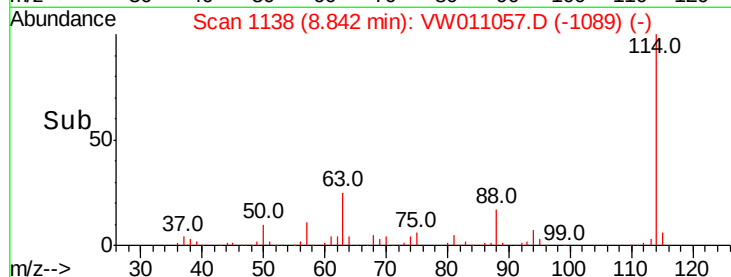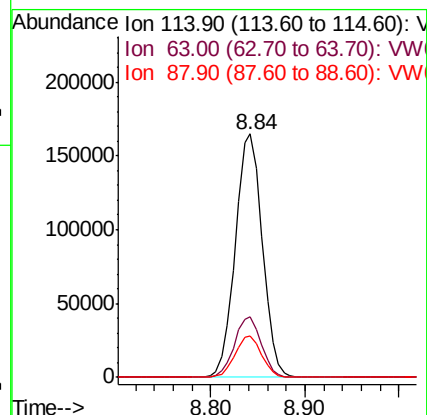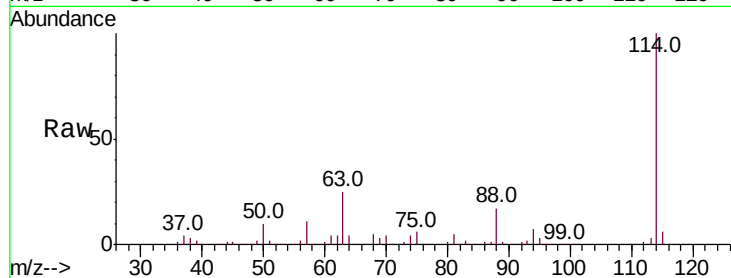

#35
 Dibromofluoromethane
 Concen: 48.590 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.01 min
 Lab File: VW011057.D
 Acq: 28 Jun 2019 13:25

Tgt Ion	Ratio	Lower	Upper
113	100		
111	102.8	83.8	125.6
192	19.6	16.0	24.0


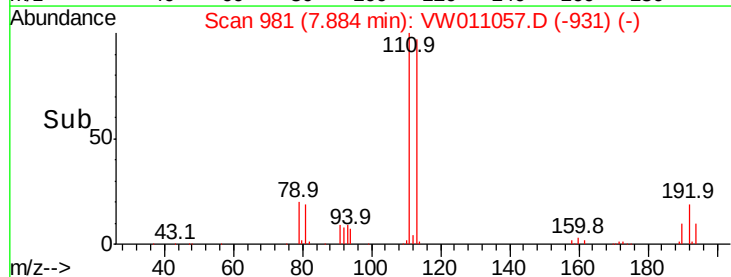
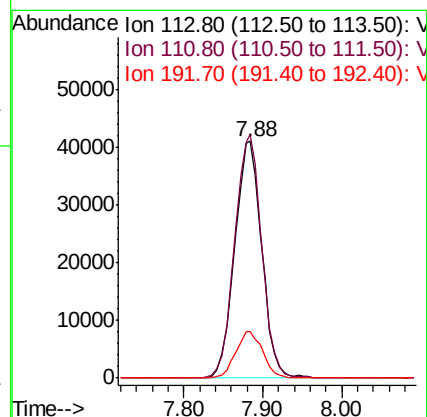
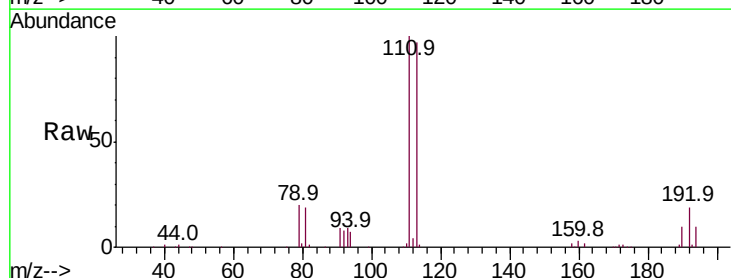


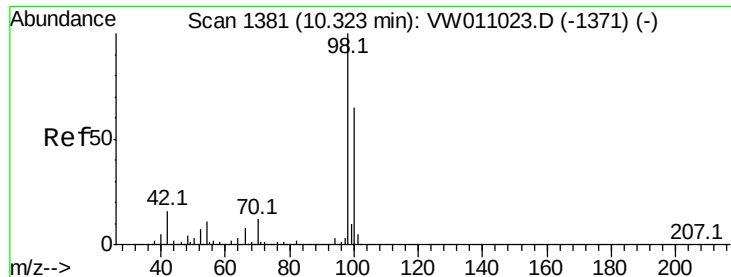

#50
Toluene-d8
Concen: 49.666 ug/l
RT: 10.32 min Scan# 1381
Delta R.T. 0.00 min
Lab File: VW011057.D
Acq: 28 Jun 2019 13:25




Instrument :
MSVOA_W
ClientSampled :
M-5A


Tot Ion: 98 Resp: 409514
Ion Ratio Lower Upper
98 100
100 65.1 52.3 78.5

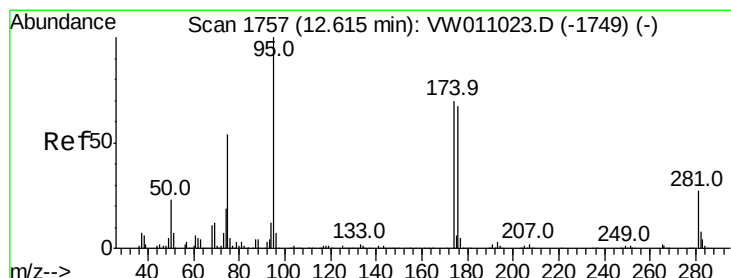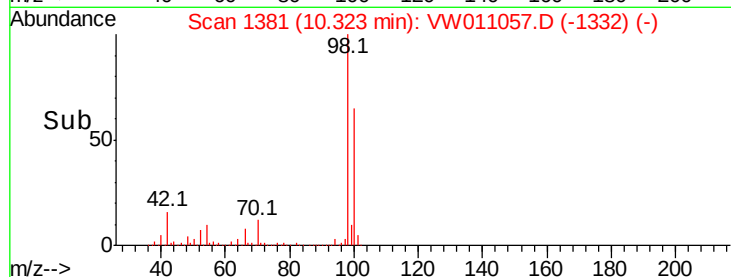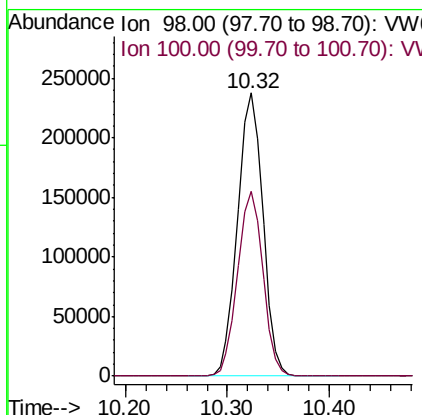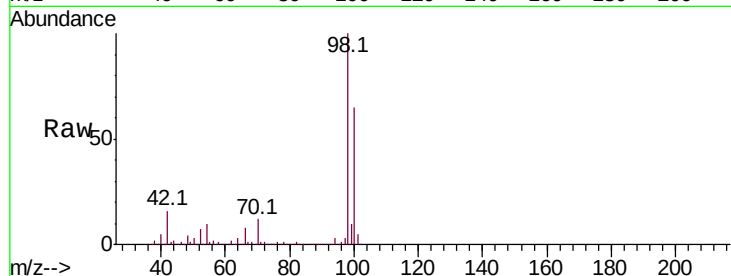

#62
4-Bromofluorobenzene
Concen: 43.752 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. 0.01 min
Lab File: VW011057.D
Acq: 28 Jun 2019 13:25

Tgt Ion: 95 Resp: 131946
Ion Ratio Lower Upper
95 100
174 74.0 0.0 149.2
176 70.6 0.0 143.6

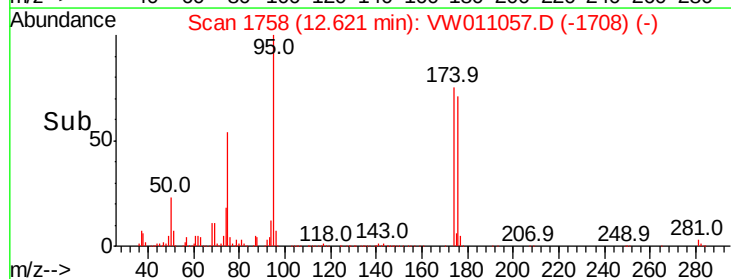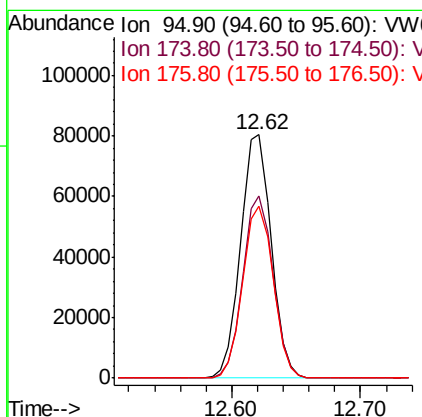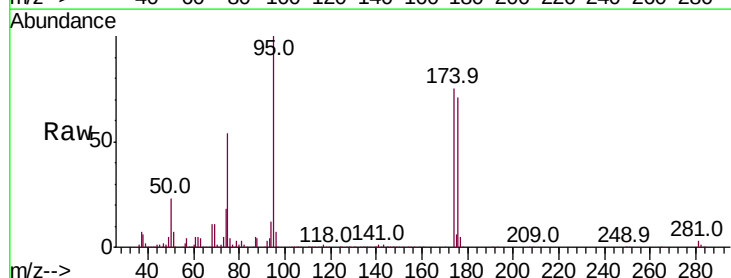


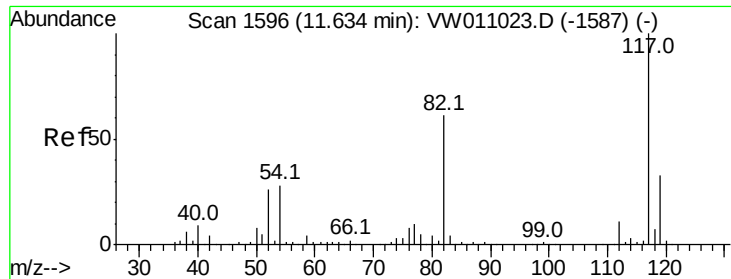




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW011057.D
Acq: 28 Jun 2019 13:25

Instrument :
MSVOA_W
ClientSampled :
M-5A

Tot Ion:117 Resp: 276805
Ion Ratio Lower Upper
117 100
82 58.8 48.6 73.0
119 31.4 26.1 39.1

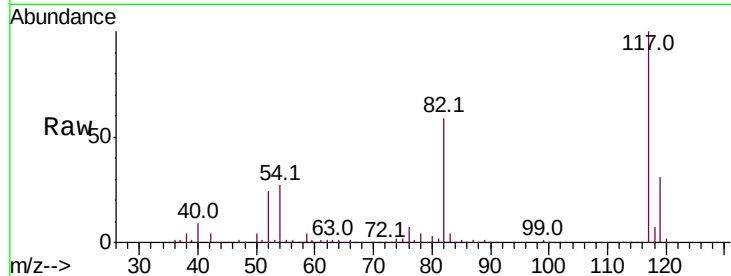


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VV
Ion 118.90 (118.60 to 119.60): V

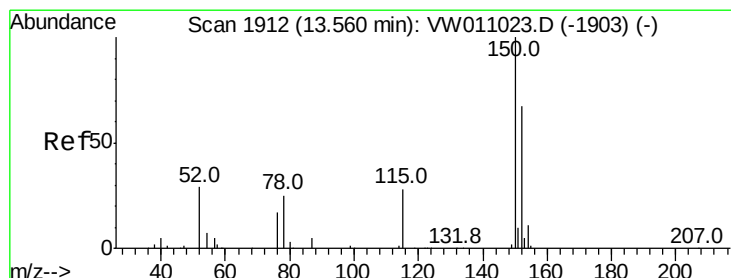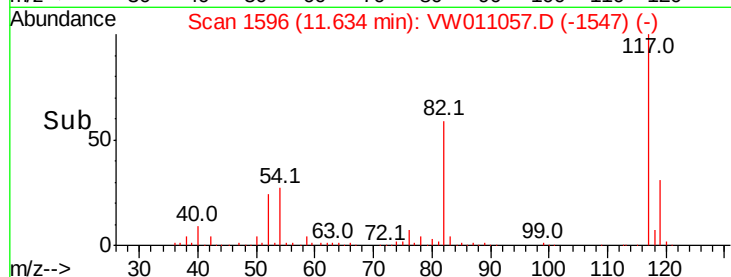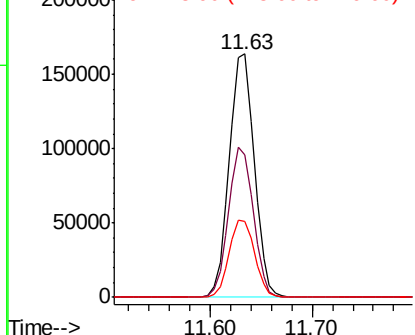

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW011057.D
Acq: 28 Jun 2019 13:25

Tgt Ion:152 Resp: 116586
Ion Ratio Lower Upper
152 100
115 61.6 30.7 92.1
150 158.8 0.0 341.8

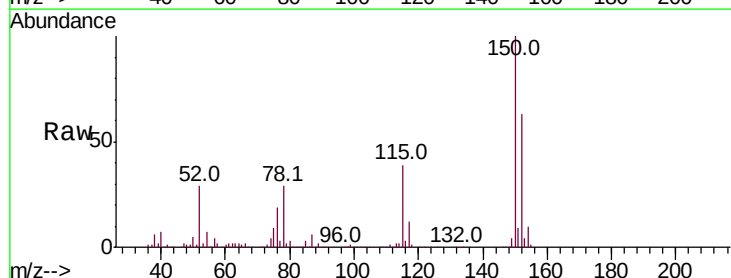

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

