


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062919\
 Data File : VW011049.D
 Acq On : 28 Jun 2019 09:21
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
 Title : SW846 8260
 Last Update : Fri Jun 28 01:55:46 2019

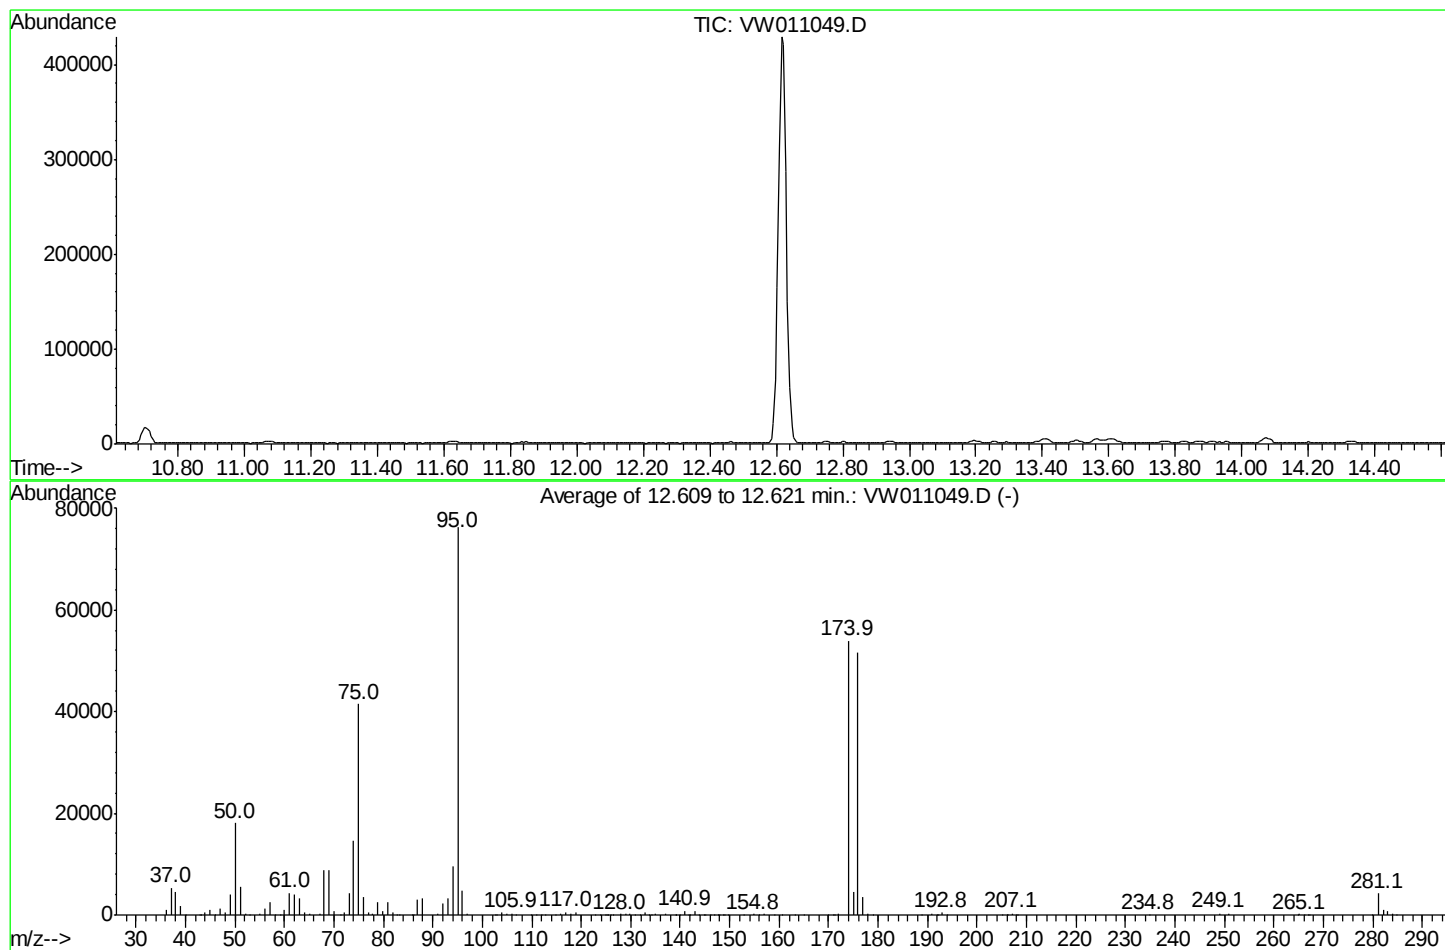

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	18028	PASS
75	95	30	60	54.4	41469	PASS
95	95	100	100	100.0	76218	PASS
96	95	5	9	6.3	4817	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.7	53856	PASS
175	174	5	9	8.3	4467	PASS
176	174	95	101	95.6	51480	PASS
177	176	5	9	6.9	3574	PASS