


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062920\
 Data File : VW015750.D
 Acq On : 29 Jun 2020 08:39
 Operator : SY/VA
 Sample : BFB14
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB14

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062920S.M
 Title : VOC Analysis
 Last Update : Wed Jul 01 01:40:19 2020

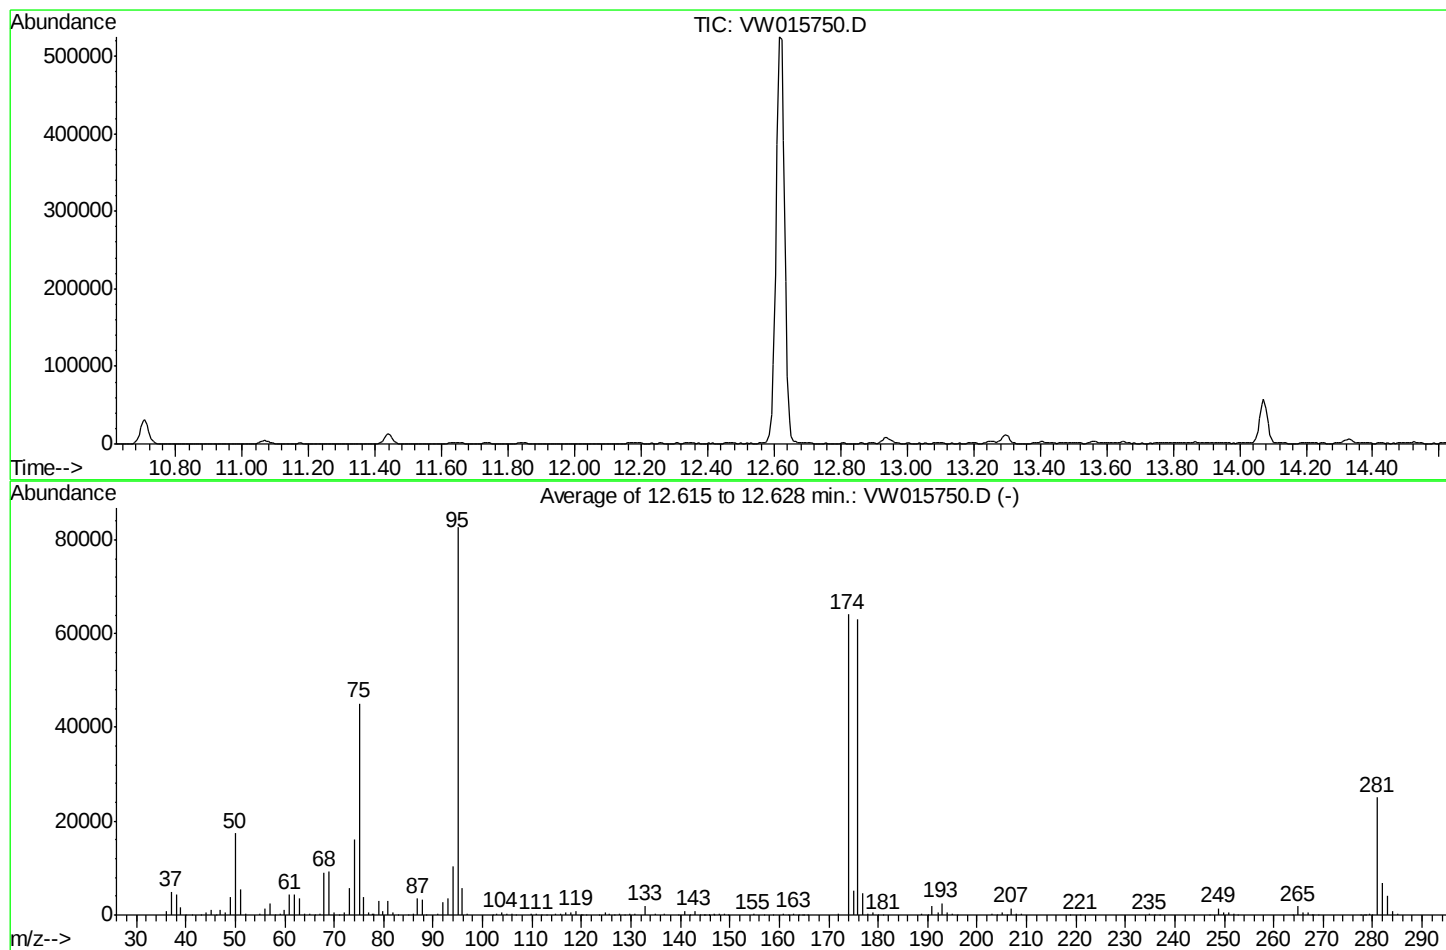

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	17402	PASS
75	95	30	80	54.6	45138	PASS
95	95	100	100	100.0	82656	PASS
96	95	5	9	6.8	5612	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.4	64010	PASS
175	174	5	9	8.0	5125	PASS
176	174	95	101	98.4	63010	PASS
177	176	5	9	7.4	4661	PASS

m/z	Abundance
36.00	1256.0
37.00	5530.0
38.00	4915.0
39.00	1804.0
39.90	253.0
41.20	75.0
42.90	223.0
44.00	907.0
45.00	1395.0
46.00	175.0
47.00	1140.0
47.90	718.0
49.00	4215.0
50.00	18664.0
51.00	5951.0
52.10	260.0
55.00	359.0
56.00	1618.0
57.00	2823.0
57.90	98.0
58.90	626.0
60.00	1093.0
61.00	4656.0
62.00	4543.0
63.00	3750.0
64.00	474.0
65.00	297.0
66.00	72.0
67.00	297.0
68.00	9733.0
69.00	10244.0
70.10	631.0
71.00	113.0
71.90	557.0
73.00	7351.0
74.00	17360.0
75.00	48496.0
76.00	4166.0
77.00	582.0
78.10	356.0
78.90	3134.0
79.90	931.0
80.90	3316.0
81.90	721.0
83.00	110.0
84.90	90.0
86.00	169.0
86.90	3933.0
87.90	3374.0
88.70	291.0
91.00	390.0
92.00	2546.0
93.00	3754.0
94.00	10704.0
95.00	84680.0
96.00	5852.0
96.90	223.0
101.90	63.0
102.80	634.0
103.90	547.0
105.00	230.0
105.90	406.0
106.70	188.0
110.00	276.0
111.00	227.0
111.80	140.0
113.00	141.0
114.90	350.0
115.90	328.0
116.90	779.0
117.90	717.0
119.00	1016.0
119.90	97.0
120.90	79.0
123.70	54.0
125.00	943.0
125.70	341.0
126.70	72.0
127.80	339.0
128.80	164.0
129.80	269.0
130.90	215.0
133.00	3510.0
134.90	463.0
136.80	196.0
139.70	102.0
140.90	812.0
142.00	155.0
142.90	945.0
144.70	137.0
145.10	103.0
145.70	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

147.00	382.0
147.90	282.0
148.90	204.0
149.90	124.0
154.80	213.0
156.90	129.0
158.80	114.0
160.90	262.0
161.80	86.0
162.90	428.0
163.90	128.0
164.80	427.0
165.80	95.0
171.90	427.0
173.90	61008.0
175.00	5479.0
175.90	59312.0
176.90	5054.0
177.90	388.0
178.90	753.0
180.00	211.0
181.10	105.0
188.90	313.0
190.10	194.0
190.90	2709.0
192.00	616.0
192.90	3806.0
193.90	822.0
194.90	491.0
195.90	68.0
202.90	389.0
204.00	97.0
204.90	741.0
206.00	164.0
207.00	2208.0
208.10	499.0
209.10	257.0
218.90	97.0
220.90	128.0
234.90	298.0
235.80	92.0
237.00	105.0
246.90	70.0
248.90	2277.0
250.00	797.0
250.90	1079.0
251.80	243.0
252.90	167.0
265.00	2837.0
266.00	824.0
266.90	734.0
267.80	184.0
269.00	60.0
277.50	99.0
278.70	280.0
279.30	284.0
281.00	38360.0
282.00	11411.0
283.00	6208.0
283.90	1390.0
285.00	549.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

m/z	Abundance
36.00	928.0
37.00	5409.0
38.00	4878.0
39.00	1884.0
39.90	221.0
41.10	114.0
43.20	152.0
43.90	866.0
45.00	1156.0
46.10	89.0
46.90	1077.0
47.90	585.0
49.00	4428.0
50.00	19664.0
51.00	6121.0
52.00	373.0
54.90	384.0
55.90	1585.0
57.00	2861.0
58.00	136.0
59.00	324.0
59.90	1005.0
61.00	4890.0
62.00	5166.0
63.00	3748.0
64.00	380.0
65.00	248.0
67.00	355.0
68.00	9664.0
69.00	10180.0
70.00	788.0
72.00	609.0
73.00	5960.0
74.00	17888.0
75.00	49104.0
76.00	4207.0
76.90	575.0
77.80	448.0
78.90	3138.0
79.90	1040.0
80.90	3539.0
81.90	775.0
82.90	126.0
84.90	53.0
85.90	159.0
86.90	3782.0
87.90	3429.0
90.80	427.0
92.00	2932.0
93.00	3877.0
94.00	11657.0
95.00	92264.0
96.00	6320.0
96.90	230.0
102.00	73.0
102.90	387.0
103.80	574.0
104.90	168.0
105.80	397.0
106.80	125.0
109.80	203.0
110.80	200.0
111.90	156.0
113.00	77.0
114.80	260.0
115.80	397.0
116.90	722.0
117.90	614.0
118.90	935.0
120.10	51.0
120.90	67.0
123.60	81.0
125.00	535.0
125.70	211.0
126.70	54.0
127.90	330.0
128.80	131.0
129.80	287.0
130.90	175.0
132.90	1850.0
134.70	282.0
136.90	165.0
140.90	1012.0
142.00	151.0
142.90	995.0
144.00	58.0
145.00	155.0
145.90	163.0
146.70	273.0
147.90	257.0
148.90	182.0
149.80	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

154.80	260.0
156.80	174.0
158.90	162.0
160.80	244.0
161.80	106.0
162.90	280.0
165.00	212.0
165.80	63.0
171.90	336.0
173.90	71120.0
174.90	5520.0
175.90	70440.0
176.90	4924.0
177.90	366.0
178.90	426.0
180.10	84.0
188.80	137.0
189.90	74.0
191.00	1895.0
192.00	477.0
192.90	2548.0
193.90	533.0
194.90	305.0
202.90	245.0
204.10	62.0
205.00	514.0
206.00	155.0
207.00	1583.0
208.00	296.0
209.00	157.0
220.90	98.0
234.90	254.0
235.80	89.0
247.00	52.0
248.90	1322.0
249.90	392.0
250.90	620.0
251.80	198.0
252.80	109.0
263.70	54.0
264.90	1644.0
265.90	417.0
267.00	533.0
268.00	66.0
269.00	63.0
277.50	76.0
278.20	67.0
279.20	181.0
280.90	24288.0
282.00	6972.0
283.00	4479.0
284.00	782.0
284.90	268.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

m/z	Abundance
36.00	881.0
37.00	4129.0
38.00	3432.0
39.00	1568.0
39.90	200.0
40.90	125.0
43.10	120.0
44.00	640.0
45.00	847.0
46.00	102.0
47.00	805.0
48.00	463.0
48.90	3092.0
50.00	13878.0
51.00	4626.0
52.00	218.0
54.90	243.0
55.90	1104.0
57.00	2124.0
58.00	111.0
59.00	141.0
59.90	811.0
61.00	3416.0
62.00	3498.0
63.00	2982.0
63.90	332.0
65.00	213.0
67.00	273.0
68.00	7825.0
69.00	7637.0
70.00	571.0
72.00	406.0
73.00	4270.0
74.00	13154.0
75.00	37816.0
76.00	3224.0
76.90	521.0
78.00	318.0
78.90	2440.0
79.90	611.0
80.90	2454.0
81.90	556.0
82.90	79.0
86.00	184.0
86.90	2813.0
87.90	2856.0
90.90	302.0
91.90	2389.0
92.90	3017.0
94.00	8886.0
95.00	71024.0
95.90	4666.0
96.90	121.0
102.90	162.0
103.90	391.0
104.80	179.0
105.80	352.0
106.60	114.0
109.90	76.0
110.80	104.0
111.80	68.0
112.90	96.0
114.90	105.0
115.80	300.0
116.90	558.0
117.80	411.0
118.80	552.0
124.80	244.0
125.60	97.0
127.70	274.0
128.70	107.0
129.80	344.0
130.80	111.0
133.00	957.0
134.90	180.0
136.90	148.0
140.80	679.0
141.90	96.0
142.90	858.0
143.90	55.0
144.90	98.0
145.90	134.0
146.90	173.0
147.90	152.0
148.70	65.0
149.00	69.0
149.70	88.0
154.90	152.0
156.70	128.0
158.70	117.0
160.70	110.0
162.90	130.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

164.90	82.0
172.00	339.0
173.90	59904.0
174.90	4378.0
175.90	59280.0
176.90	4005.0
177.90	159.0
179.00	299.0
188.80	102.0
190.90	764.0
191.90	225.0
192.90	1206.0
193.80	215.0
194.90	180.0
203.00	79.0
204.90	253.0
207.00	649.0
207.90	197.0
209.00	107.0
220.90	69.0
234.90	87.0
248.80	794.0
250.00	182.0
251.00	363.0
251.90	80.0
252.70	88.0
264.90	970.0
266.00	170.0
266.90	201.0
279.40	96.0
279.90	193.0
281.00	12823.0
282.00	2505.0
282.90	1922.0
284.00	408.0
284.80	111.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14

Scan 1750 (12.573 min): VW015750.D
BFB14

m/z	Abundance
35.90	206.0
38.10	79.0
39.00	72.0
39.90	189.0
41.00	103.0
43.00	75.0
44.10	182.0
57.10	99.0
72.80	71.0
132.90	59.0
281.10	114.0

Instrument :
MSVOA_W
ClientSampleId :
BFB14