

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063021\
 Data File : VW019373.D
 Acq On : 30 Jun 2021 12:49
 Operator : SY/VA
 Sample : M2869-19
 Misc : 5.02G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Quant Time: Jul 01 01:17:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jul 01 01:07:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	498331	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	468243	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	220258	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	165054	25.228	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.920%
7) Chloroethane-d5	2.897	69	129490	25.460	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.840%
11) 1,1-Dichloroethene-d2	4.031	63	247034	18.477	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.920%
21) 2-Butanone-d5	7.079	46	88223	54.293	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.580%
24) Chloroform-d	7.652	84	346304	25.157	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.640%
26) 1,2-Dichloroethane-d4	8.311	65	188243	26.628	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.520%
32) Benzene-d6	8.280	84	723177	25.200	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.800%
36) 1,2-Dichloropropane-d6	9.274	67	222529	25.441	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.760%
41) Toluene-d8	10.323	98	646753	24.883	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.520%
43) trans-1,3-Dichloroprop...	10.579	79	81884	23.775	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.080%
47) 2-Hexanone-d5	10.926	63	71064	51.985	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.960%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	167623	25.977	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	218378	27.103	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.400%
Target Compounds						
16) Methylene chloride	4.927	84	21735	2.495	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063021\
Data File : VW019373.D
Acq On : 30 Jun 2021 12:49
Operator : SY/VA
Sample : M2869-19
Misc : 5.02G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Quant Time: Jul 01 01:17:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jul 01 01:07:02 2021
Response via : Initial Calibration

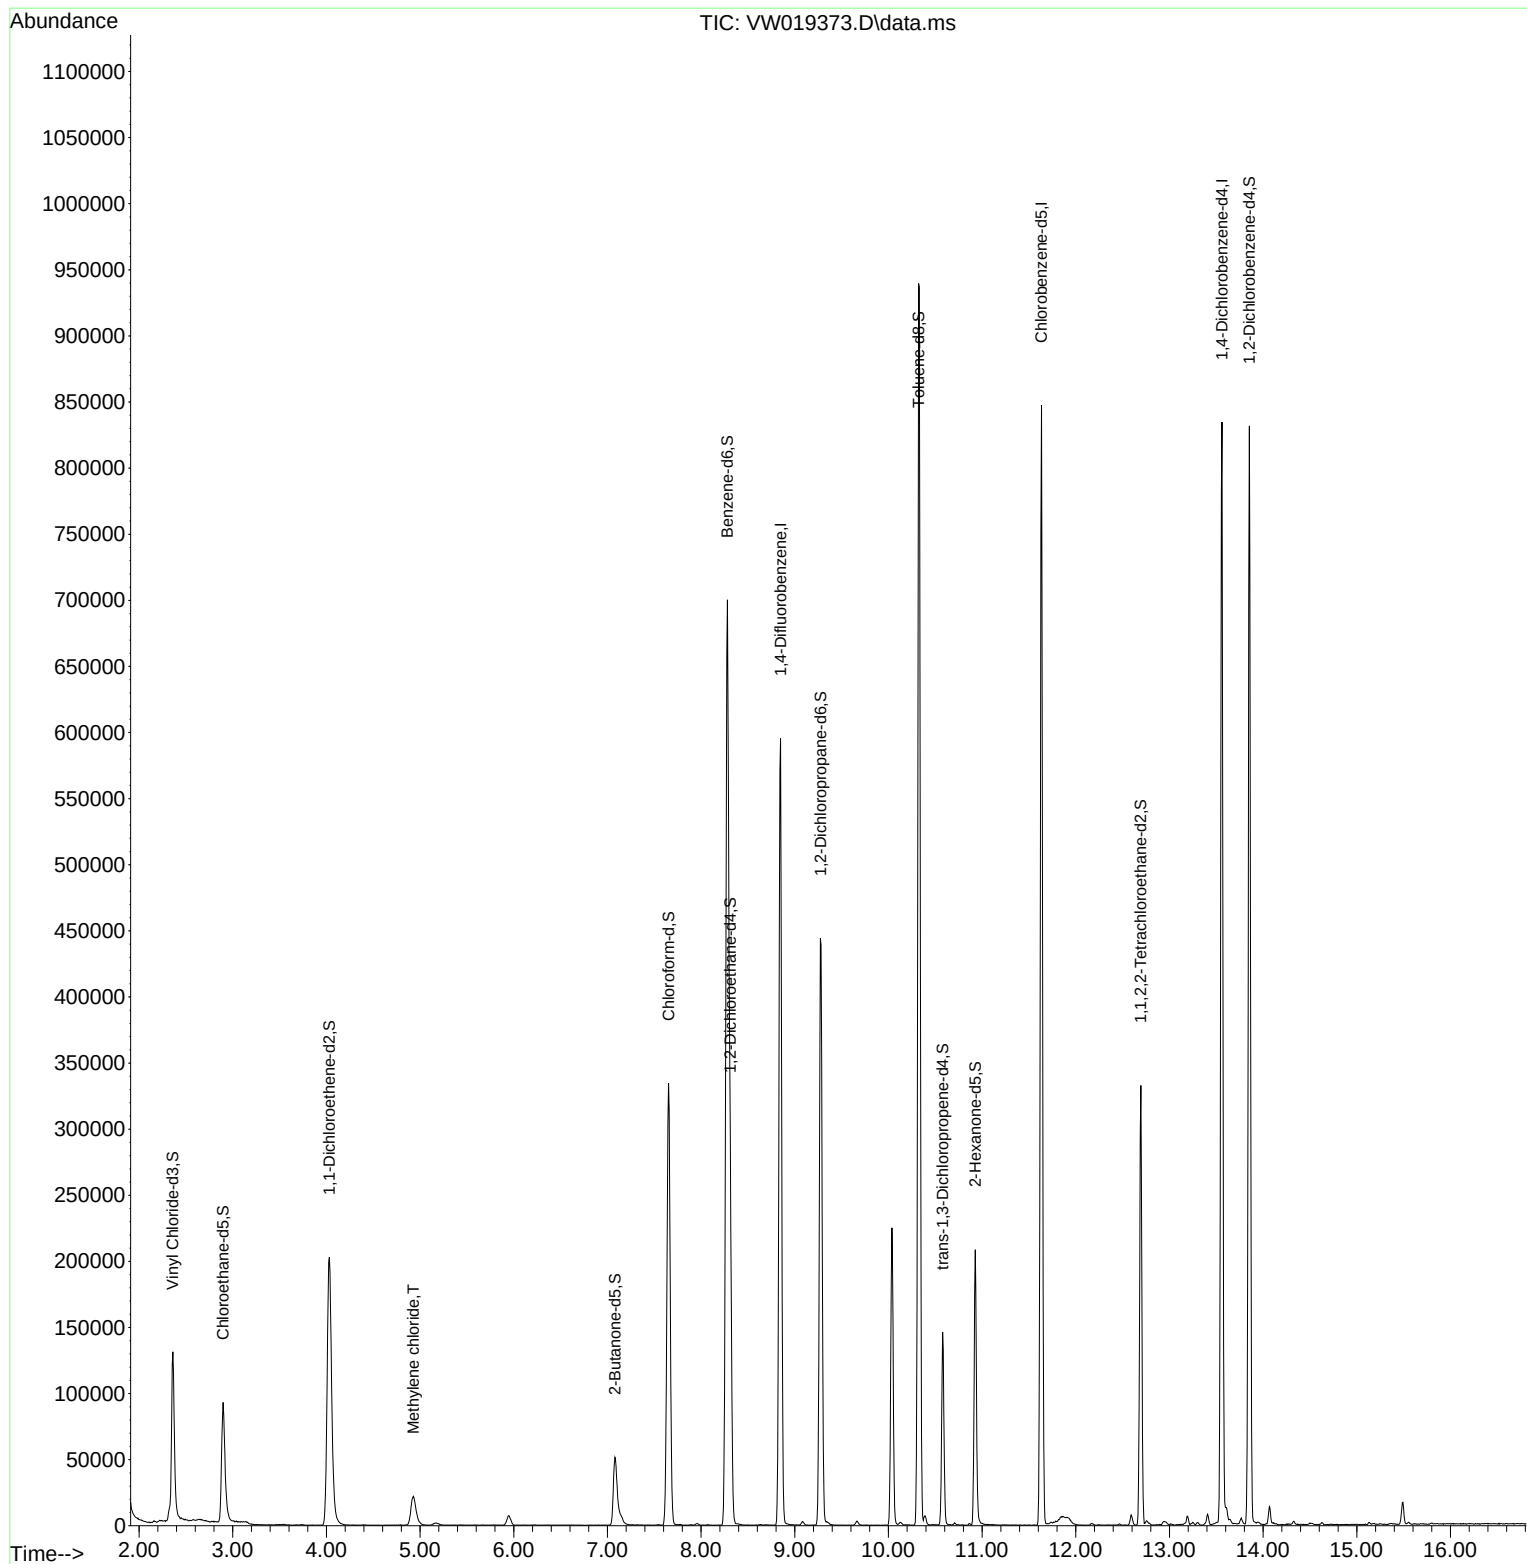

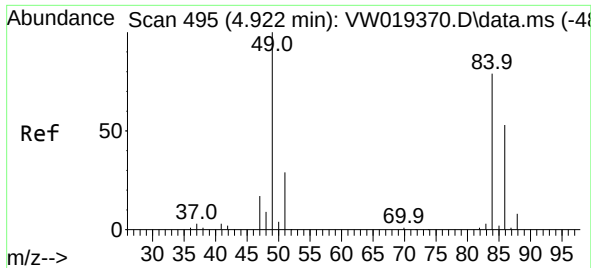

#16
Methylene chloride
Concen: 2.495 ug/L
RT: 4.927 min Scan# 496
Delta R.T. 0.006 min
Lab File: VW019373.D
Acq: 30 Jun 2021 12:49

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Tgt Ion: 84	Resp: 21735
Ion Ratio	Lower Upper
84 100	
86 63.9	45.3 84.1
49 116.5	86.6 160.8

