
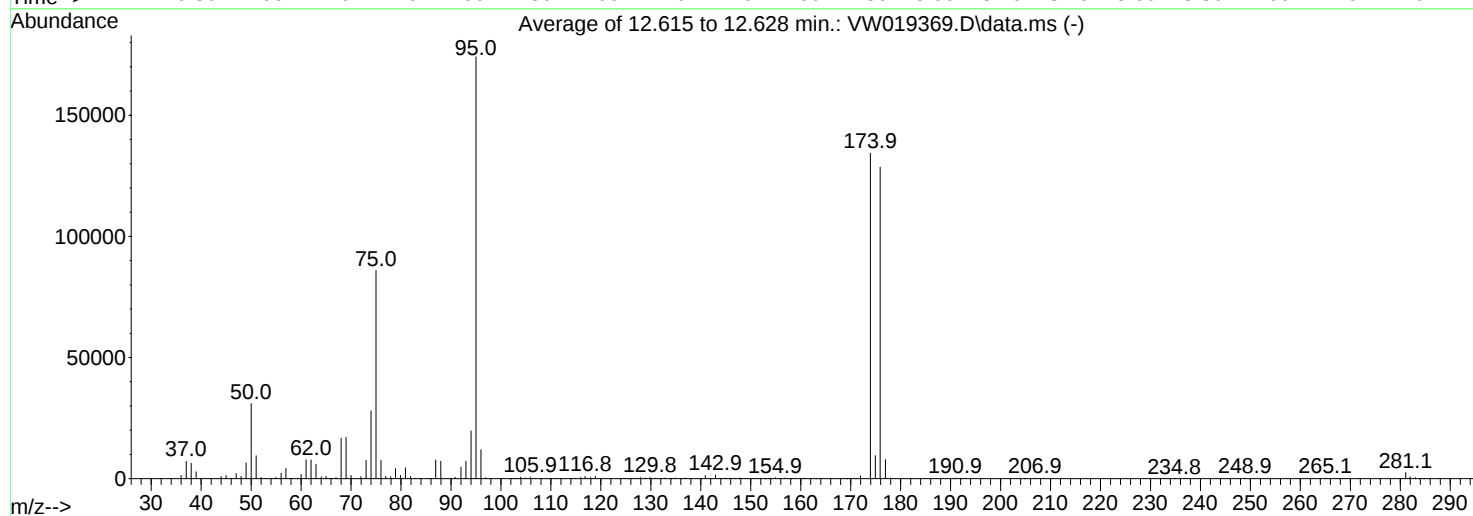


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063021\
 Data File : VW019369.D
 Acq On : 30 Jun 2021 09:52
 Operator : SY/VA
 Sample : BFB17
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB117

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM062821SMA.M
 Title : SFAM01.0
 Last Update : Sat Jul 03 04:03:43 2021

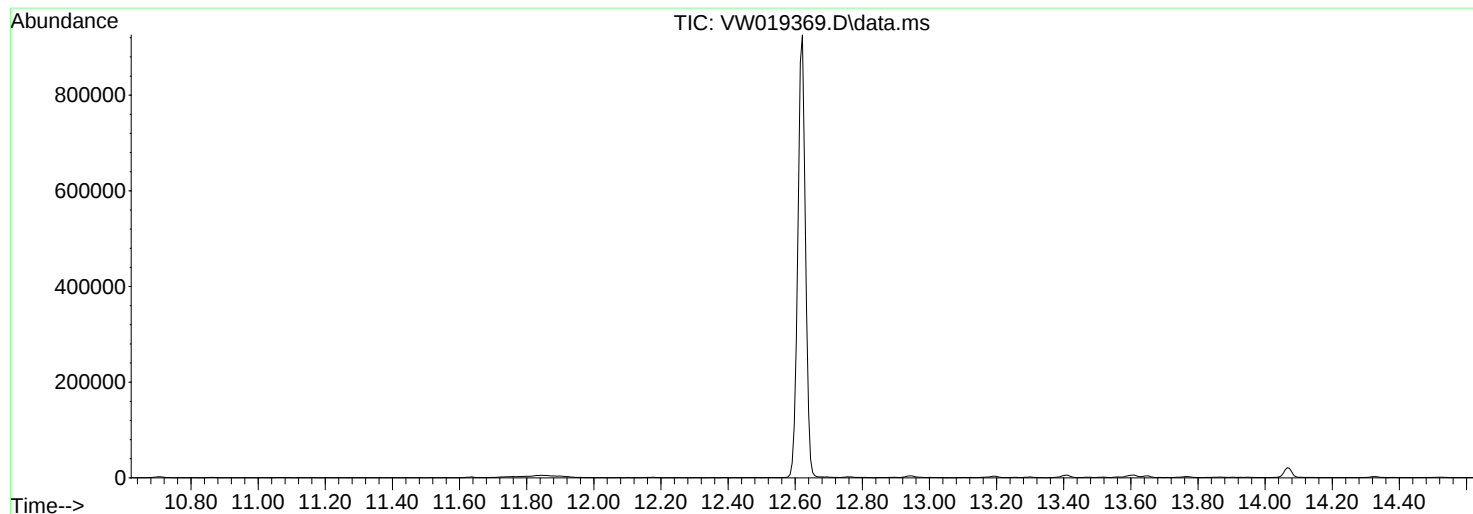

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	31008	PASS
75	95	30	80	49.3	85923	PASS
95	95	100	100	100.0	174123	PASS
96	95	5	9	6.9	11934	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.1	134333	PASS
175	174	5	9	7.1	9540	PASS
176	174	95	105	95.7	128533	PASS
177	176	5	10	6.1	7867	PASS

m/z	Abundance
36.00	1437.0
37.00	8403.0
38.00	7418.0
39.00	3464.0
40.00	378.0
43.10	112.0
44.00	1139.0
45.00	1392.0
46.00	228.0
47.00	2002.0
48.00	1138.0
49.00	7315.0
50.00	35128.0
51.00	11139.0
52.10	469.0
53.00	105.0
55.00	683.0
56.00	2444.0
57.00	4852.0
57.90	240.0
59.20	88.0
60.00	1798.0
61.00	8985.0
62.00	8850.0
63.00	6545.0
64.00	860.0
65.00	1169.0
66.20	92.0
67.10	347.0
68.00	19280.0
69.00	18536.0
70.00	1758.0
72.00	807.0
73.00	8480.0
74.00	30936.0
75.00	96560.0
76.00	8795.0
76.90	1016.0
78.00	853.0
78.90	4599.0
79.90	1747.0
80.90	4948.0
81.90	892.0
82.90	127.0
85.80	345.0
86.90	8368.0
87.90	7622.0
90.80	688.0
92.00	5266.0
93.00	7670.0
94.00	20992.0
95.00	183232.0
96.00	13199.0
97.00	316.0
103.00	186.0
103.90	629.0
104.90	270.0
105.90	717.0
106.90	171.0
109.90	109.0
110.90	160.0
111.90	112.0
112.90	132.0
114.90	171.0
115.90	514.0
116.80	1155.0
118.00	612.0
118.90	905.0
123.90	80.0
124.80	209.0
125.90	87.0
127.90	562.0
128.90	272.0
129.90	614.0
130.90	204.0
132.80	418.0
134.00	85.0
135.00	291.0
137.00	221.0
140.00	85.0
140.90	1484.0
141.90	190.0
142.90	1522.0
144.00	118.0
145.10	240.0
145.90	226.0
146.80	170.0
147.90	324.0
148.90	153.0
149.80	144.0
153.10	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117

m/z	Abundance
40.10	171.0
40.90	53.0
44.10	294.0
56.90	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117

m/z	Abundance
36.00	1460.0
37.00	8192.0
38.00	7138.0
39.00	3206.0
40.00	305.0
41.00	61.0
43.20	63.0
44.00	1444.0
45.00	1521.0
46.10	188.0
47.00	2681.0
48.00	859.0
49.00	7219.0
50.00	34320.0
51.00	10371.0
52.00	565.0
53.00	71.0
54.90	427.0
56.00	2495.0
57.00	4780.0
58.20	194.0
60.00	1911.0
61.00	8295.0
62.00	8763.0
63.00	6677.0
64.10	740.0
65.00	966.0
66.10	84.0
66.90	476.0
68.00	18000.0
69.00	19496.0
70.00	1376.0
72.00	847.0
73.00	8284.0
74.00	31680.0
75.00	94912.0
76.00	8158.0
77.00	1209.0
77.90	916.0
78.90	4931.0
79.90	1341.0
80.90	4959.0
81.90	934.0
82.90	156.0
86.90	8629.0
88.00	8320.0
90.90	647.0
92.00	5250.0
93.00	8034.0
94.00	22248.0
95.00	202176.0
96.00	13145.0
96.90	313.0
102.80	103.0
103.90	688.0
105.00	246.0
105.90	697.0
106.90	159.0
110.00	87.0
110.90	158.0
112.00	127.0
112.80	140.0
114.90	196.0
116.00	500.0
116.90	1101.0
117.90	582.0
118.90	1117.0
124.00	54.0
124.90	112.0
125.30	70.0
125.90	103.0
126.90	74.0
127.90	579.0
129.00	292.0
129.80	512.0
130.90	226.0
132.90	193.0
135.00	191.0
136.90	326.0
140.00	169.0
140.90	1384.0
141.90	261.0
143.00	1743.0
143.90	110.0
144.90	283.0
145.90	331.0
147.00	156.0
147.90	326.0
148.90	176.0
150.10	151.0
152.00	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117

153.80	117.0
155.00	349.0
155.70	55.0
156.80	211.0
158.90	182.0
160.80	259.0
163.00	73.0
170.80	147.0
171.10	147.0
172.00	1409.0
173.90	136768.0
174.90	9698.0
175.90	122560.0
177.00	7982.0
178.00	312.0
178.80	118.0
191.00	386.0
192.10	71.0
192.90	330.0
204.80	91.0
207.00	292.0
208.00	72.0
248.90	307.0
249.90	51.0
250.90	142.0
265.00	314.0
266.10	96.0
267.10	141.0
281.10	4250.0
282.00	1423.0
283.10	411.0
283.80	130.0
284.70	84.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117

153.00	150.0
154.10	122.0
154.90	471.0
155.80	89.0
156.80	345.0
158.10	55.0
158.90	128.0
160.80	207.0
169.20	61.0
170.90	183.0
171.90	1148.0
173.90	155520.0
175.00	11534.0
175.90	145728.0
176.90	9413.0
177.90	259.0
178.80	85.0
190.90	188.0
193.00	188.0
206.90	204.0
207.90	59.0
234.80	58.0
249.00	173.0
249.90	61.0
250.90	91.0
265.10	277.0
265.90	68.0
267.00	68.0
281.10	2265.0
281.90	659.0
283.00	494.0
283.90	104.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117

m/z	Abundance
36.00	1013.0
37.00	4915.0
38.00	4457.0
39.00	1948.0
40.00	221.0
43.10	70.0
44.10	804.0
45.00	1075.0
46.00	131.0
47.00	1713.0
48.00	739.0
49.00	4830.0
50.00	23576.0
51.00	6752.0
51.90	300.0
52.90	74.0
54.90	289.0
56.00	1769.0
57.00	3238.0
58.00	119.0
60.00	1403.0
61.00	5867.0
62.00	5620.0
63.00	4676.0
64.10	576.0
65.10	603.0
67.00	346.0
68.00	12954.0
69.00	13203.0
70.00	930.0
71.90	744.0
73.00	5814.0
74.00	21368.0
75.00	66296.0
76.00	5586.0
76.90	664.0
78.00	515.0
78.90	3019.0
80.00	981.0
80.90	3322.0
81.90	786.0
82.90	109.0
87.00	6157.0
87.90	5626.0
90.90	450.0
92.00	3706.0
93.00	5793.0
94.00	15896.0
95.00	136960.0
96.00	9457.0
97.00	401.0
103.00	86.0
103.90	518.0
104.90	204.0
105.90	420.0
107.00	149.0
110.00	66.0
110.80	80.0
112.00	126.0
112.80	135.0
115.00	133.0
115.90	456.0
116.90	802.0
117.90	525.0
118.90	703.0
127.00	58.0
127.90	408.0
128.90	210.0
129.90	530.0
130.80	186.0
133.00	117.0
134.90	244.0
136.80	188.0
140.10	138.0
140.90	1078.0
141.80	156.0
142.90	1191.0
143.90	101.0
144.90	143.0
145.80	258.0
147.00	101.0
147.80	293.0
148.80	58.0
149.90	123.0
152.00	74.0
152.80	61.0
154.00	92.0
155.00	398.0
155.80	69.0
156.90	304.0
158.00	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117

158.90	121.0
160.80	144.0
171.10	132.0
171.90	919.0
174.00	110712.0
175.00	7389.0
175.90	117312.0
177.00	6205.0
178.00	225.0
191.10	65.0
193.00	85.0
206.90	140.0
248.90	56.0
264.90	110.0
265.90	59.0
281.00	982.0
281.90	344.0
283.00	212.0

Instrument :
MSVOA_W
ClientSampleId :
BFB117