
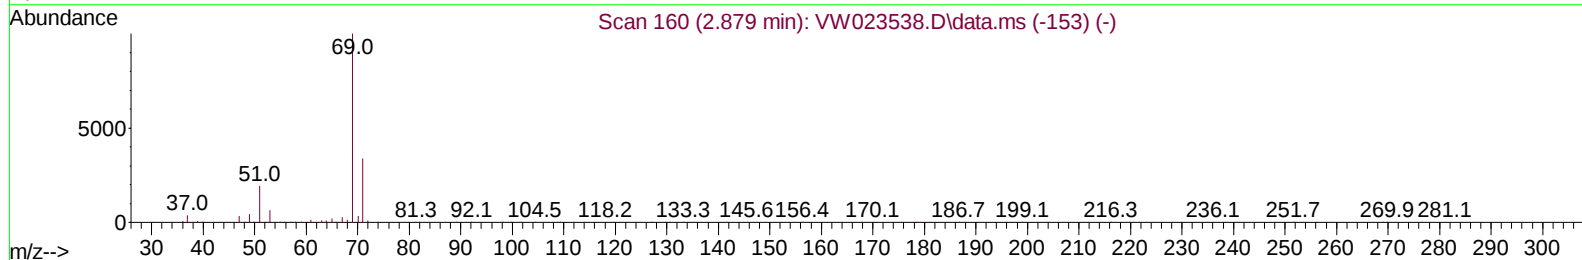
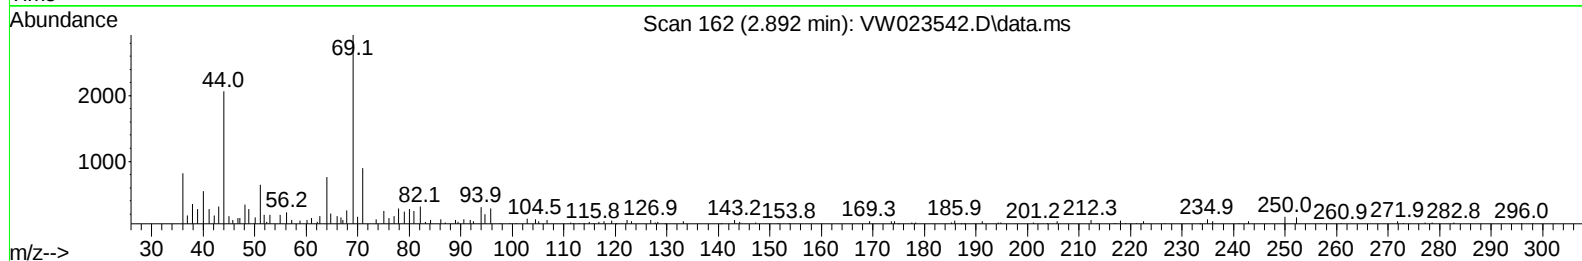


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063022\
Data File : VW023542.D
Acq On : 30 Jun 2022 12:32
Operator : SY/VA
Sample : VSTD2.533
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 05:32:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 01 05:29:39 2022
Response via : Initial Calibration

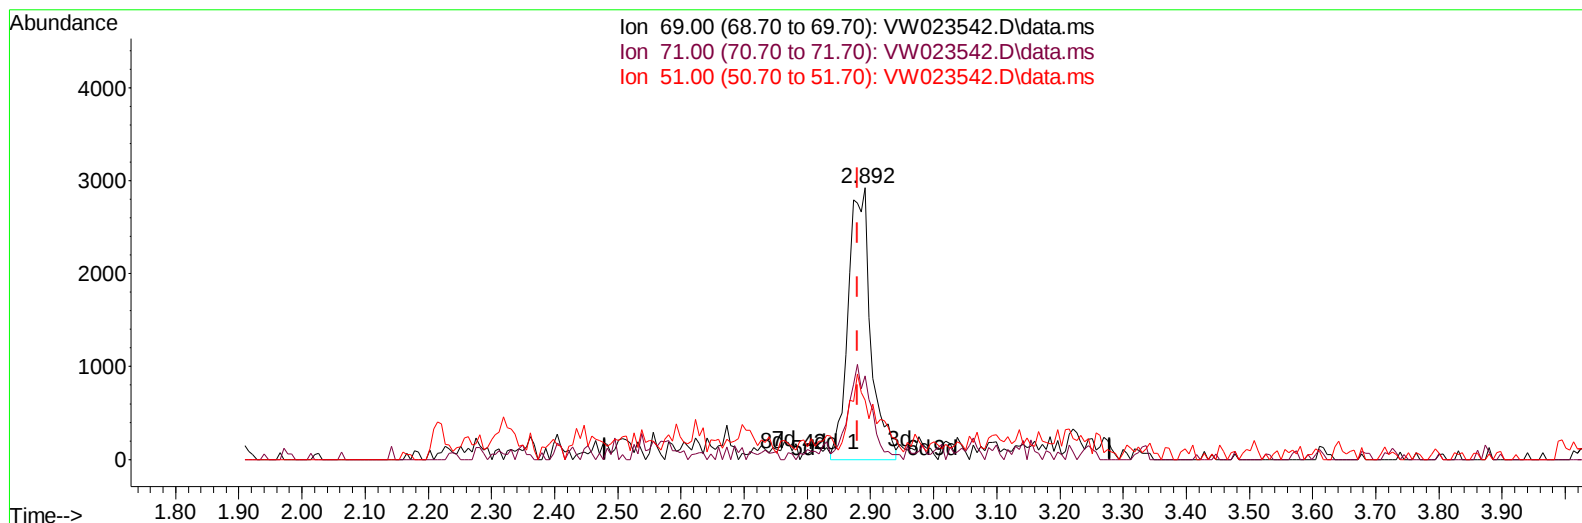

TIC: VW023542.D\data.ms

(7) Chloroethane-d5 (S)

2.892min (+ 0.012) 2.08 ug/L m

response 7298

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.70	30.99
51.00	26.00	23.57
0.00	0.00	0.00