
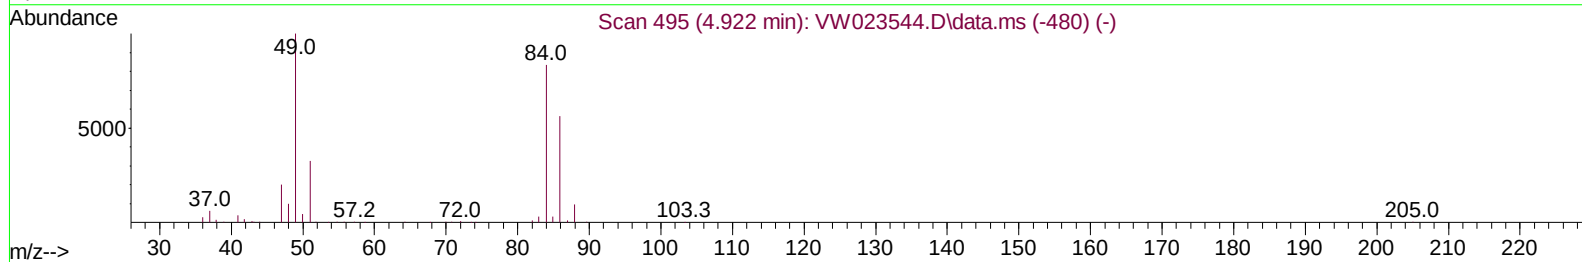
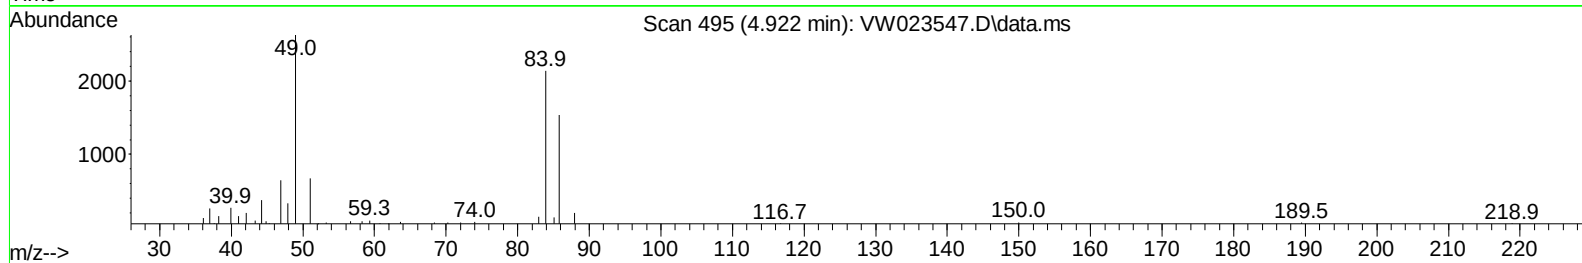


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063022\
Data File : VW023547.D
Acq On : 30 Jun 2022 15:40
Operator : SY/VA
Sample : N3553-01
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 05:58:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 01 05:57:56 2022
Response via : Initial Calibration

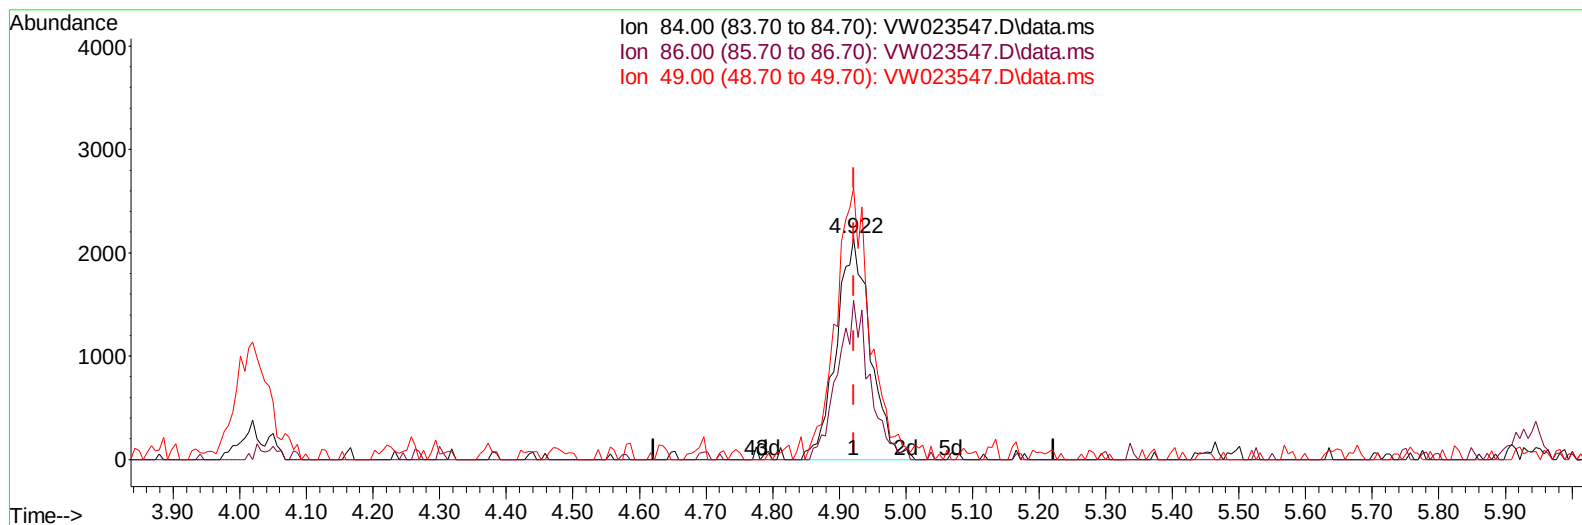

TIC: VW023547.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.000) 1.33 ug/L m

response 7605

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.10	71.77
49.00	125.10	122.63
0.00	0.00	0.00