
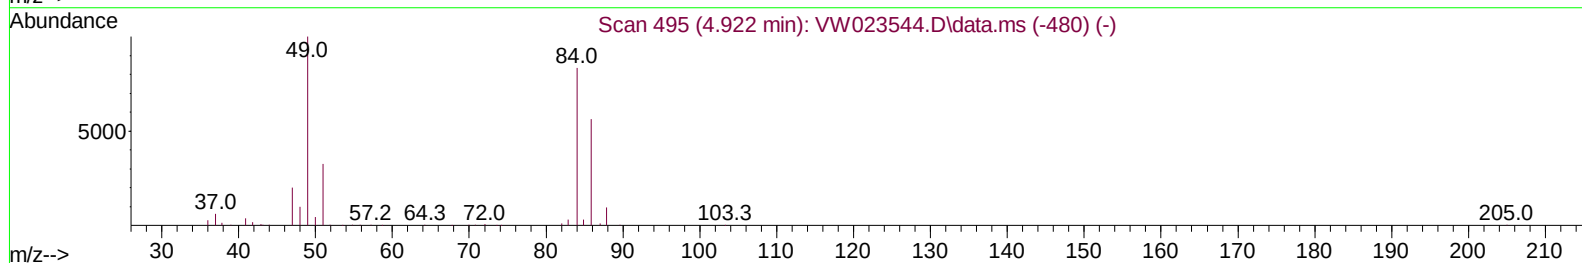
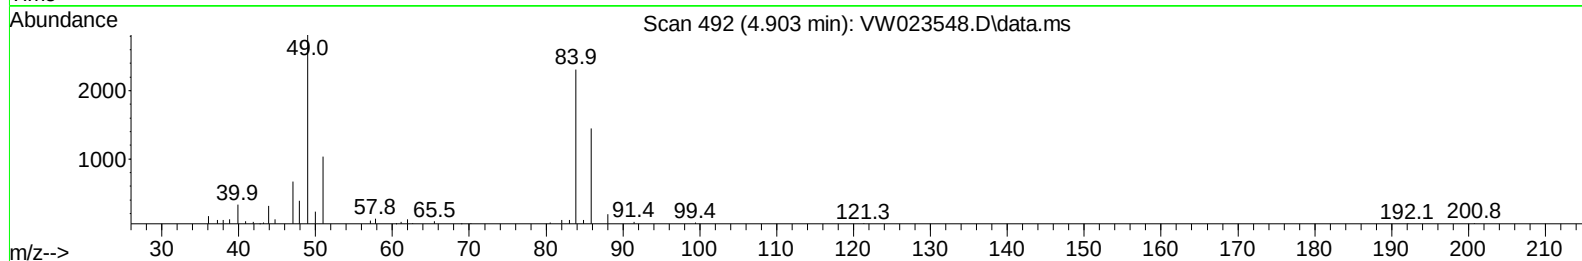


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063022\
Data File : VW023548.D
Acq On : 30 Jun 2022 16:04
Operator : SY/VA
Sample : N3553-02
Misc : 5.54g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 01 05:59:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 01 05:57:56 2022
Response via : Initial Calibration

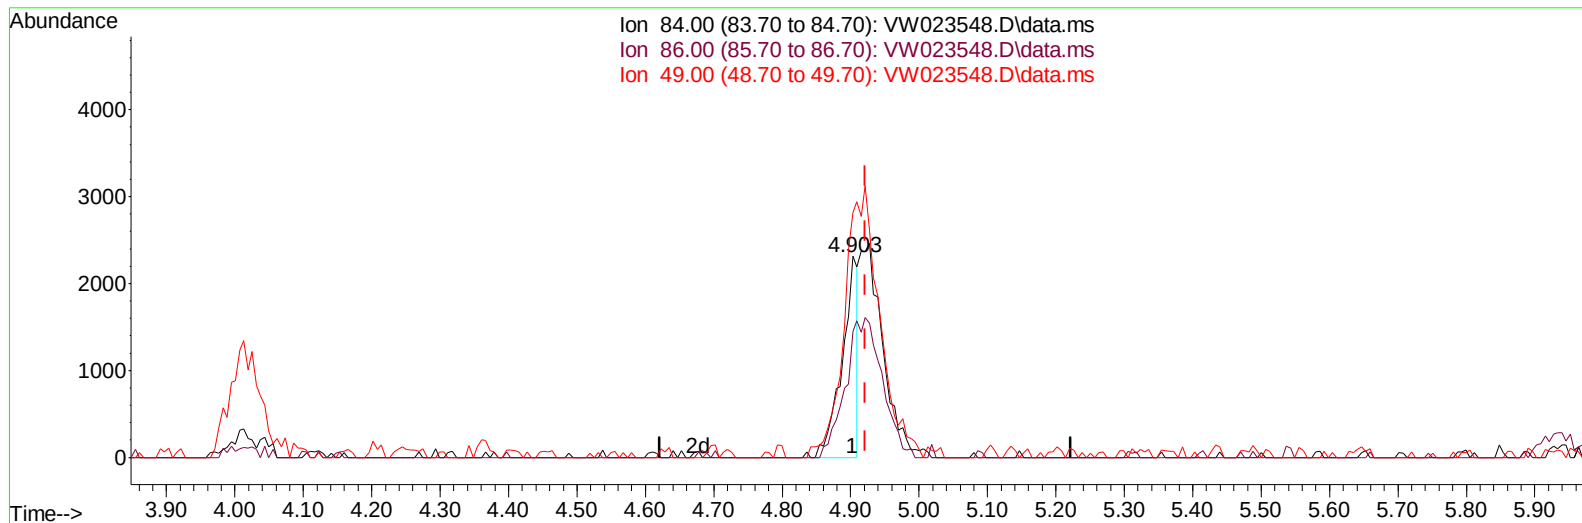

TIC: VW023548.D\data.ms

(16) Methylene chloride (T)

4.903min (-0.019) 0.62 ug/L

response 3714

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.10	62.73
49.00	125.10	121.79
0.00	0.00	0.00