

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063022\
 Data File : VW023547.D
 Acq On : 30 Jun 2022 15:40
 Operator : SY/VA
 Sample : N3553-01
 Misc : 6.37g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AG0

Quant Time: Jul 01 05:58:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 01 05:57:56 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	399695	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	373937	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	178229	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	97094	16.983	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.920%
7) Chloroethane-d5	2.885	69	68631	17.430	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.720%
11) 1,1-Dichloroethene-d2	4.019	63	84677	11.970	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.880%
21) 2-Butanone-d5	7.080	46	75773	52.916	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.840%
24) Chloroform-d	7.647	84	218372	20.014	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	80.040%
26) 1,2-Dichloroethane-d4	8.305	65	120847	20.057	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.240%
32) Benzene-d6	8.275	84	375166	18.556	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.240%
36) 1,2-Dichloropropane-d6	9.275	67	121580	20.340	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.360%
41) Toluene-d8	10.323	98	354883	18.048	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.200%
43) trans-1,3-Dichloroprop...	10.579	79	52120	19.683	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.720%
47) 2-Hexanone-d5	10.927	63	59042	52.072	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.140%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	134996	23.522	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	142207	21.877	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.520%
Target Compounds						Qvalue
14) Carbon disulfide	4.385	76	15904	1.468	ug/L	# 92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW063022\
Data File : VW023547.D
Acq On : 30 Jun 2022 15:40
Operator : SY/VA
Sample : N3553-01
Misc : 6.37g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AG0


Quant Time: Jul 01 05:58:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM063022SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 01 05:57:56 2022
Response via : Initial Calibration

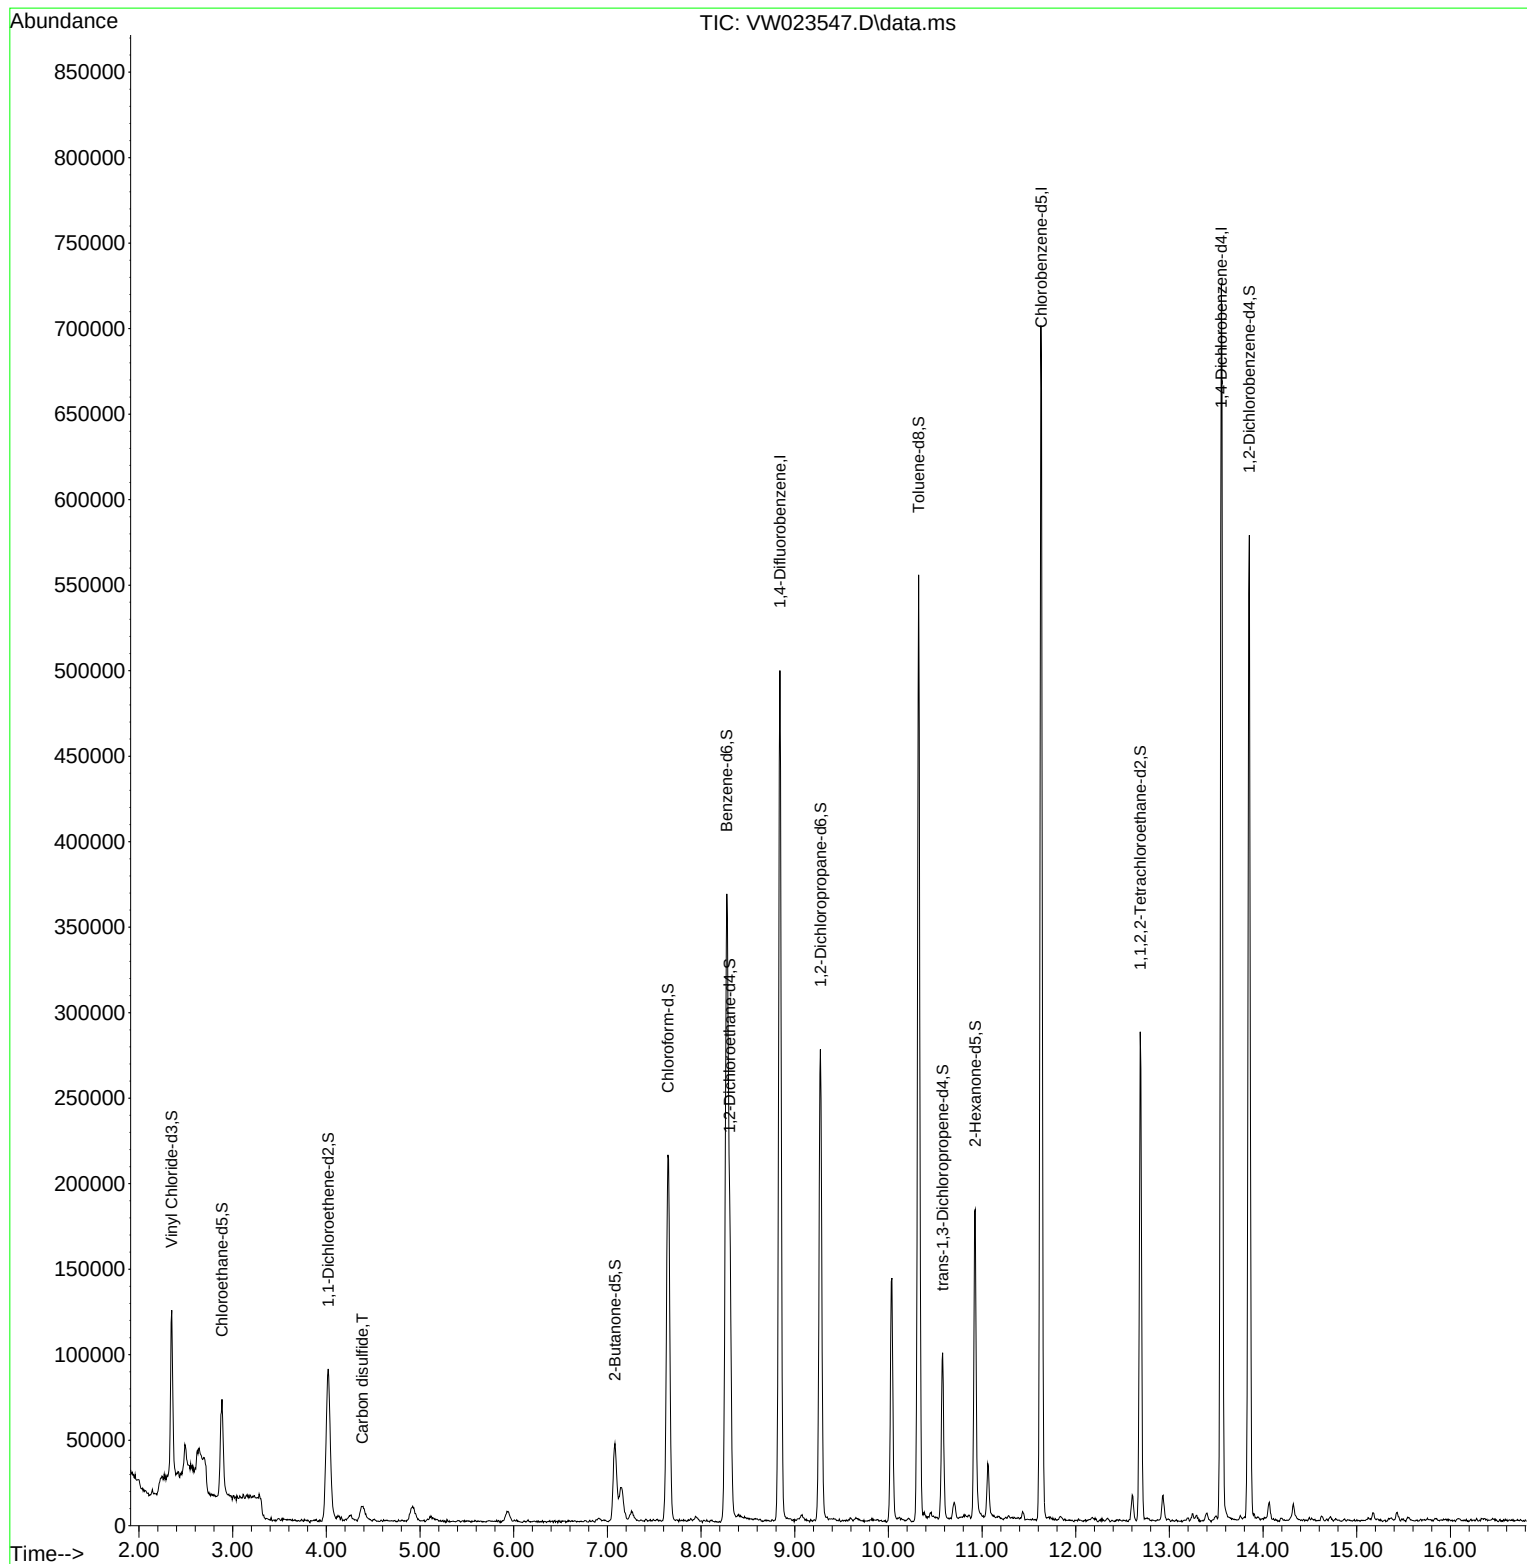

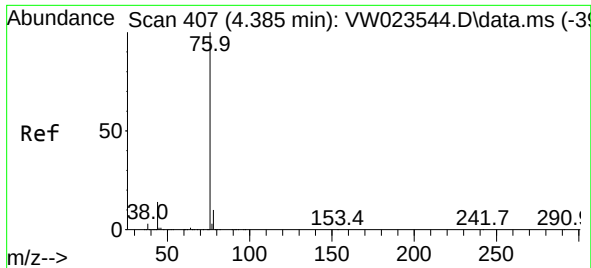

#14
Carbon disulfide
Concen: 1.468 ug/L
RT: 4.385 min Scan# 407
Delta R.T. 0.000 min
Lab File: VW023547.D
Acq: 30 Jun 2022 15:40

Instrument :
MSVOA_W
ClientSampleId :
C0AG0

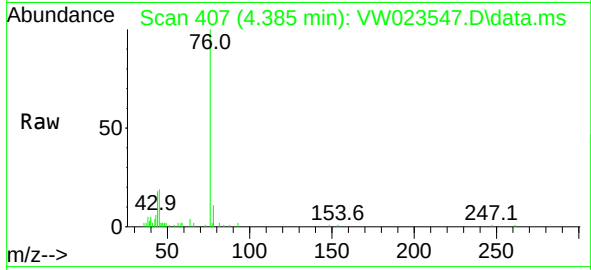

Tgt Ion: 76 Resp: 15904
Ion Ratio Lower Upper
76 100
78 11.2 6.8 10.2#

