

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW070119\
 Data File : VW011080.D
 Acq On : 01 Jul 2019 13:08
 Operator : SY/VA
 Sample : K3580-03
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 SB-12-9.5-10.0

Quant Time: Jul 02 08:58:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 01:55:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	197424	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	335622	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	290379	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	126061	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	140345	54.38	ug/l	0.00
Spiked Amount						
			Recovery	=	108.76%	
35) Dibromofluoromethane	7.88	113	104220	50.85	ug/l	0.00
Spiked Amount						
			Recovery	=	101.70%	
50) Toluene-d8	10.32	98	418607	49.62	ug/l	0.00
Spiked Amount						
			Recovery	=	99.24%	
62) 4-Bromofluorobenzene	12.62	95	141120	45.74	ug/l	0.00
Spiked Amount						
			Recovery	=	91.48%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW070119\
Data File : VW011080.D
Acq On : 01 Jul 2019 13:08
Operator : SY/VA
Sample : K3580-03
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
SB-12-9.5-10.0

Quant Time: Jul 02 08:58:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 01:55:46 2019
Response via : Initial Calibration

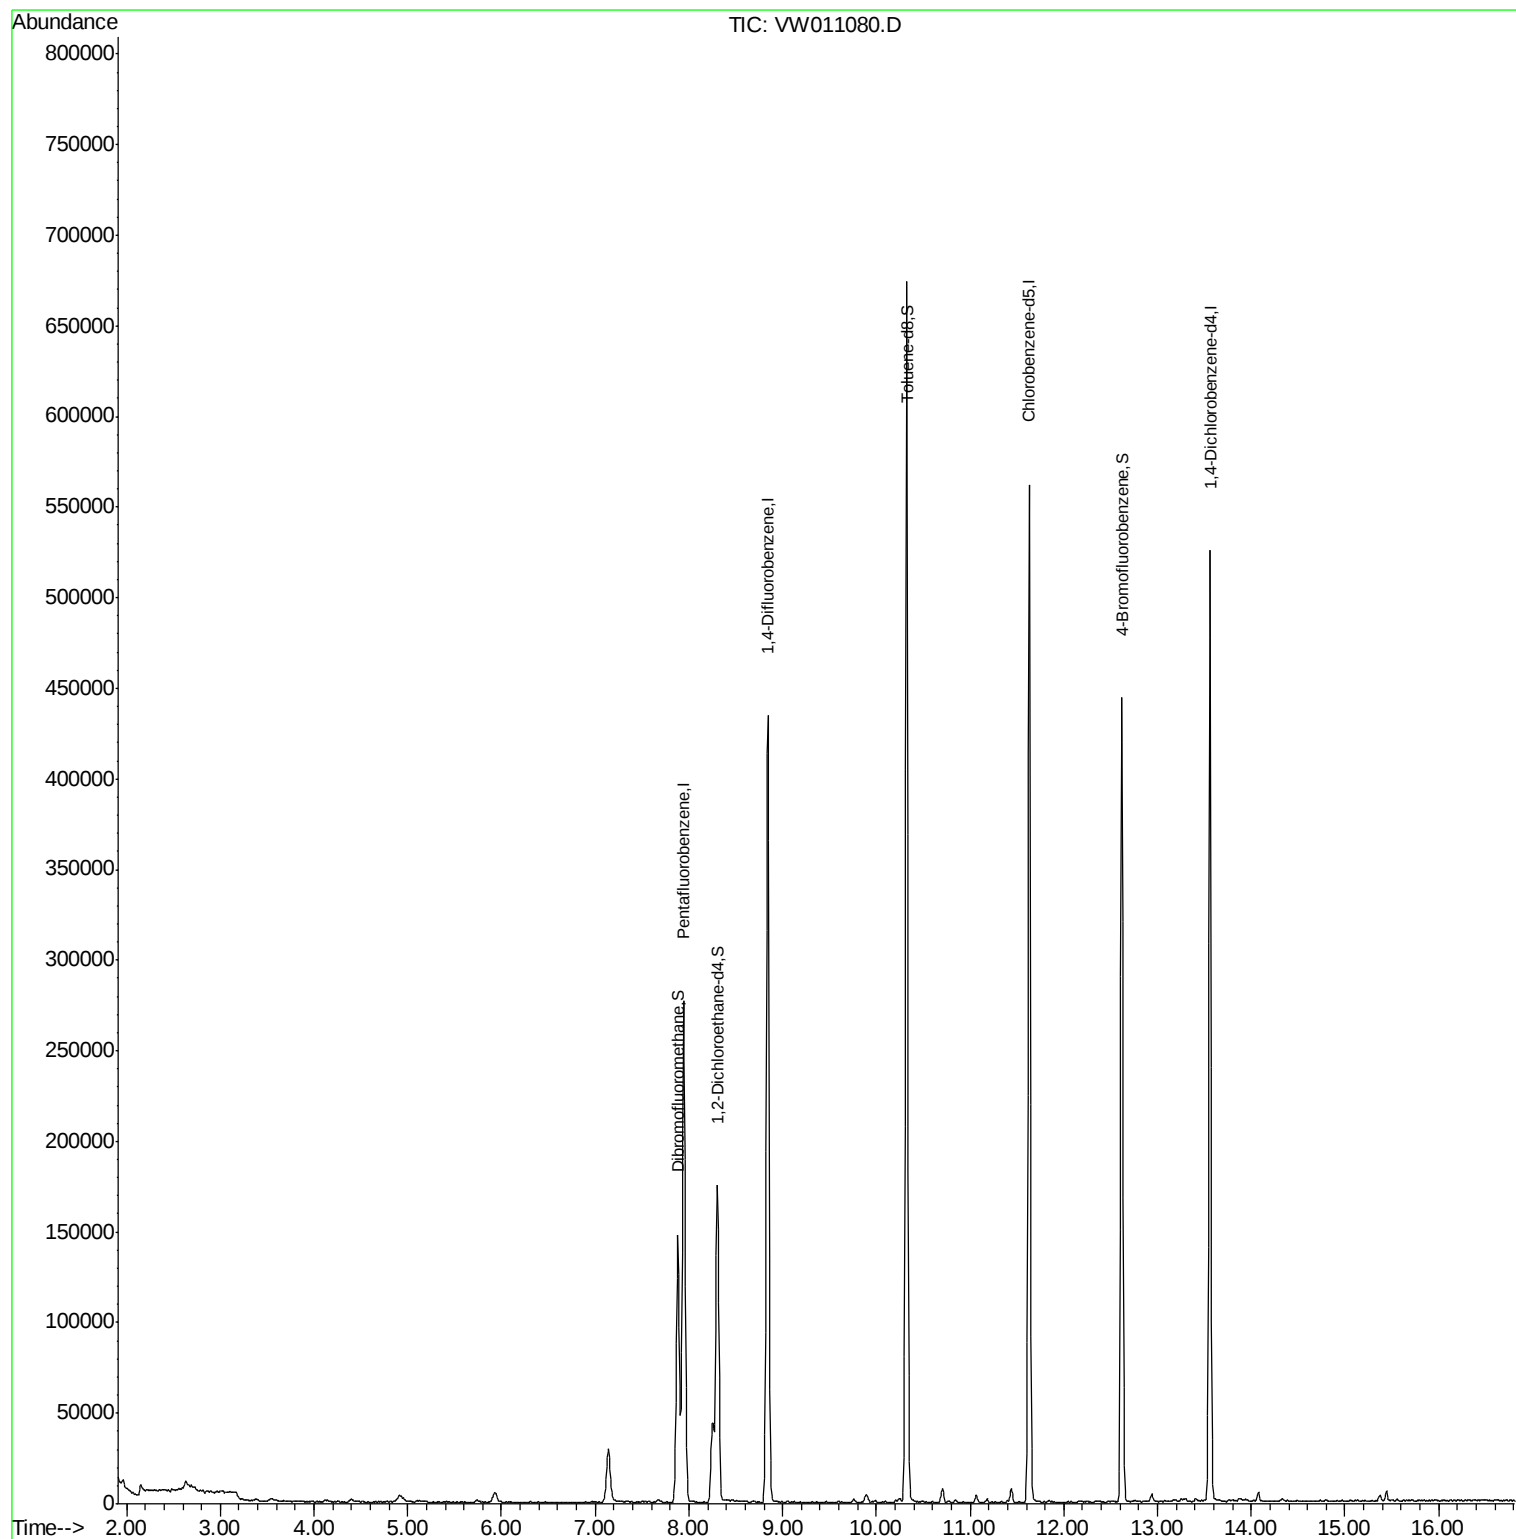

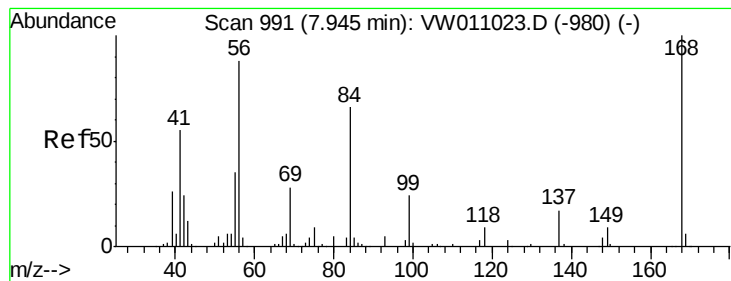

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011080.D

Acq: 01 Jul 2019 13:08

Instrument :

MSVOA_W

ClientSampleId :


SB-12-9.5-10.0

Tot Ion:168 Resp: 197424

Ion Ratio Lower Upper

168 100

99 61.3 47.8 71.6

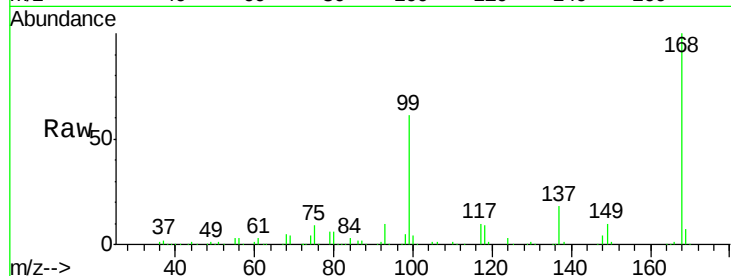

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

80000



60000

40000

20000

0

Time--> 7.80 7.90 8.00 8.10

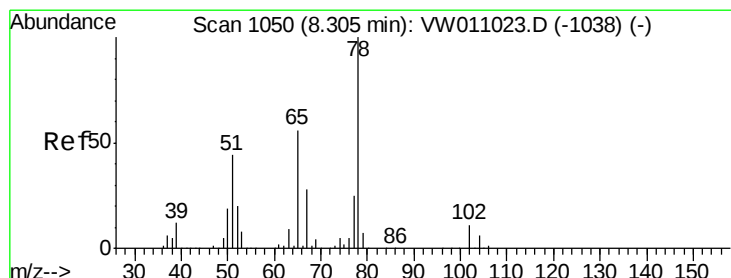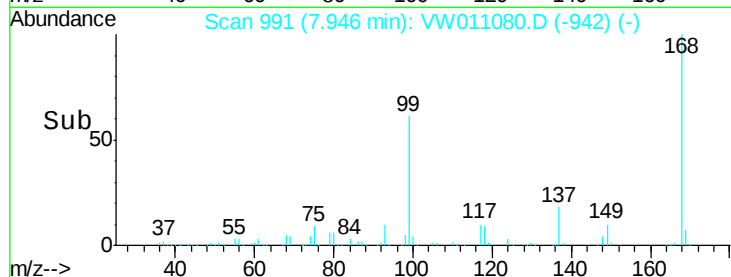

#33

1,2-Dichloroethane-d4

Concen: 54.379 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW011080.D


Acq: 01 Jul 2019 13:08

Tgt Ion: 65 Resp: 140345

Ion Ratio Lower Upper

65 100

67 51.5 0.0 102.4

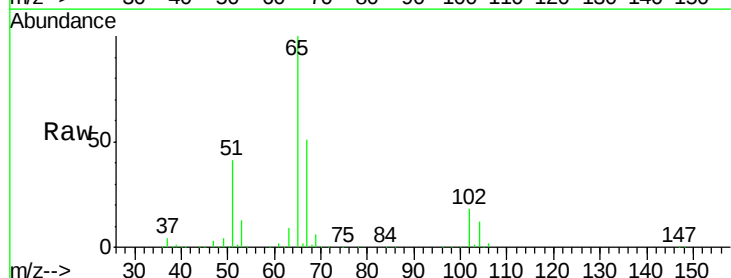

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31


60000


40000

20000

0

Time--> 8.20 8.30 8.40




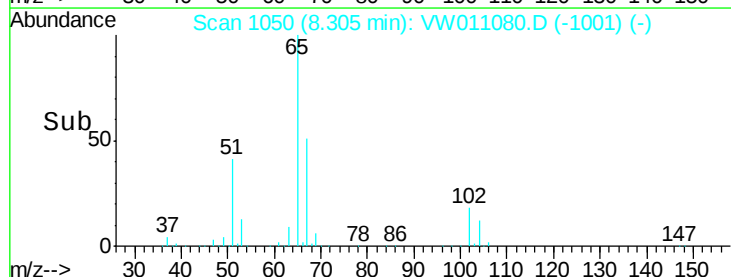


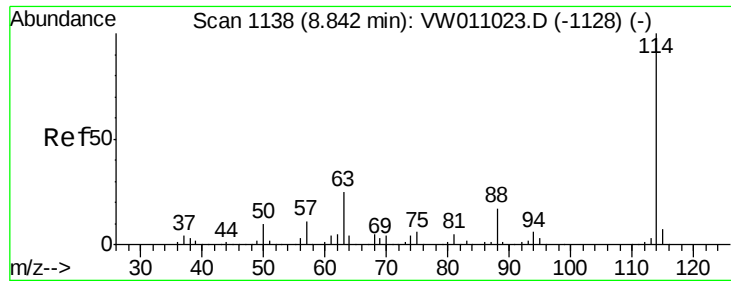

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.84 min Scan# 1138
Delta R.T. 0.00 min
Lab File: VW011080.D
Acq: 01 Jul 2019 13:08




Instrument :
MSVOA_W
ClientSampleId :
SB-12-9.5-10.0


Tot Ion:114 Resp: 335622
Ion Ratio Lower Upper
114 100
63 24.2 0.0 50.6
88 17.0 0.0 34.0

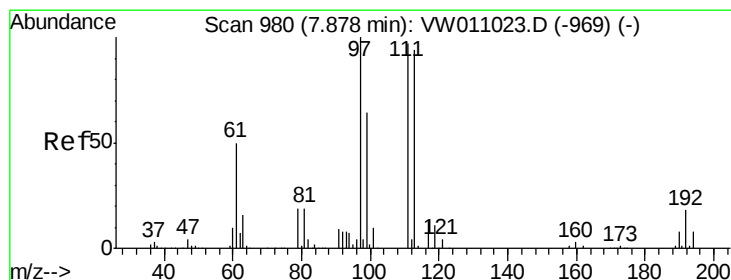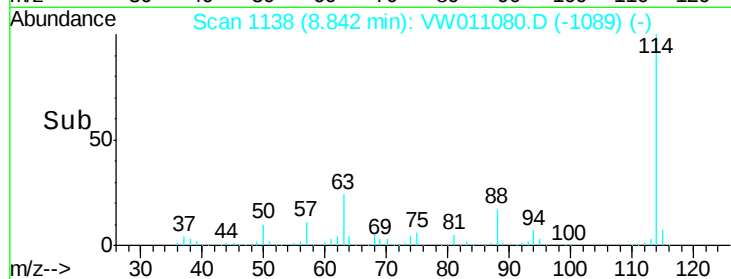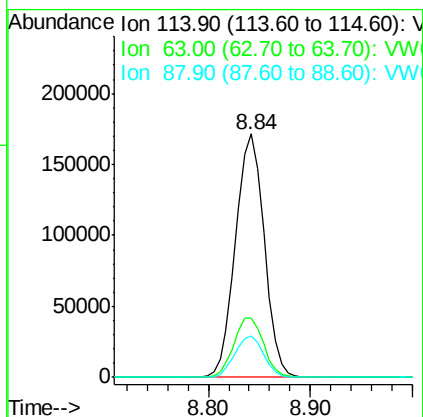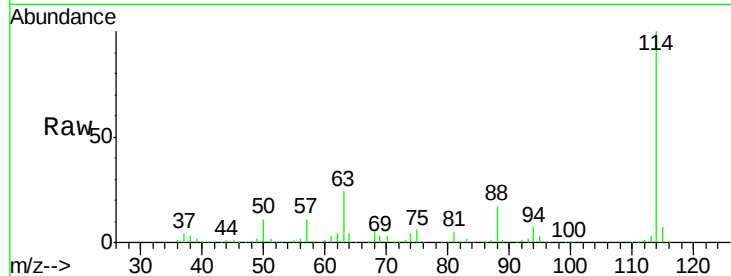

#35
Dibromofluoromethane
Concen: 50.853 ug/l
RT: 7.88 min Scan# 981
Delta R.T. 0.01 min
Lab File: VW011080.D
Acq: 01 Jul 2019 13:08

Tgt Ion:113 Resp: 104220
Ion Ratio Lower Upper
113 100
111 102.2 83.8 125.6
192 19.7 16.0 24.0

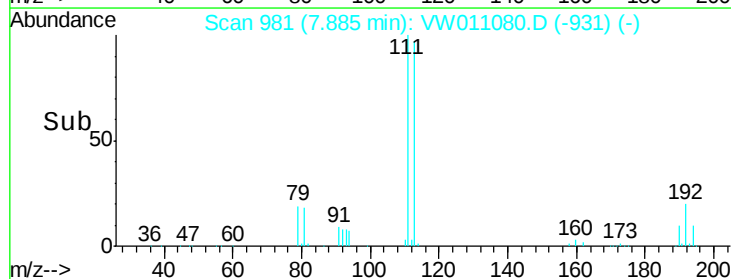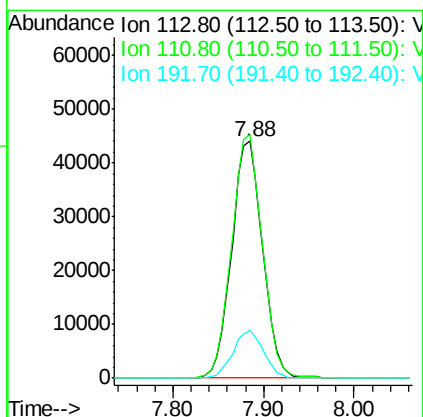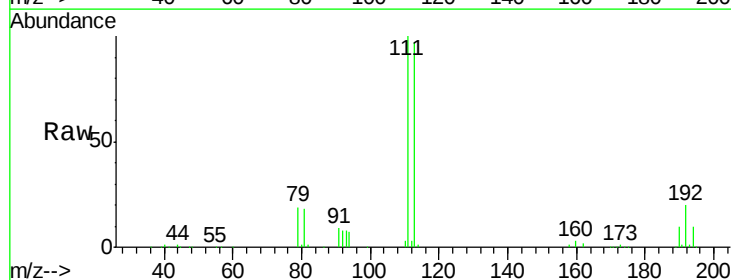

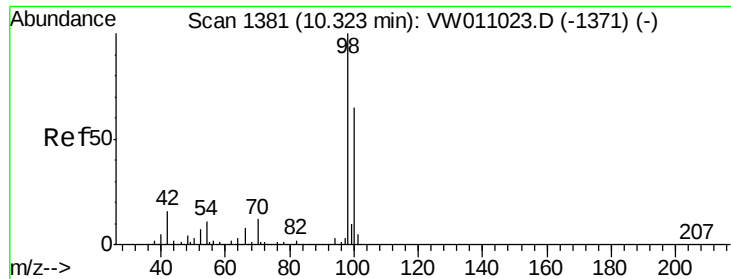

#50

Toluene-d8

Concen: 49.621 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW011080.D

Acq: 01 Jul 2019 13:08

Instrument :

MSVOA_W

ClientSampleId :


SB-12-9.5-10.0

Tot Ion: 98 Resp: 418607

Ion Ratio Lower Upper




98 100

100 65.6 52.3 78.5

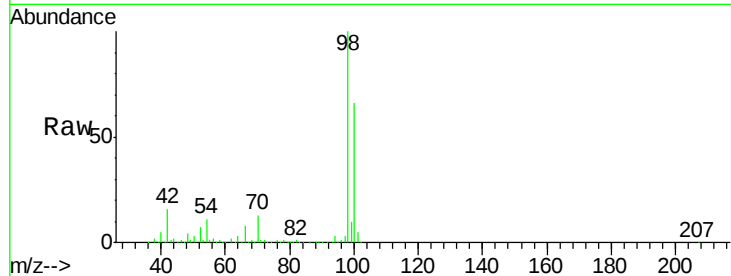

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

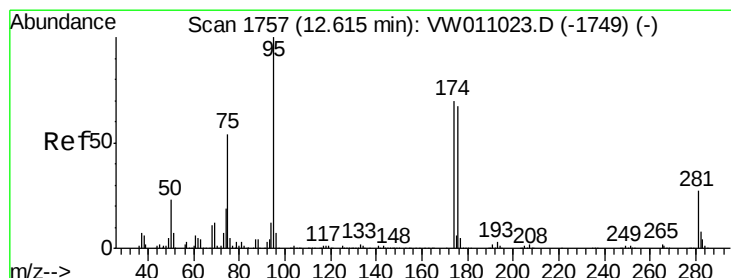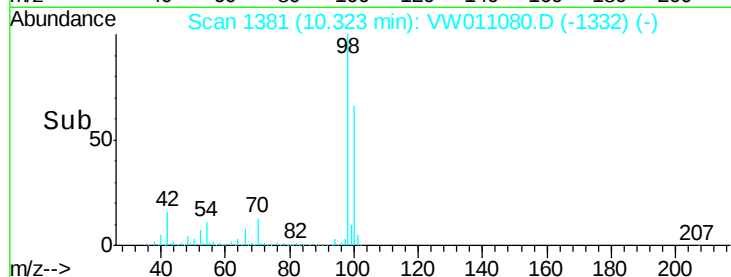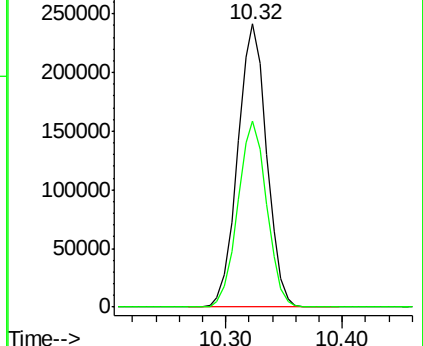

#62

4-Bromofluorobenzene

Concen: 45.737 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.01 min

Lab File: VW011080.D

Acq: 01 Jul 2019 13:08


Tgt Ion: 95 Resp: 141120

Ion Ratio Lower Upper

95 100

174 74.6 0.0 149.2



176 71.5 0.0 143.6

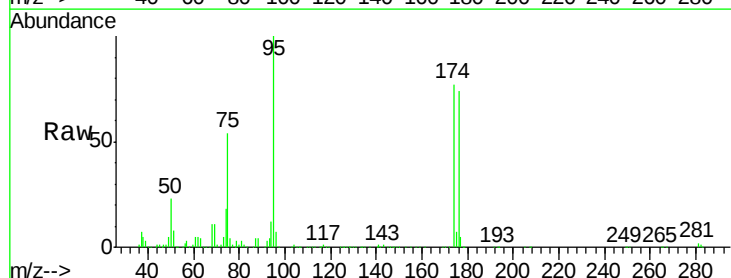


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

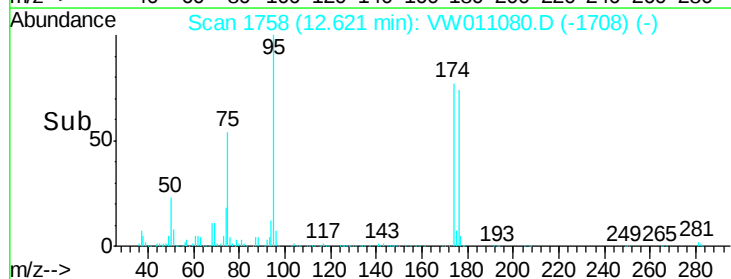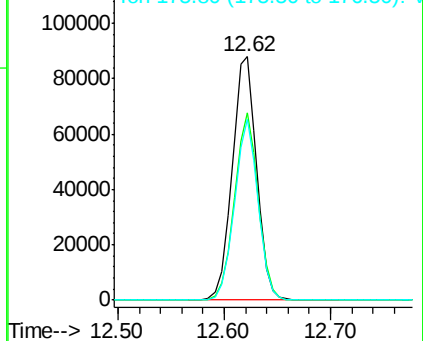


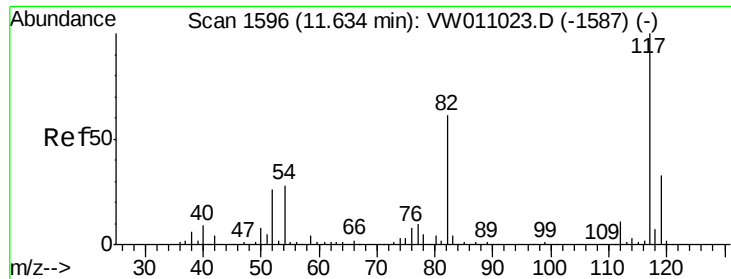




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW011080.D
Acq: 01 Jul 2019 13:08

Instrument :
MSVOA_W
ClientSampleId :
SB-12-9.5-10.0

Tot Ion:117 Resp: 290379
Ion Ratio Lower Upper
117 100
82 59.6 48.6 73.0
119 32.2 26.1 39.1

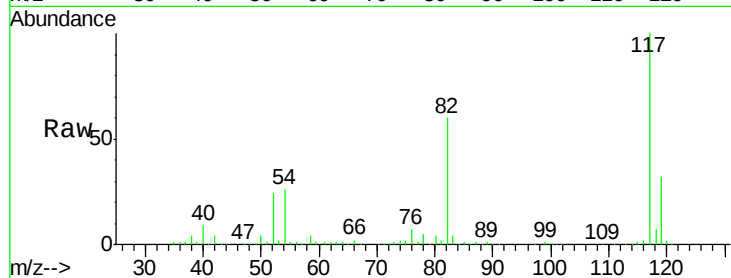


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

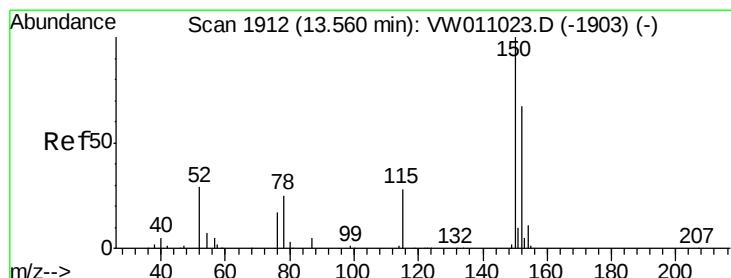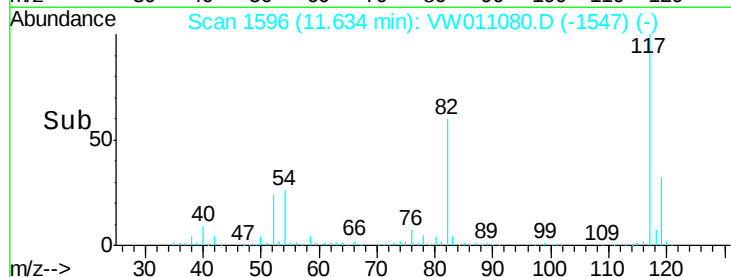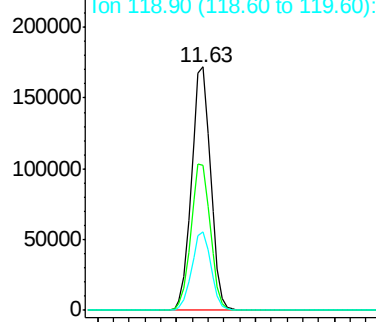

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW011080.D
Acq: 01 Jul 2019 13:08

Tgt Ion:152 Resp: 126061
Ion Ratio Lower Upper
152 100
115 60.0 30.7 92.1
150 156.3 0.0 341.8

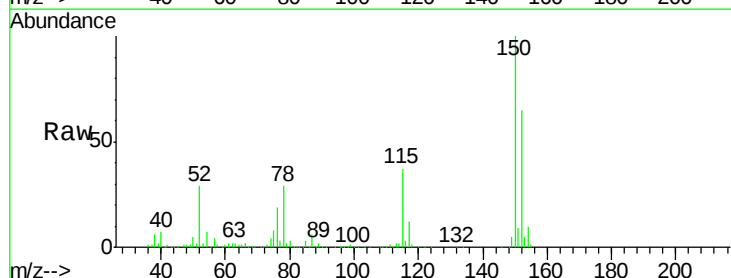

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

