

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW070119\
 Data File : VW011085.D
 Acq On : 01 Jul 2019 15:21
 Operator : SY/VA
 Sample : K3606-01
 Misc : 5.07G/5ML/MSVOA W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 HJDC-GRAB-1

Quant Time: Jul 02 09:08:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jun 28 01:55:46 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	199394	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	341559	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	289688	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	119068	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	140296	53.82	ug/l	0.00
Spiked Amount	50.000		Recovery	=	107.64%	
35) Dibromofluoromethane	7.88	113	106270	50.95	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.90%	
50) Toluene-d8	10.32	98	427899	49.84	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.68%	
62) 4-Bromofluorobenzene	12.62	95	139071	44.29	ug/l	0.00
Spiked Amount	50.000		Recovery	=	88.58%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW070119\
Data File : VW011085.D
Acq On : 01 Jul 2019 15:21
Operator : SY/VA
Sample : K3606-01
Misc : 5.07G/5ML/MSVOA W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
HJDC-GRAB-1

Quant Time: Jul 02 09:08:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W062819S.M
Quant Title : SW846 8260
QLast Update : Fri Jun 28 01:55:46 2019
Response via : Initial Calibration

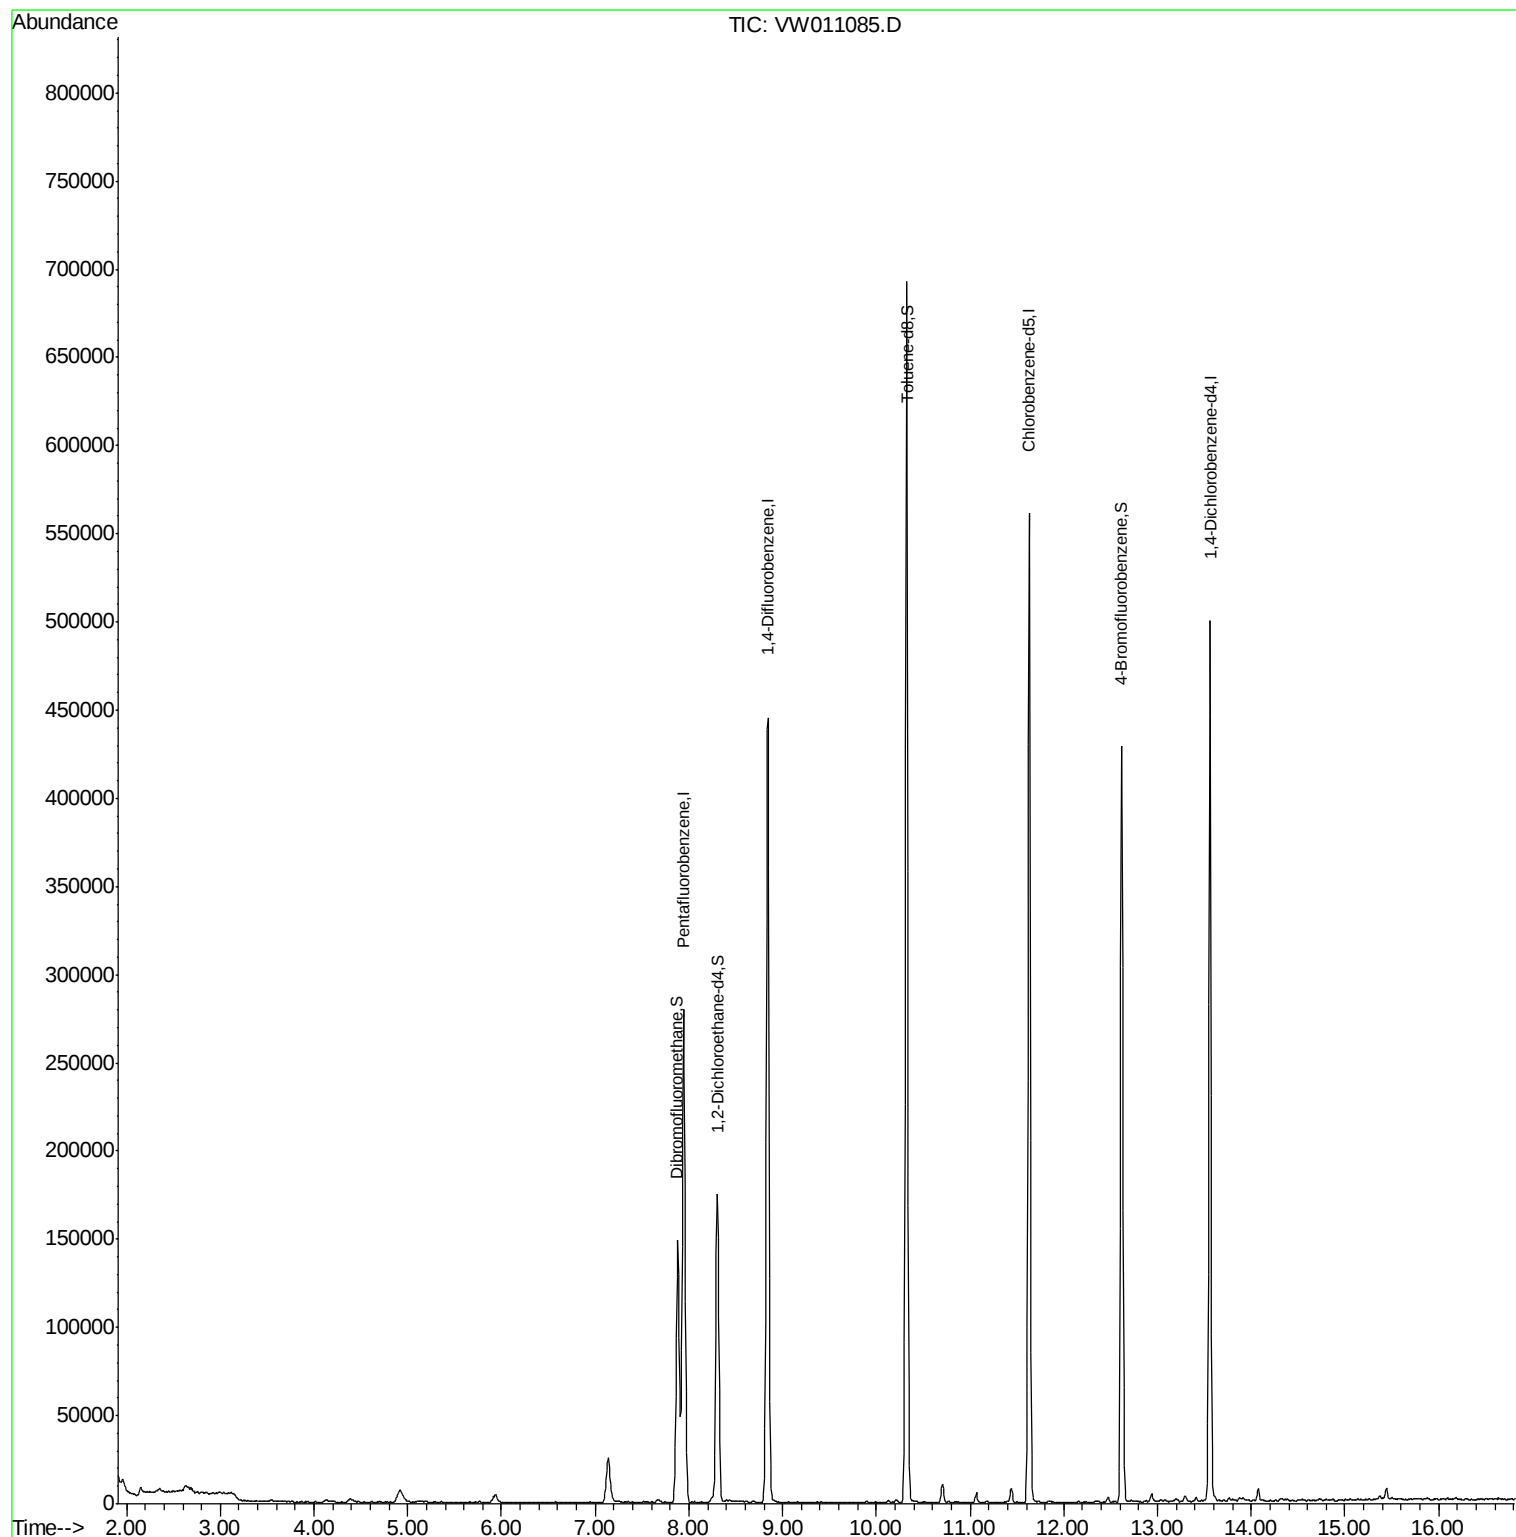

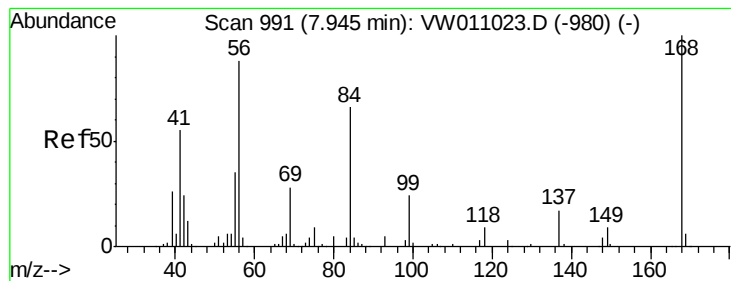

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW011085.D

Acq: 01 Jul 2019 15:21

Instrument :

MSVOA_W

ClientSampleId :


HJDC-GRAB-1

Tot Ion:168 Resp: 199394

Ion Ratio Lower Upper




168 100

99 61.4 47.8 71.6

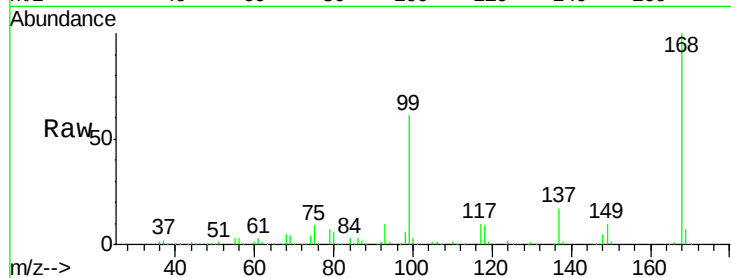

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

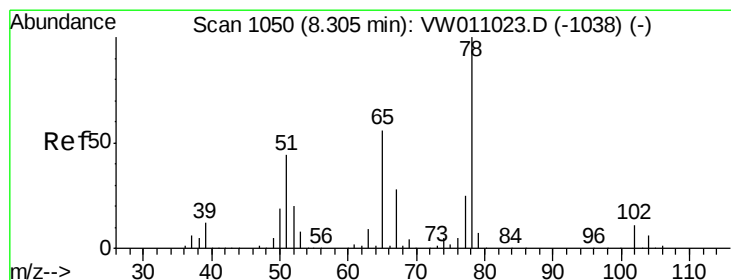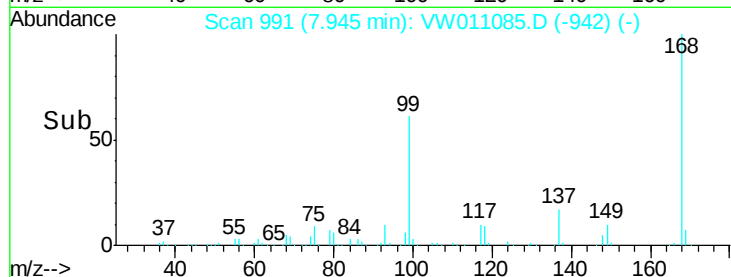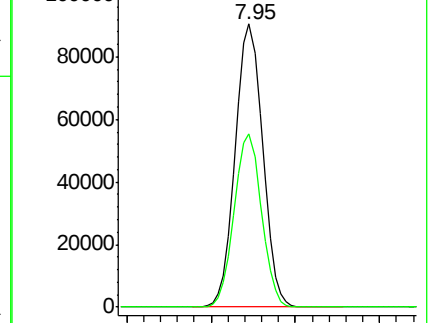

#33

1,2-Dichloroethane-d4

Concen: 53.823 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. 0.00 min

Lab File: VW011085.D


Acq: 01 Jul 2019 15:21

Tgt Ion: 65 Resp: 140296

Ion Ratio Lower Upper



65 100


67 51.9 0.0 102.4

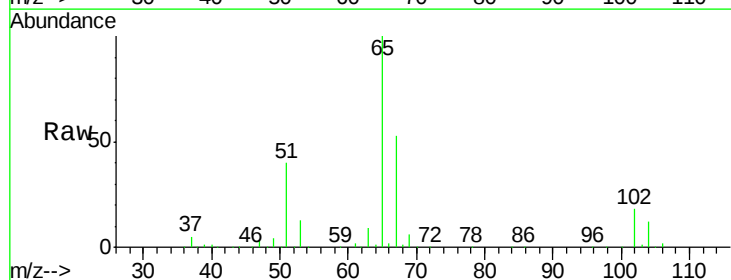

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

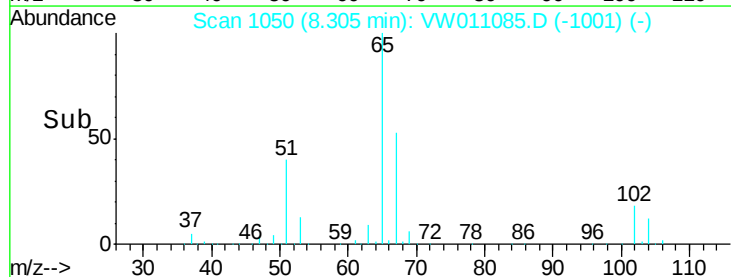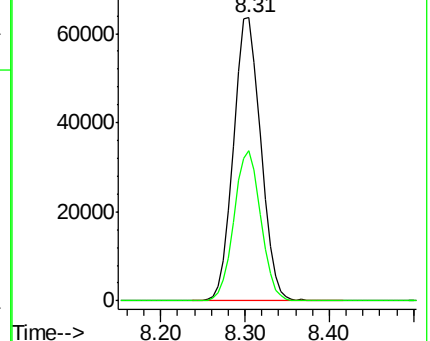

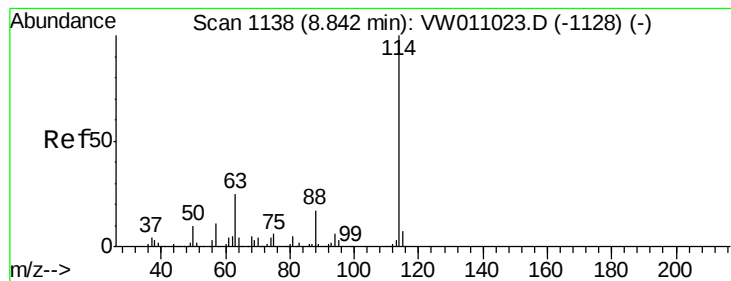

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. 0.00 min

Lab File: VW011085.D

Acq: 01 Jul 2019 15:21

Instrument :

MSVOA_W

ClientSampleId :

HJDC-GRAB-1


Tot Ion:114 Resp: 341559

Ion Ratio Lower Upper

114 100

63 25.1 0.0 50.6




88 17.4 0.0 34.0

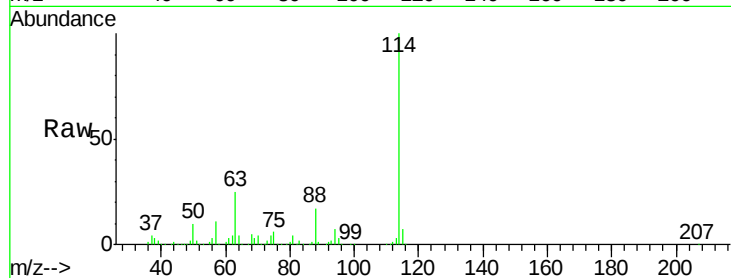

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

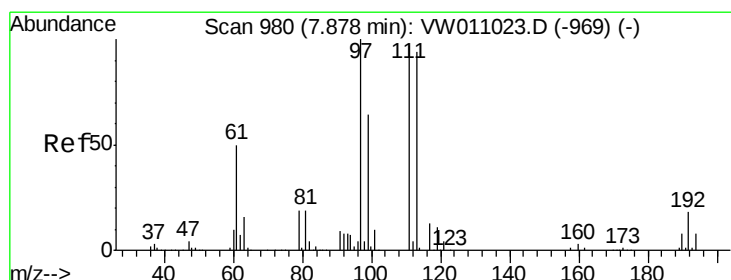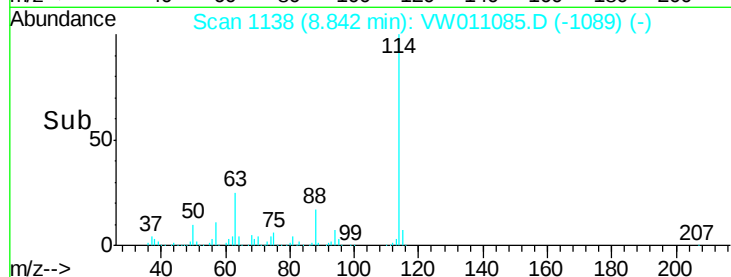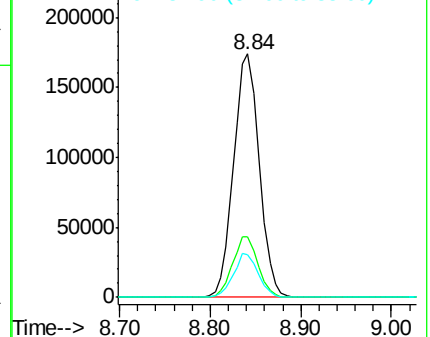

#35

Dibromofluoromethane

Concen: 50.952 ug/l

RT: 7.88 min Scan# 980

Delta R.T. 0.00 min

Lab File: VW011085.D

Acq: 01 Jul 2019 15:21


Tgt Ion:113 Resp: 106270

Ion Ratio Lower Upper

113 100

111 102.9 83.8 125.6



192 19.4 16.0 24.0

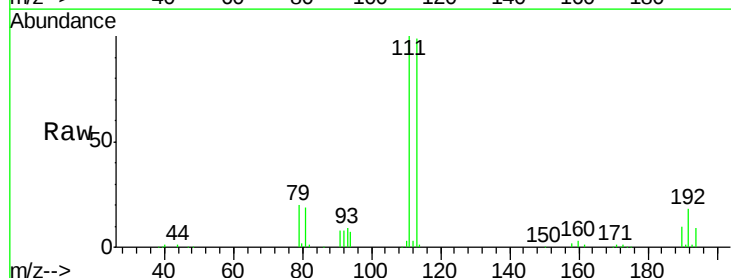


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

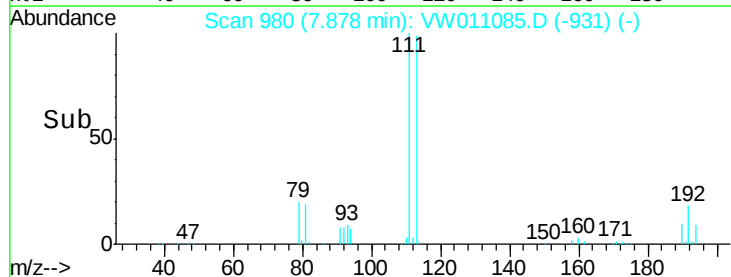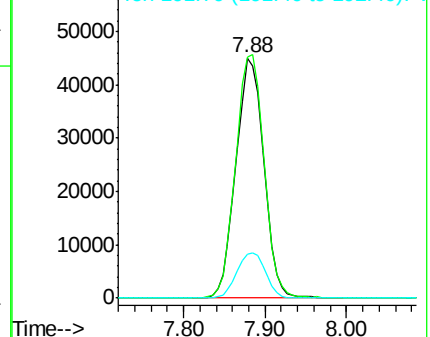

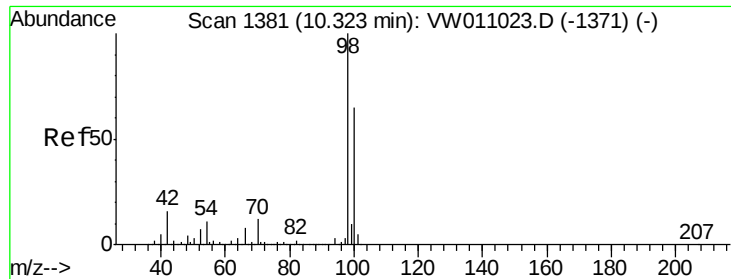

#50

Toluene-d8

Concen: 49.841 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW011085.D

Acq: 01 Jul 2019 15:21

Instrument :

MSVOA_W

ClientSampleId :


HJDC-GRAB-1

Tot Ion: 98 Resp: 427899

Ion Ratio Lower Upper




98 100

100 64.9 52.3 78.5

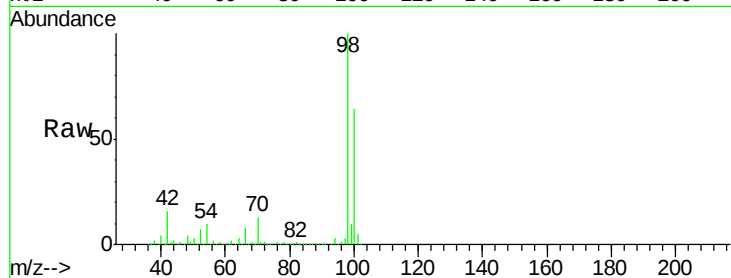

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

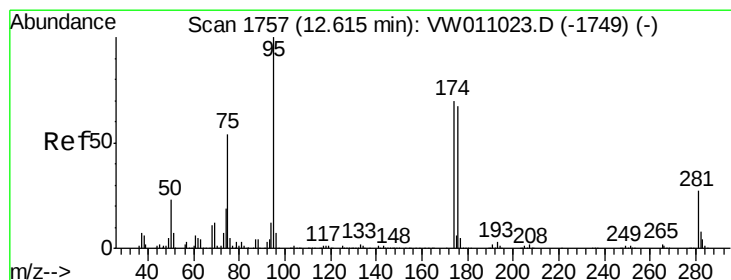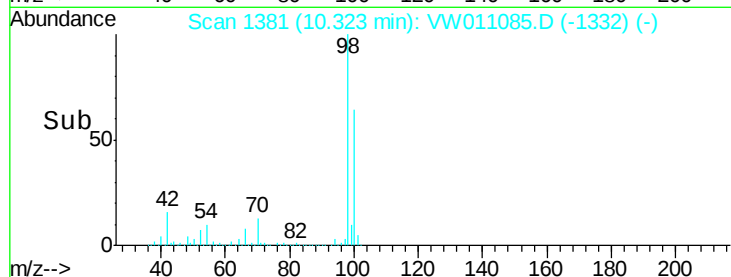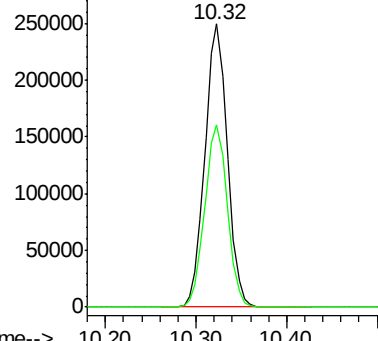

#62

4-Bromofluorobenzene

Concen: 44.289 ug/l

RT: 12.62 min Scan# 1757

Delta R.T. 0.00 min

Lab File: VW011085.D

Acq: 01 Jul 2019 15:21


Tgt Ion: 95 Resp: 139071

Ion Ratio Lower Upper

95 100

174 73.6 0.0 149.2



176 70.0 0.0 143.6

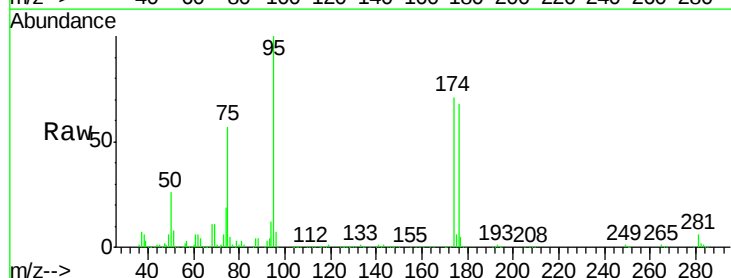


Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

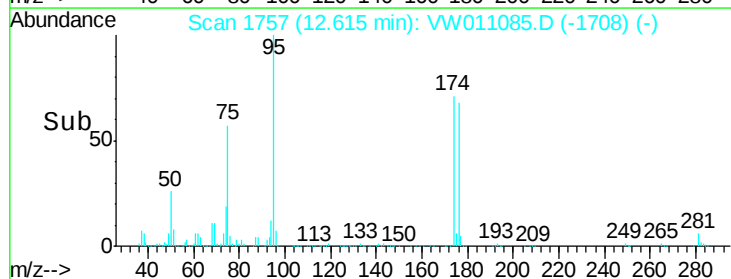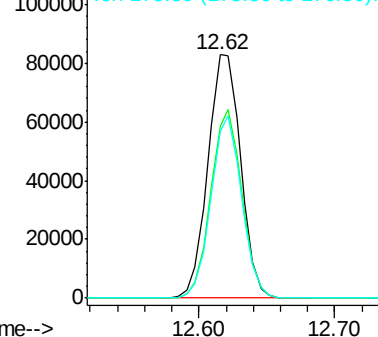


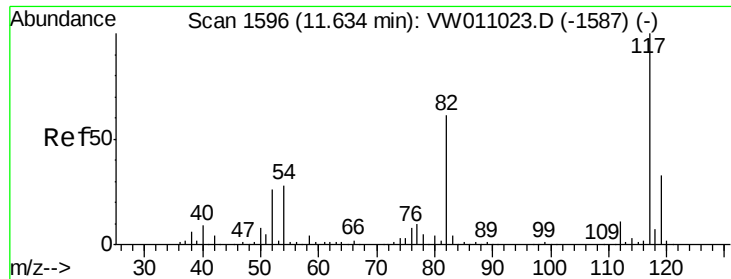




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW011085.D
Acq: 01 Jul 2019 15:21

Instrument :
MSVOA_W
ClientSampleId :
HJDC-GRAB-1

Tot Ion:117 Resp: 289688
Ion Ratio Lower Upper
117 100
82 59.9 48.6 73.0
119 32.1 26.1 39.1

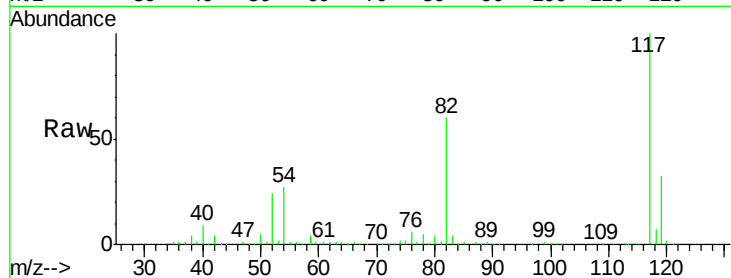


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

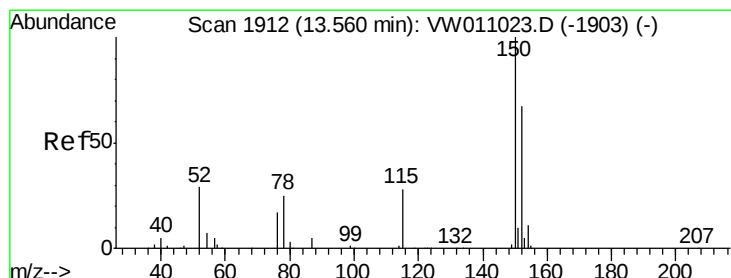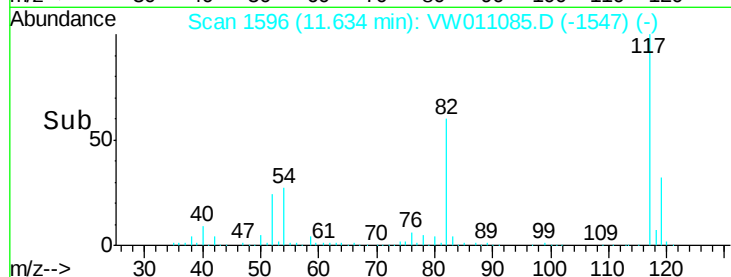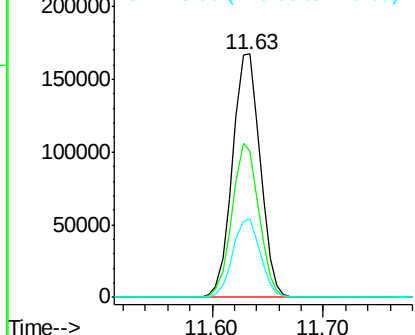

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW011085.D
Acq: 01 Jul 2019 15:21

Tgt Ion:152 Resp: 119068
Ion Ratio Lower Upper
152 100
115 59.7 30.7 92.1
150 155.8 0.0 341.8

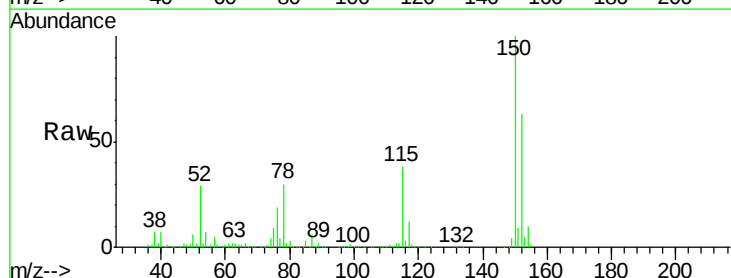

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

