

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070124\
 Data File : VW029427.D
 Acq On : 01 Jul 2024 15:17
 Operator : SY/MD
 Sample : P3088-17
 Misc : 4.68g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 A4D12

Quant Time: Jul 02 08:11:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 29 02:05:50 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	330161	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	196157	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	34002	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	110850	24.257	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.040%
7) Chloroethane-d5	2.899	69	96296	24.953	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.800%
11) 1,1-Dichloroethene-d2	4.021	65	49946	22.637	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	90.560%
21) 2-Butanone-d5	7.075	46	70528	51.585	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.180%
24) Chloroform-d	7.648	84	233773	23.736	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.960%
26) 1,2-Dichloroethane-d4	8.307	65	142925	25.275	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.120%
32) Benzene-d6	8.276	84	429032	36.009	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	144.040%#
36) 1,2-Dichloropropane-d6	9.276	67	148449	39.195	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	156.800%#
41) Toluene-d8	10.325	98	294032	27.893	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	111.560%
43) trans-1,3-Dichloroprop...	10.575	79	38597	25.289	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.160%
47) 2-Hexanone-d5	10.922	63	32164	54.174	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.340%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	75363	25.001	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	28501	24.148	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.600%
Target Compounds						
13) Acetone	4.125	43	4829	4.156	ug/L	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070124\
Data File : VW029427.D
Acq On : 01 Jul 2024 15:17
Operator : SY/MD
Sample : P3088-17
Misc : 4.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
A4D12

Quant Time: Jul 02 08:11:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 29 02:05:50 2024
Response via : Initial Calibration

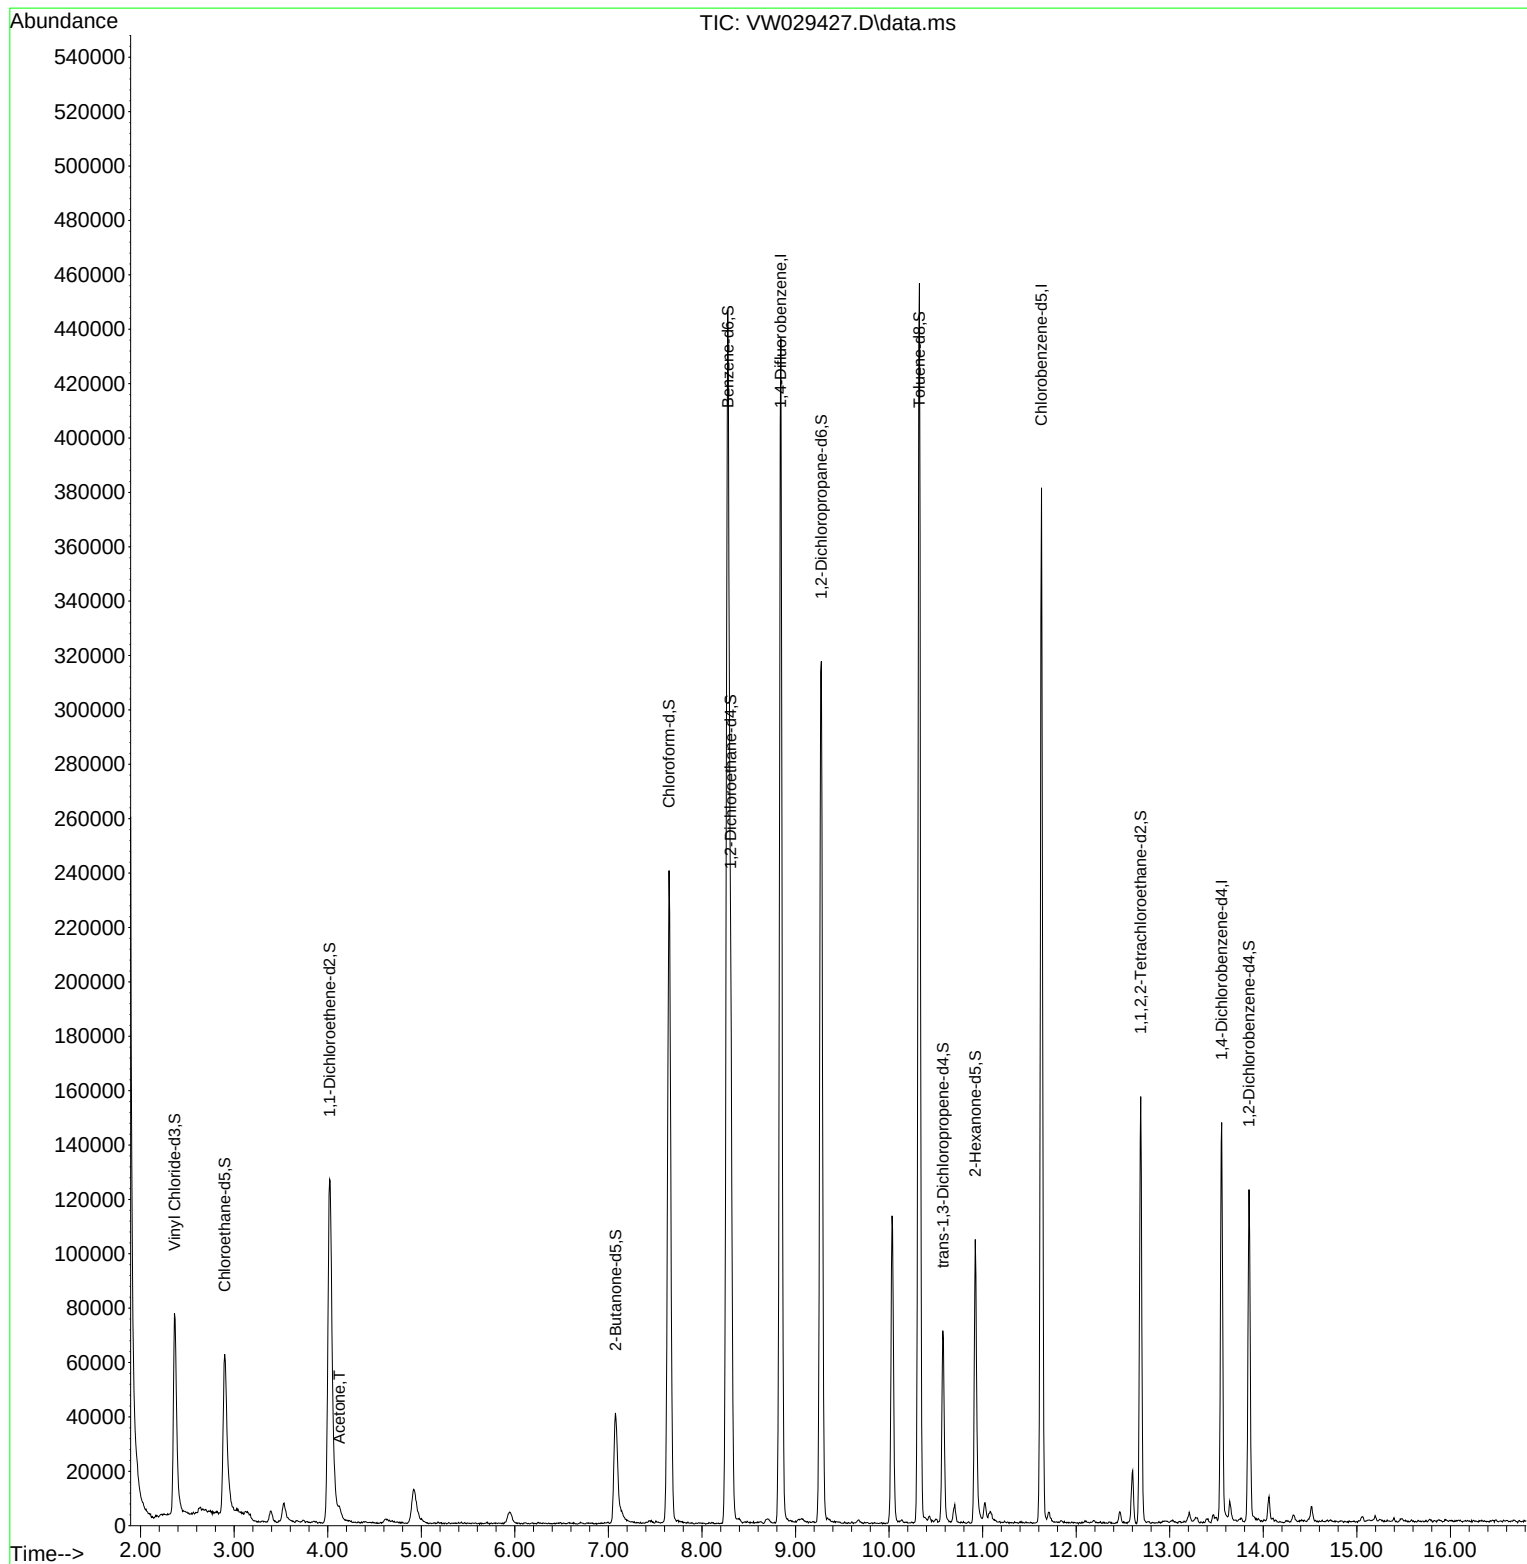

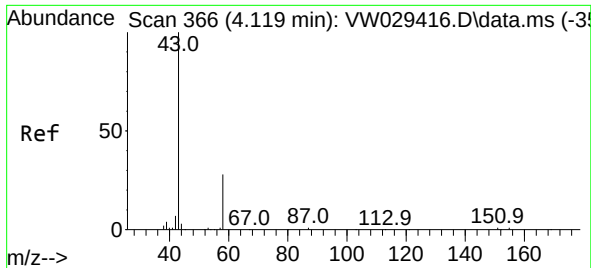

#13
 Acetone
 Concen: 4.156 ug/L
 RT: 4.125 min Scan# 30
 Delta R.T. -0.000 min
 Lab File: VW029427.D
 Acq: 01 Jul 2024 15:17

Instrument :
 MSVOA_W
 ClientSampleId :
 A4D12

Tgt Ion: 43 Resp: 4829
 Ion Ratio Lower Upper
 43 100
 58 17.5 0.0 61.4

