


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW070220\
 Data File : VW015776.D
 Acq On : 02 Jul 2020 09:51
 Operator : SY/VA
 Sample : BFB16
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB16

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062920S.M
 Title : VOC Analysis
 Last Update : Mon Jul 06 01:14:02 2020

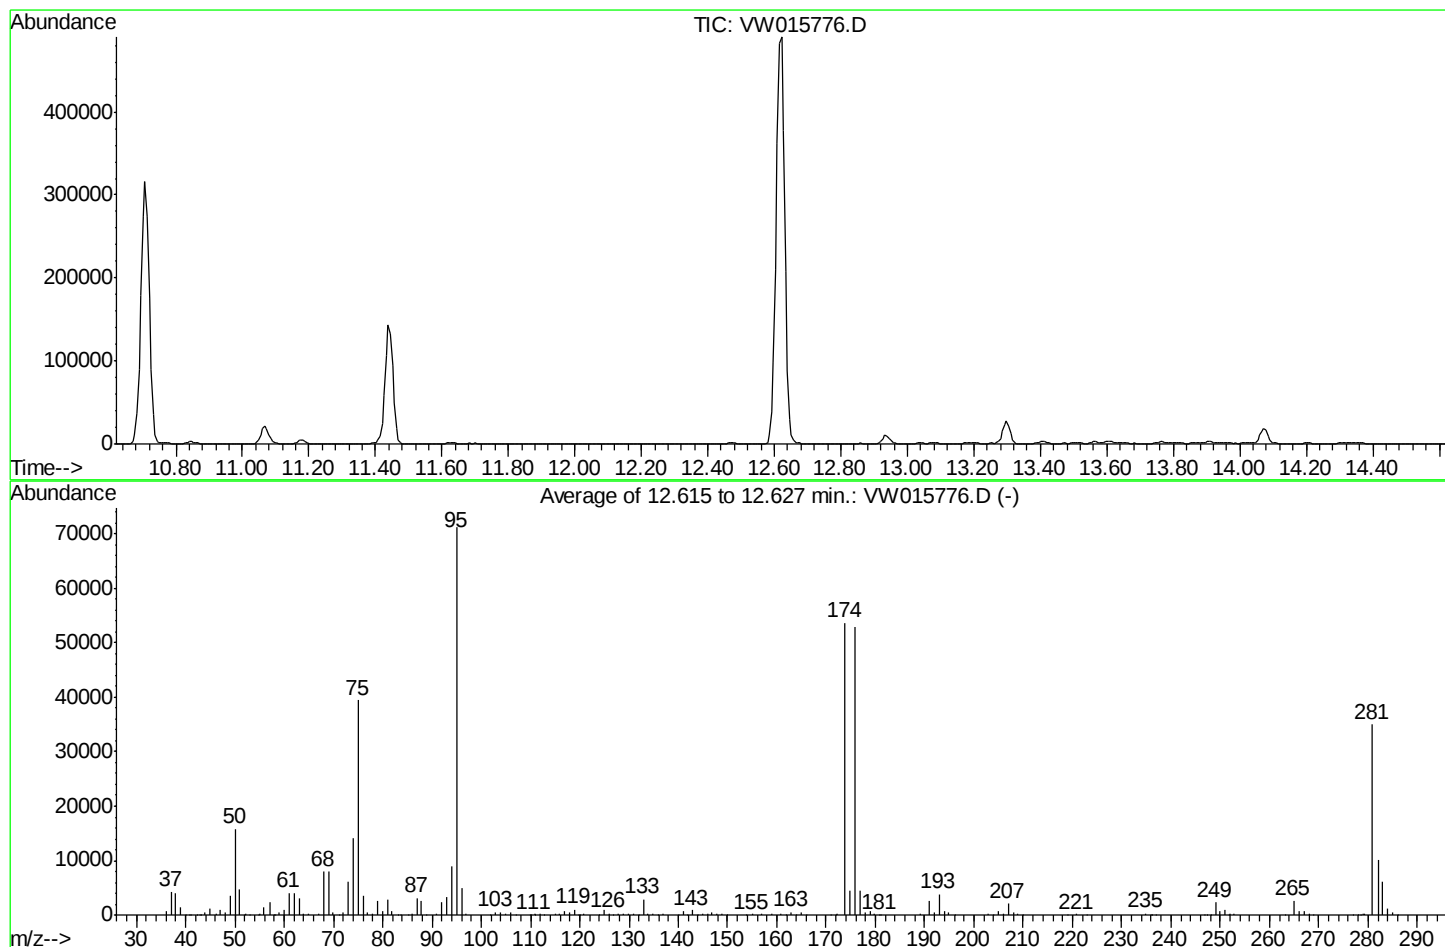

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	15765	PASS
75	95	30	80	55.4	39498	PASS
95	95	100	100	100.0	71234	PASS
96	95	5	9	7.0	4956	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.3	53669	PASS
175	174	5	9	8.2	4419	PASS
176	174	95	101	98.6	52901	PASS
177	176	5	9	8.3	4371	PASS

m/z	Abundance
35.90	949.0
37.00	4506.0
38.00	4414.0
39.00	1501.0
39.90	143.0
40.80	59.0
42.20	52.0
42.90	342.0
44.00	821.0
45.00	1623.0
46.10	168.0
46.90	1025.0
48.00	575.0
49.00	3413.0
50.00	16488.0
51.00	4846.0
52.10	194.0
53.10	57.0
54.80	268.0
56.00	1493.0
57.00	2501.0
57.90	148.0
59.00	886.0
60.00	894.0
61.00	4525.0
62.00	4009.0
63.00	3018.0
63.90	351.0
65.00	255.0
66.90	240.0
68.00	7755.0
69.00	8241.0
69.90	600.0
71.10	114.0
72.00	460.0
73.00	8045.0
74.00	14036.0
75.00	39112.0
76.00	3406.0
77.00	543.0
77.90	331.0
78.90	2636.0
79.90	745.0
80.90	2791.0
81.90	651.0
83.20	125.0
83.60	133.0
85.10	143.0
85.90	125.0
86.90	3437.0
87.90	2858.0
88.90	313.0
90.90	387.0
91.90	2226.0
93.00	3296.0
94.00	8626.0
95.00	69760.0
96.00	5257.0
97.00	211.0
101.80	70.0
102.90	775.0
103.90	636.0
104.90	329.0
105.80	318.0
106.90	98.0
109.80	296.0
110.80	335.0
112.00	250.0
112.70	102.0
115.00	373.0
115.80	342.0
116.90	712.0
118.00	686.0
118.90	1318.0
120.00	182.0
120.90	184.0
124.00	96.0
125.00	1278.0
125.90	474.0
127.90	249.0
128.80	184.0
129.80	239.0
131.00	254.0
131.90	169.0
133.00	4732.0
134.90	425.0
135.80	74.0
136.80	165.0
140.00	78.0
140.90	719.0
142.00	136.0
142.80	836.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

144.00	67.0
144.80	169.0
145.80	169.0
146.90	630.0
147.80	209.0
148.90	274.0
149.80	65.0
154.90	190.0
156.90	166.0
158.80	163.0
160.90	363.0
161.80	150.0
162.90	908.0
163.90	177.0
164.90	564.0
165.90	125.0
171.90	373.0
173.90	50568.0
174.90	3949.0
175.90	45712.0
176.90	4543.0
177.90	531.0
178.90	1351.0
179.80	224.0
180.80	129.0
181.00	129.0
189.00	421.0
190.90	4226.0
192.00	957.0
192.90	6027.0
194.00	911.0
194.90	681.0
196.10	89.0
203.00	547.0
204.80	1090.0
206.00	265.0
207.00	3402.0
208.00	733.0
209.00	403.0
210.00	112.0
219.00	147.0
220.80	202.0
223.00	58.0
235.00	428.0
235.90	160.0
237.00	120.0
246.80	96.0
249.00	3144.0
249.90	869.0
250.90	1293.0
252.00	315.0
252.80	172.0
263.10	54.0
264.90	4053.0
265.90	1201.0
266.90	1089.0
268.10	253.0
268.90	94.0
276.90	102.0
278.90	430.0
281.00	48968.0
282.00	13419.0
283.00	8503.0
284.00	1809.0
285.00	533.0
285.90	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

m/z	Abundance
36.00	824.0
37.00	4744.0
38.00	4320.0
39.00	1572.0
40.00	239.0
43.10	188.0
44.00	924.0
45.00	1293.0
46.20	102.0
47.00	884.0
48.00	552.0
49.00	4108.0
50.00	16984.0
51.00	5533.0
52.20	293.0
53.00	66.0
55.00	264.0
55.90	1399.0
57.00	2609.0
57.90	110.0
59.10	448.0
60.00	1011.0
60.90	4395.0
62.00	4546.0
63.00	3449.0
64.00	404.0
65.00	258.0
67.00	214.0
68.00	8839.0
69.00	9193.0
70.00	633.0
71.90	538.0
73.00	6558.0
74.00	16172.0
75.00	45208.0
76.00	3846.0
76.90	522.0
77.90	296.0
78.90	2826.0
79.90	890.0
80.90	3165.0
81.90	724.0
83.00	115.0
86.00	180.0
86.90	3457.0
87.90	2787.0
90.90	359.0
91.90	2755.0
93.00	3803.0
94.00	9621.0
95.00	79456.0
96.00	5712.0
96.80	212.0
103.00	556.0
104.00	515.0
104.90	203.0
105.80	452.0
107.00	84.0
110.10	185.0
111.00	235.0
111.80	166.0
112.70	87.0
114.90	319.0
115.90	359.0
116.90	617.0
118.00	564.0
118.90	1070.0
119.70	58.0
120.90	140.0
124.00	67.0
124.90	816.0
125.80	301.0
127.80	350.0
128.90	195.0
129.80	326.0
130.90	246.0
133.00	2892.0
133.80	740.0
134.90	377.0
136.70	156.0
139.80	69.0
140.90	618.0
141.80	135.0
142.90	898.0
143.90	83.0
144.90	192.0
145.90	154.0
146.80	306.0
147.90	225.0
148.90	125.0
149.80	63.0
153.70	57.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

154.90	193.0
156.90	154.0
158.90	149.0
160.80	235.0
162.90	463.0
163.80	95.0
165.00	382.0
166.00	72.0
171.00	94.0
172.10	490.0
173.90	57200.0
174.90	4542.0
175.90	58120.0
176.90	4532.0
177.90	394.0
179.00	747.0
179.90	115.0
181.00	87.0
189.00	268.0
191.00	2479.0
192.90	3791.0
194.00	627.0
194.90	500.0
202.90	288.0
204.00	63.0
204.90	687.0
206.10	182.0
207.00	2006.0
207.90	423.0
208.90	278.0
218.80	82.0
220.90	171.0
234.90	395.0
236.10	87.0
236.90	117.0
247.20	51.0
249.00	2500.0
250.00	709.0
250.90	1009.0
252.00	262.0
252.90	221.0
265.00	2524.0
266.00	778.0
267.00	822.0
267.90	174.0
268.90	82.0
278.40	112.0
279.20	309.0
281.00	36680.0
282.00	11213.0
283.00	6238.0
284.00	1217.0
285.00	382.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

m/z	Abundance
36.00	625.0
37.00	3512.0
38.00	3072.0
39.00	1324.0
39.90	123.0
41.10	58.0
43.00	126.0
44.00	655.0
45.00	740.0
46.10	124.0
46.90	759.0
47.90	514.0
49.00	3029.0
50.00	13825.0
51.00	4101.0
51.90	105.0
54.90	268.0
55.90	1027.0
57.00	2205.0
58.10	134.0
59.00	186.0
59.90	705.0
61.00	3214.0
62.00	3405.0
63.00	2605.0
64.10	282.0
65.00	155.0
67.00	160.0
68.00	7202.0
69.00	6851.0
70.00	552.0
71.20	92.0
72.00	327.0
73.00	3776.0
74.00	11836.0
75.00	34176.0
76.00	3050.0
77.00	408.0
77.70	171.0
78.90	2338.0
79.90	690.0
80.90	2451.0
81.90	596.0
83.00	105.0
85.80	169.0
86.90	2462.0
87.90	2304.0
90.90	288.0
92.00	2078.0
93.00	3097.0
94.00	8428.0
95.00	64488.0
96.00	3900.0
96.80	115.0
102.80	179.0
103.90	338.0
104.90	205.0
105.90	327.0
106.90	81.0
110.10	152.0
110.80	226.0
111.90	58.0
114.90	131.0
115.80	262.0
116.90	545.0
117.90	418.0
119.00	538.0
120.90	82.0
124.90	446.0
125.90	149.0
126.80	79.0
127.90	267.0
128.90	145.0
129.80	334.0
130.90	145.0
132.00	73.0
133.00	1053.0
133.90	283.0
134.90	255.0
136.90	83.0
141.00	585.0
141.90	81.0
142.90	808.0
143.80	73.0
144.90	109.0
146.00	161.0
146.90	216.0
147.80	184.0
148.80	131.0
149.80	127.0
153.80	51.0
155.00	161.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

156.80	145.0
158.80	139.0
160.90	190.0
162.70	163.0
164.90	239.0
171.00	66.0
172.10	347.0
173.90	53240.0
174.90	4766.0
175.90	54872.0
176.90	4038.0
177.90	233.0
178.90	347.0
179.90	135.0
188.90	93.0
190.90	1289.0
192.00	380.0
192.90	1698.0
194.00	336.0
194.90	174.0
202.80	198.0
204.80	270.0
206.00	112.0
206.90	908.0
208.00	268.0
209.00	156.0
221.00	112.0
234.90	155.0
248.00	72.0
249.00	1178.0
249.90	274.0
250.90	592.0
251.70	90.0
252.00	104.0
265.00	1470.0
266.00	376.0
266.90	357.0
267.90	71.0
277.90	53.0
279.20	161.0
281.00	19584.0
282.00	5622.0
283.00	3345.0
284.10	434.0
284.80	218.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16

Scan 1750 (12.573 min): VW015776.D
BFB16

m/z	Abundance
39.70	80.0
40.00	87.0
43.00	52.0
43.90	279.0
73.10	91.0
132.90	51.0
280.90	97.0
282.10	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB16