


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW070318\
 Data File : VW003687.D
 Acq On : 03 Jul 2018 09:36
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070218S.M
 Title : SW846 8260
 Last Update : Tue Jul 03 08:55:34 2018

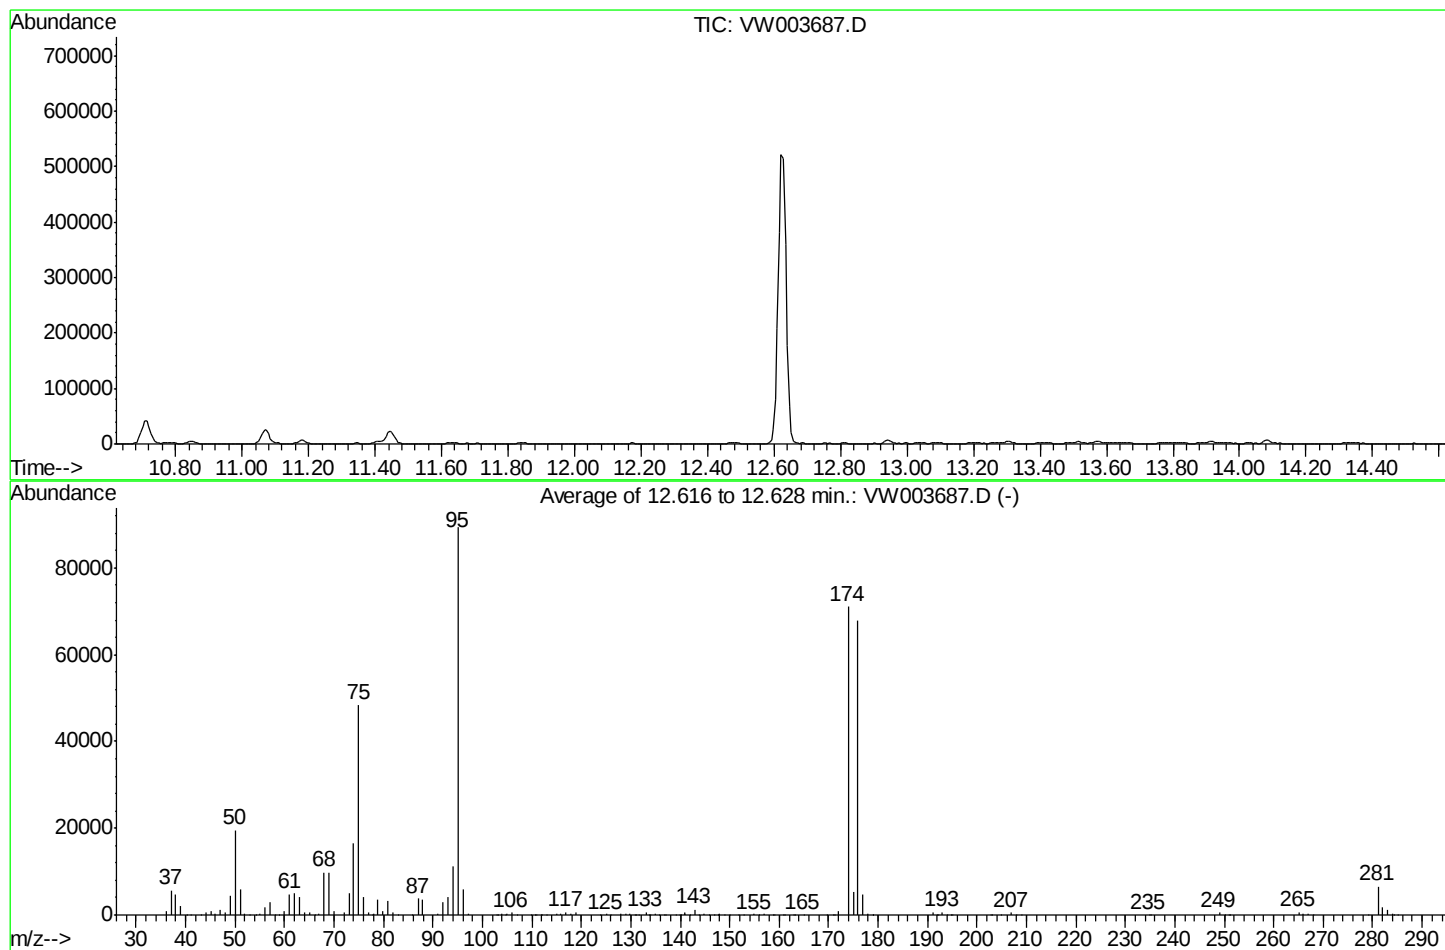

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	19513	PASS
75	95	30	60	54.2	48464	PASS
95	95	100	100	100.0	89349	PASS
96	95	5	9	6.7	6003	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.6	71088	PASS
175	174	5	9	7.6	5434	PASS
176	174	95	101	95.4	67786	PASS
177	176	5	9	7.0	4718	PASS