


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW070620\
 Data File : VW015781.D
 Acq On : 06 Jul 2020 09:25
 Operator : SY/VA
 Sample : BFB17
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB17

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062920S.M
 Title : VOC Analysis
 Last Update : Tue Jul 07 00:28:21 2020

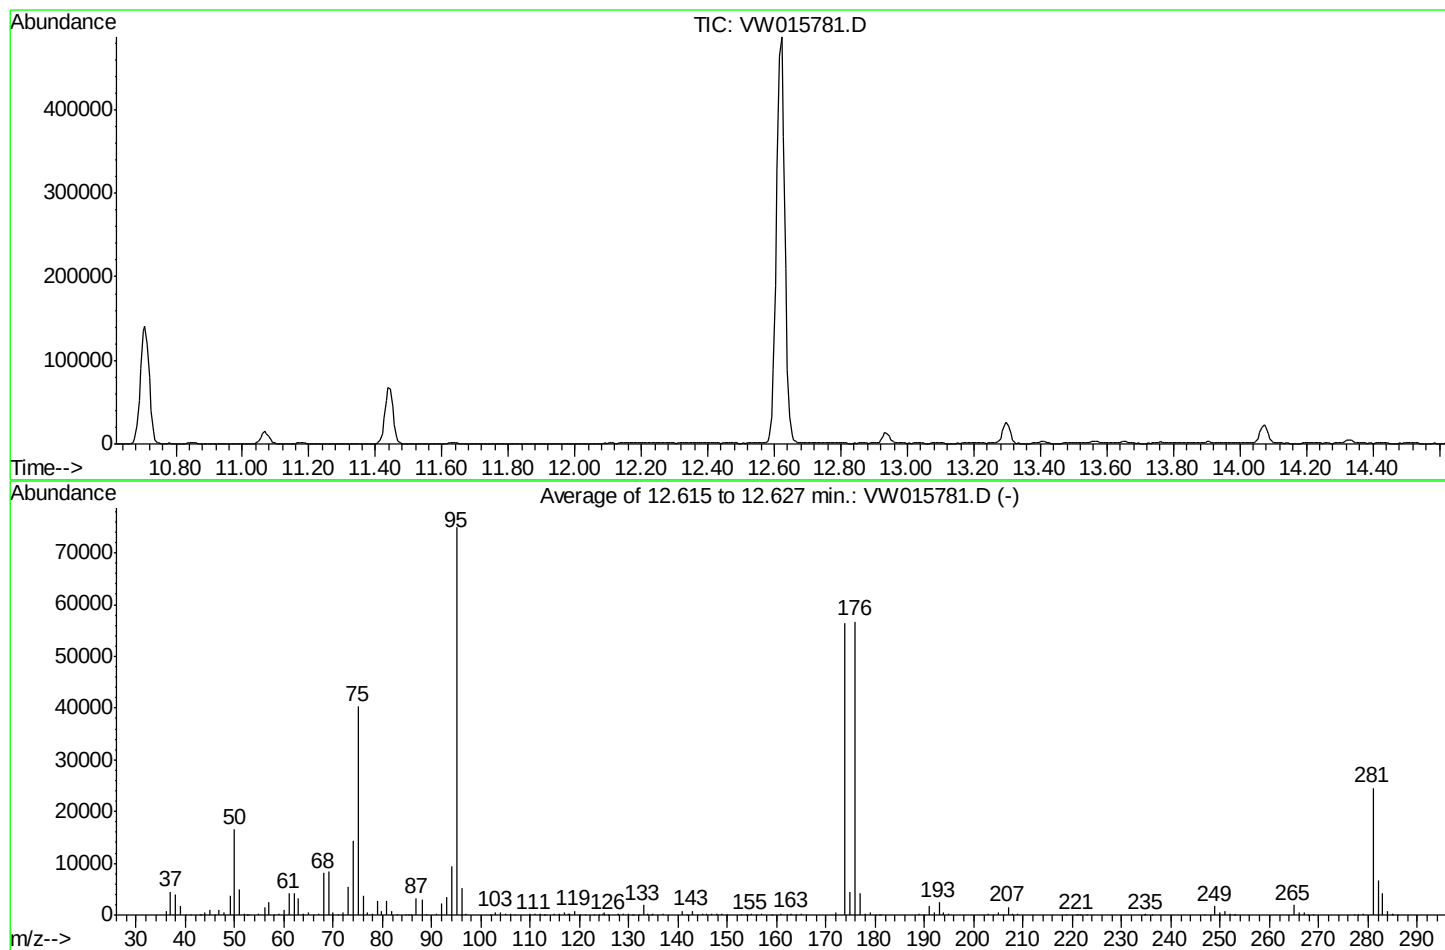

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	16562	PASS
75	95	30	80	53.8	40280	PASS
95	95	100	100	100.0	74928	PASS
96	95	5	9	7.0	5227	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.3	56434	PASS
175	174	5	9	7.8	4397	PASS
176	174	95	101	100.4	56680	PASS
177	176	5	9	7.5	4226	PASS

m/z	Abundance
36.00	1264.0
37.00	4938.0
38.00	4062.0
39.00	1869.0
39.90	169.0
41.00	113.0
42.00	54.0
42.90	237.0
44.00	814.0
45.00	1258.0
46.00	157.0
46.90	1126.0
47.90	605.0
49.00	3937.0
50.00	17384.0
51.00	5361.0
52.00	256.0
54.90	283.0
56.00	1401.0
57.00	2493.0
58.00	162.0
59.00	537.0
59.90	844.0
61.00	4222.0
62.00	4290.0
63.00	3371.0
64.00	438.0
64.90	509.0
65.90	59.0
67.00	289.0
68.00	8217.0
69.00	9202.0
70.00	612.0
70.90	102.0
71.90	626.0
73.00	6722.0
74.00	14788.0
75.00	41232.0
76.00	3628.0
76.90	621.0
78.00	467.0
78.90	2766.0
79.90	857.0
80.90	2791.0
81.80	604.0
82.90	165.0
84.80	100.0
85.90	113.0
86.90	3091.0
87.90	3116.0
88.90	195.0
90.80	333.0
92.00	2134.0
93.00	3636.0
94.00	9006.0
95.00	74816.0
96.00	5347.0
97.00	207.0
101.90	52.0
102.90	805.0
103.90	545.0
104.80	310.0
105.90	367.0
106.80	69.0
109.80	209.0
110.90	298.0
111.90	186.0
113.10	94.0
114.80	257.0
115.80	290.0
116.90	574.0
117.70	552.0
118.90	1006.0
119.90	127.0
121.00	127.0
122.90	66.0
123.90	56.0
124.80	969.0
125.10	917.0
127.70	239.0
128.80	181.0
129.80	283.0
130.80	177.0
133.00	3209.0
134.70	331.0
136.90	179.0
140.90	662.0
141.90	97.0
142.90	889.0
144.90	230.0
145.80	129.0
146.90	450.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17

147.80	259.0
148.80	270.0
149.90	154.0
153.80	58.0
154.80	193.0
156.90	113.0
159.00	85.0
161.00	233.0
162.00	76.0
162.90	557.0
164.00	83.0
164.90	351.0
165.90	67.0
172.00	564.0
173.90	50680.0
174.90	4314.0
175.90	52008.0
176.90	4105.0
177.90	388.0
178.90	869.0
180.00	129.0
180.80	82.0
188.90	372.0
190.00	178.0
191.00	2583.0
192.00	605.0
192.90	3561.0
194.00	630.0
194.90	517.0
203.00	321.0
204.00	80.0
204.90	693.0
206.00	180.0
207.00	2315.0
207.90	469.0
208.80	340.0
218.70	92.0
221.00	149.0
221.70	88.0
222.90	56.0
235.00	418.0
236.10	68.0
246.90	92.0
248.90	2502.0
249.90	585.0
250.90	1051.0
251.90	351.0
253.00	128.0
265.00	2572.0
266.00	730.0
267.00	671.0
267.90	176.0
268.80	70.0
277.20	96.0
278.00	82.0
278.90	321.0
281.00	35456.0
282.00	8897.0
283.00	5723.0
283.90	1218.0
284.90	405.0
285.90	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17

m/z	Abundance
36.00	1047.0
37.00	5203.0
38.00	4335.0
39.00	1688.0
39.90	212.0
41.20	52.0
43.10	147.0
44.00	899.0
45.00	1086.0
45.90	103.0
46.90	967.0
47.90	671.0
49.00	4021.0
50.00	18432.0
51.00	5623.0
52.00	202.0
52.60	71.0
54.90	346.0
56.00	1754.0
57.00	2780.0
57.90	116.0
59.00	302.0
60.00	1078.0
61.00	4617.0
62.00	4747.0
63.00	3786.0
64.00	371.0
65.00	473.0
66.00	65.0
67.00	216.0
68.00	9074.0
69.00	9307.0
69.90	653.0
71.90	704.0
73.00	6007.0
74.00	15749.0
75.00	45032.0
76.00	3979.0
77.00	526.0
78.00	368.0
78.90	2976.0
79.90	846.0
80.90	3079.0
81.90	770.0
82.80	140.0
85.10	91.0
85.80	123.0
86.90	3664.0
88.00	3135.0
90.90	383.0
92.00	2592.0
93.00	3824.0
94.00	10481.0
95.00	83440.0
96.00	5671.0
97.00	198.0
103.00	442.0
103.80	465.0
104.90	219.0
106.00	337.0
106.80	73.0
109.80	146.0
111.00	250.0
111.70	115.0
112.00	125.0
112.70	138.0
114.90	255.0
115.80	372.0
116.80	702.0
117.90	486.0
118.90	816.0
119.90	86.0
120.90	105.0
125.00	550.0
125.80	251.0
127.90	357.0
128.90	180.0
129.80	312.0
131.00	176.0
131.90	66.0
133.00	1811.0
133.80	472.0
134.90	395.0
136.70	189.0
140.90	887.0
142.00	146.0
142.80	923.0
144.70	131.0
145.80	163.0
146.80	299.0
147.80	237.0
148.80	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17

149.90	110.0
152.80	72.0
154.80	267.0
155.90	60.0
156.80	139.0
158.90	123.0
160.90	233.0
162.00	67.0
163.00	331.0
164.00	72.0
164.80	255.0
165.90	51.0
171.90	650.0
173.90	65424.0
174.90	4930.0
175.90	62568.0
176.90	5009.0
177.80	263.0
178.90	609.0
181.00	59.0
188.80	132.0
189.80	131.0
190.90	1724.0
191.90	408.0
192.90	2660.0
193.80	382.0
194.80	289.0
202.80	265.0
205.00	554.0
207.00	1680.0
207.90	301.0
208.90	209.0
218.70	81.0
220.80	65.0
234.80	209.0
248.90	1695.0
249.90	460.0
250.90	772.0
252.00	181.0
252.90	89.0
264.90	2165.0
265.90	607.0
267.00	437.0
268.00	108.0
278.90	194.0
281.00	25928.0
282.00	7623.0
283.00	4614.0
284.00	758.0
285.10	176.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17

m/z	Abundance
36.00	968.0
37.00	3477.0
38.00	3388.0
39.00	1350.0
40.10	152.0
41.10	58.0
42.70	56.0
44.00	613.0
44.90	851.0
46.00	97.0
46.90	794.0
48.00	381.0
49.00	3017.0
50.00	13872.0
51.00	3993.0
52.00	173.0
52.80	59.0
55.00	210.0
56.00	1093.0
57.00	2084.0
58.00	87.0
58.90	176.0
59.90	751.0
61.00	3728.0
62.00	3542.0
63.00	2606.0
64.00	318.0
64.90	364.0
66.00	81.0
67.00	244.0
67.90	7208.0
69.00	6918.0
70.00	595.0
72.00	404.0
73.00	3991.0
74.00	12468.0
75.00	34576.0
76.00	3201.0
76.90	446.0
77.90	293.0
78.90	2321.0
79.80	730.0
80.90	2530.0
81.80	590.0
82.80	85.0
85.90	108.0
86.90	2765.0
87.90	2733.0
90.80	298.0
92.00	1899.0
93.00	3104.0
94.00	8463.0
95.00	66528.0
96.00	4665.0
97.00	137.0
102.90	251.0
103.80	349.0
104.80	121.0
105.80	356.0
106.90	88.0
109.80	91.0
110.80	136.0
111.80	151.0
112.80	84.0
114.90	182.0
115.90	226.0
116.90	561.0
117.90	375.0
118.90	538.0
123.80	57.0
124.90	239.0
127.70	254.0
128.80	116.0
129.80	284.0
130.80	95.0
132.90	812.0
134.80	233.0
136.80	120.0
140.90	681.0
141.80	112.0
142.80	661.0
143.80	82.0
144.80	205.0
145.90	148.0
146.90	163.0
147.80	212.0
148.80	104.0
150.00	81.0
152.80	60.0
154.00	59.0
154.80	175.0
156.00	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17

156.90	166.0
158.90	110.0
160.80	144.0
162.80	173.0
165.00	83.0
171.90	493.0
173.90	53200.0
174.90	3949.0
175.90	55464.0
176.90	3565.0
178.00	216.0
178.90	312.0
188.70	92.0
190.90	988.0
191.90	176.0
192.90	1112.0
193.90	258.0
194.90	123.0
203.00	132.0
204.90	184.0
205.90	70.0
207.00	715.0
208.00	119.0
208.90	113.0
220.70	64.0
234.70	108.0
248.90	723.0
249.90	180.0
250.90	441.0
251.90	76.0
252.70	62.0
264.90	1052.0
265.90	265.0
267.00	324.0
267.80	56.0
280.90	12189.0
282.00	3760.0
282.90	2167.0
284.00	381.0
285.00	169.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17

Scan 1749 (12.567 min): VW015781.D
BFB17

m/z	Abundance
36.00	297.0
37.90	84.0
40.00	146.0
41.00	93.0
42.00	53.0
43.80	226.0

Instrument :
MSVOA_W
ClientSampleId :
BFB17