




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070722\
Data File : VW023581.D
Acq On : 07 Jul 2022 18:21
Operator : SY/VA
Sample : N3626-05
Misc : 5.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZC1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/08/2022
Supervised By :Mahesh Dadoda 07/08/2022

Quant Time: Jul 08 01:48:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 08 01:46:16 2022
Response via : Initial Calibration

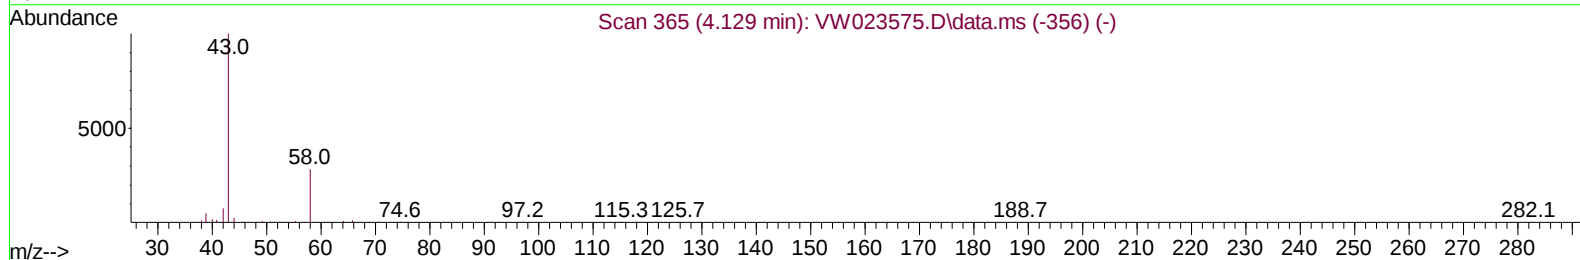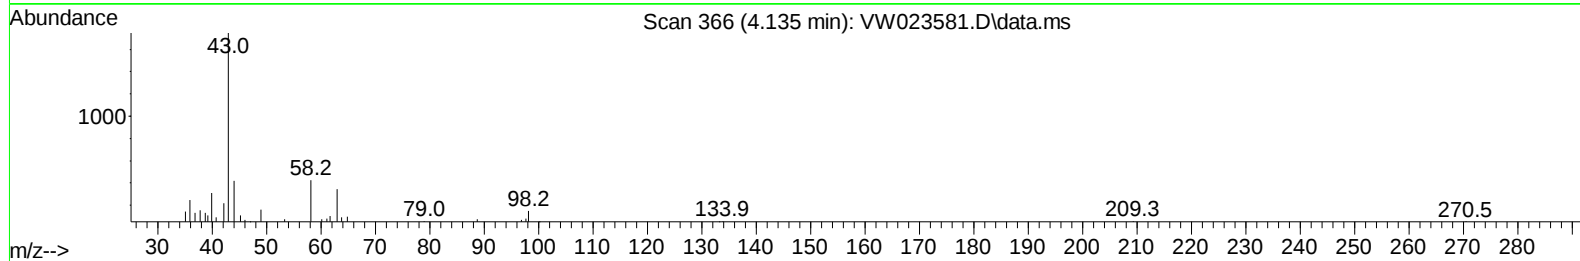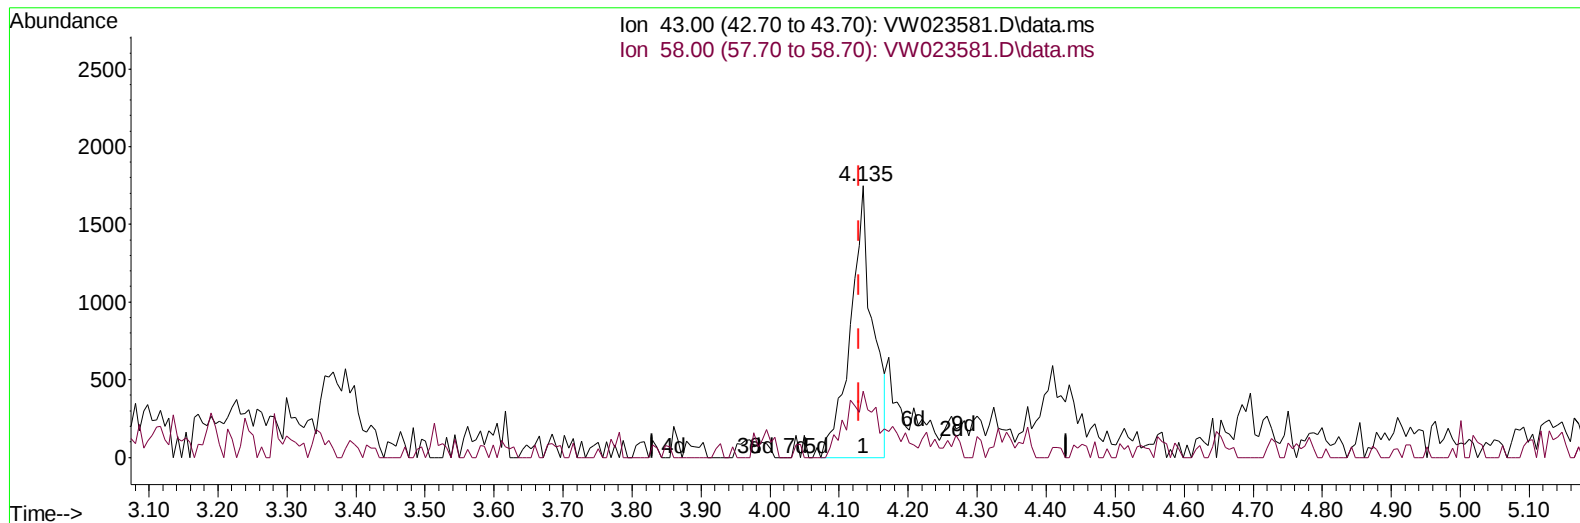

TIC: VW023581.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 4.13 ug/L

response 3914

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.60	9.56
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070722\
 Data File : VW023581.D
 Acq On : 07 Jul 2022 18:21
 Operator : SY/VA
 Sample : N3626-05
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZC1

Manual IntegrationsAPPROVED

Quant Time: Jul 08 01:48:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 08 01:46:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/08/2022
 Supervised By :Mahesh Dadoda 07/08/2022

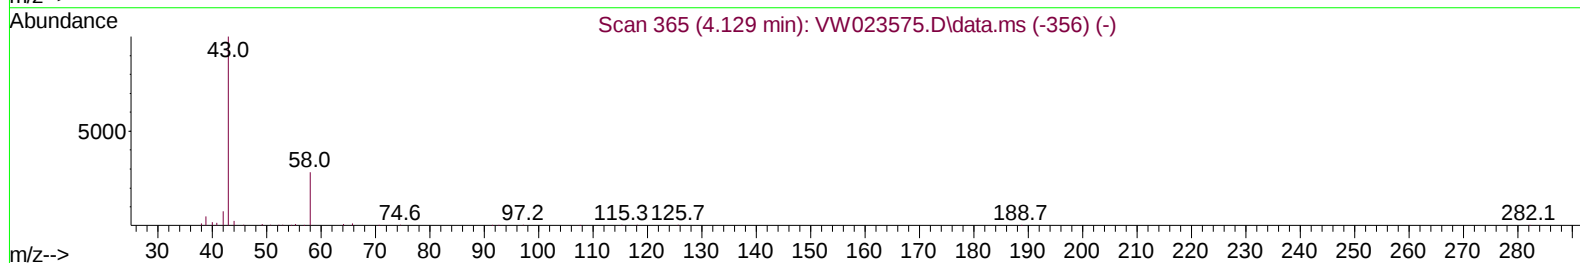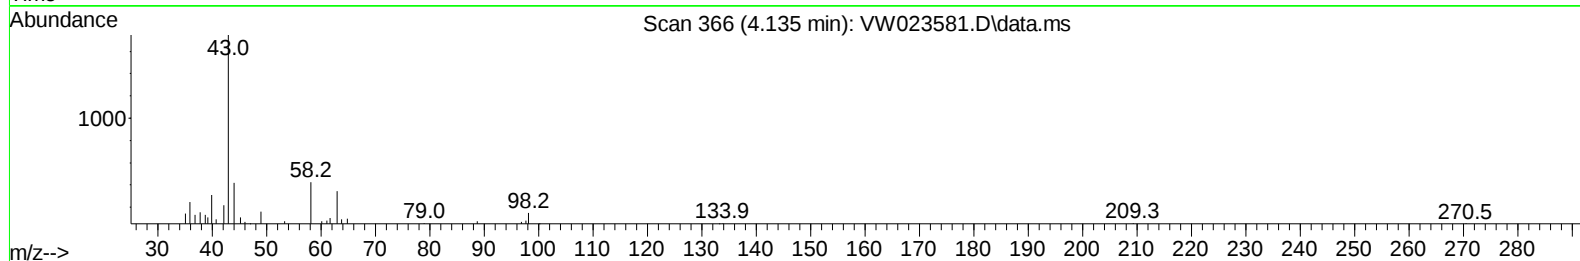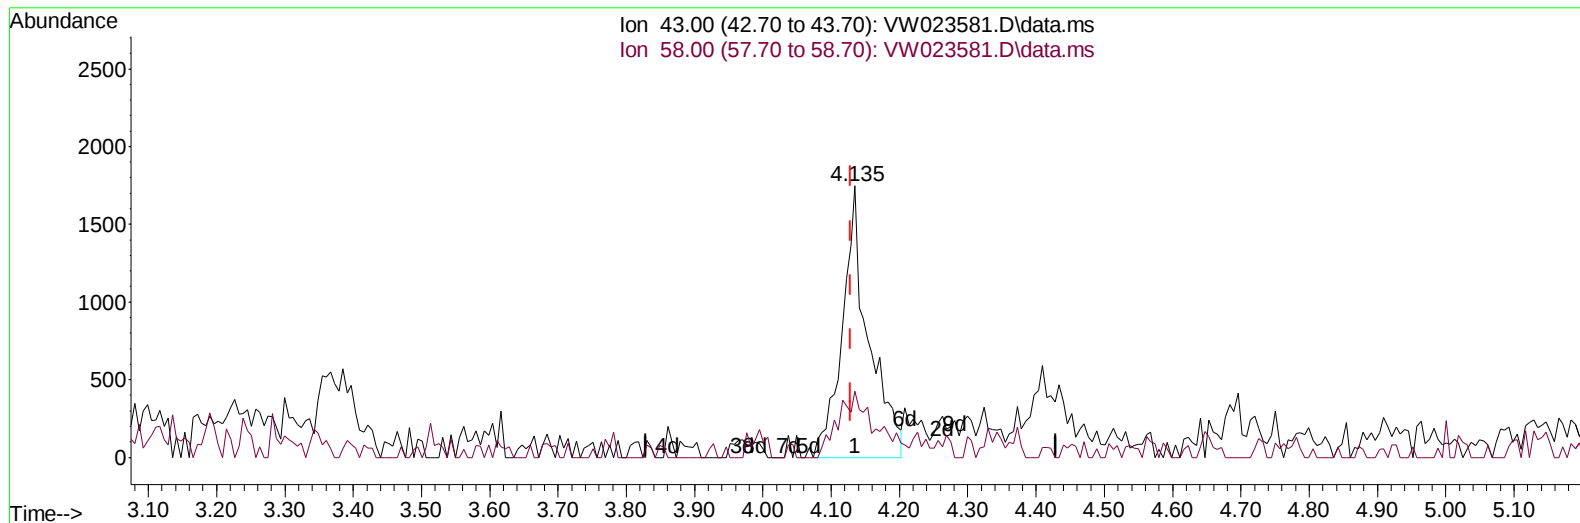

TIC: VW023581.D\data.ms

(13) Acetone (T)

4.135min (+ 0.006) 4.91 ug/L m

response 4659

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	30.60	8.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070722\
Data File : VW023581.D
Acq On : 07 Jul 2022 18:21
Operator : SY/VA
Sample : N3626-05
Misc : 5.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZC1

Manual IntegrationsAPPROVED

Quant Time: Jul 08 01:48:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 08 01:46:16 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/08/2022
Supervised By :Mahesh Dadoda 07/08/2022

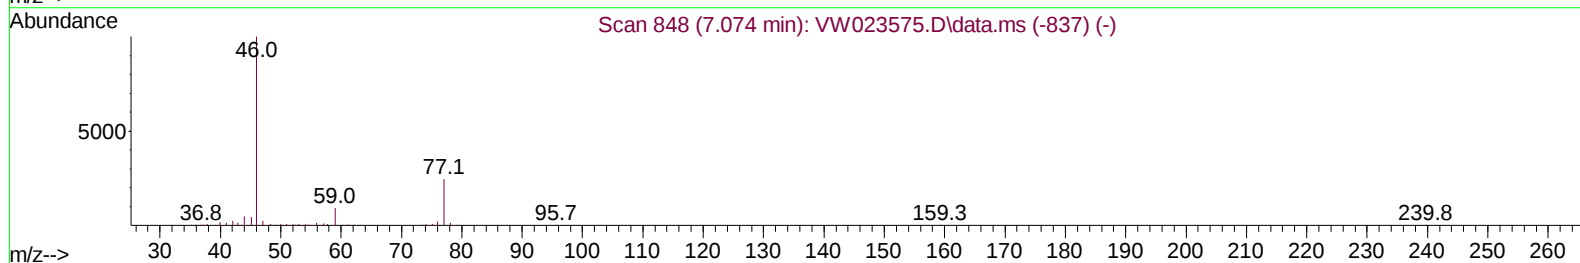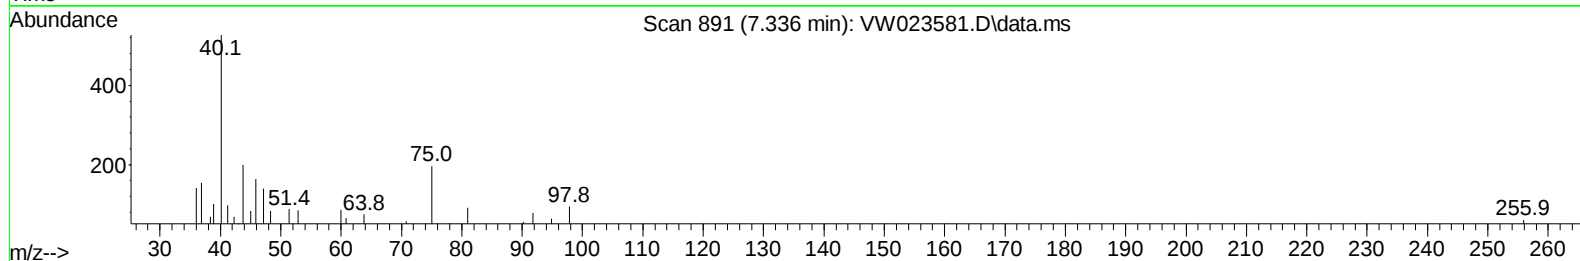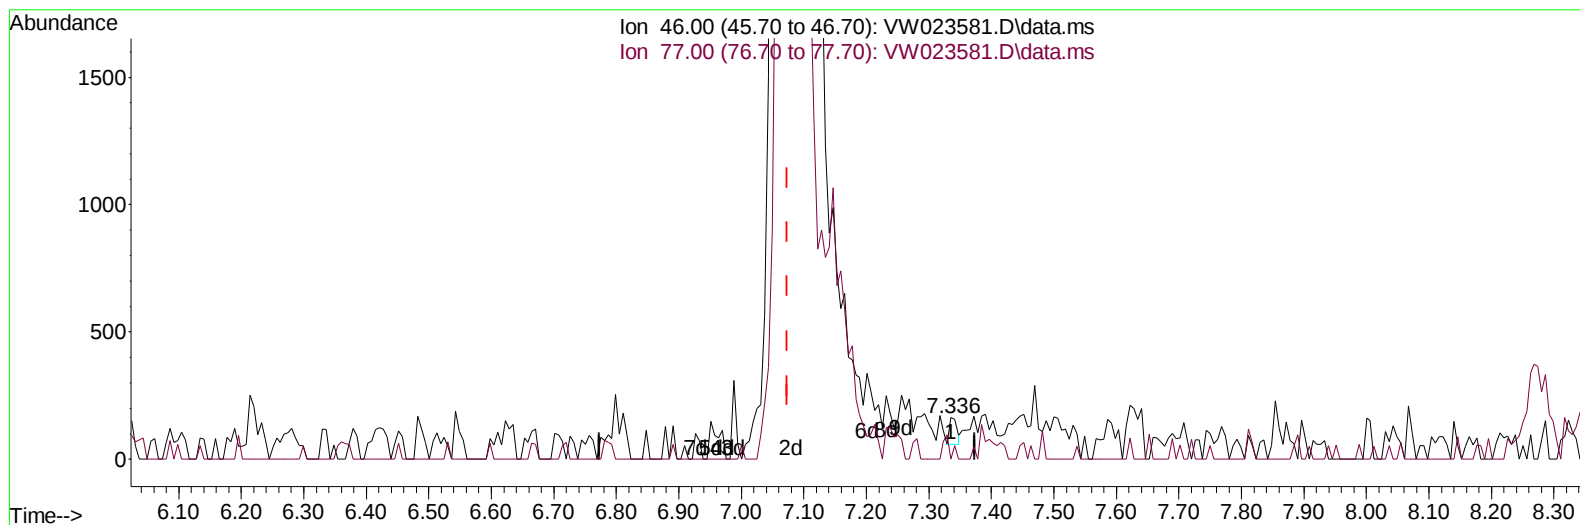

TIC: VW023581.D\data.ms

(21) 2-Butanone-d5 (S)

7.336min (+ 0.262) 0.07 ug/L

response	86	
Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	22.09
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070722\
 Data File : VW023581.D
 Acq On : 07 Jul 2022 18:21
 Operator : SY/VA
 Sample : N3626-05
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZC1

Manual IntegrationsAPPROVED

Quant Time: Jul 08 01:48:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 08 01:46:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/08/2022
 Supervised By :Mahesh Dadoda 07/08/2022

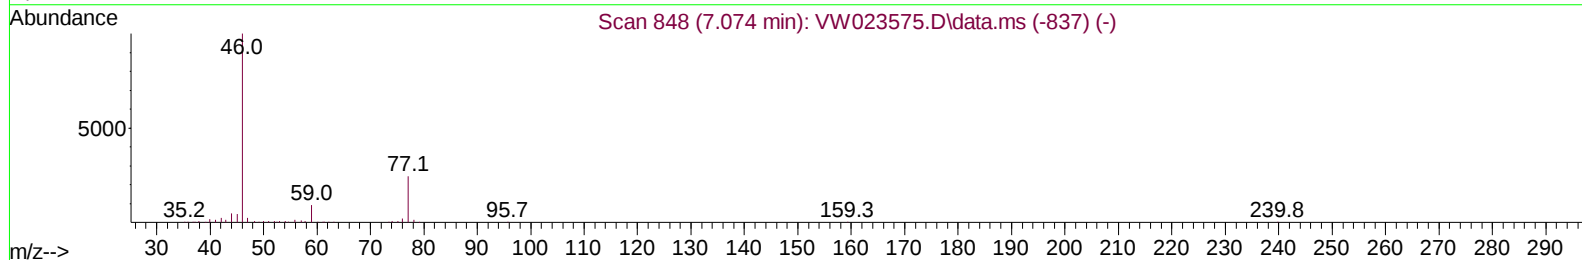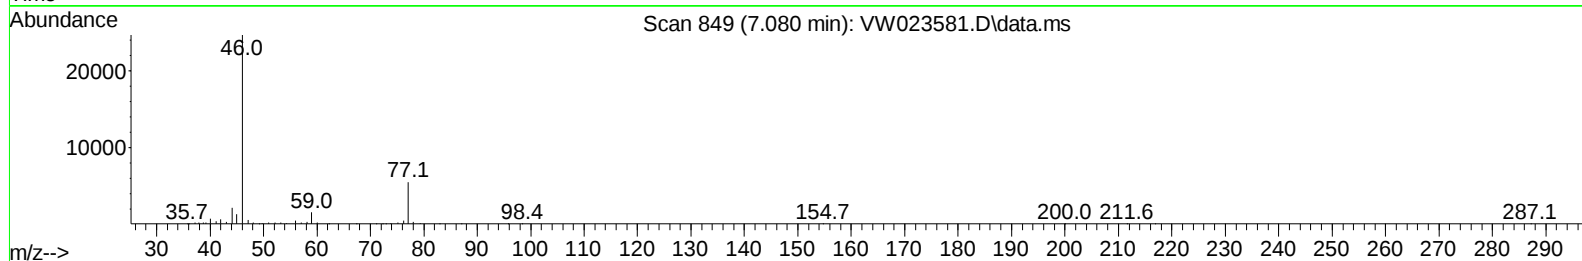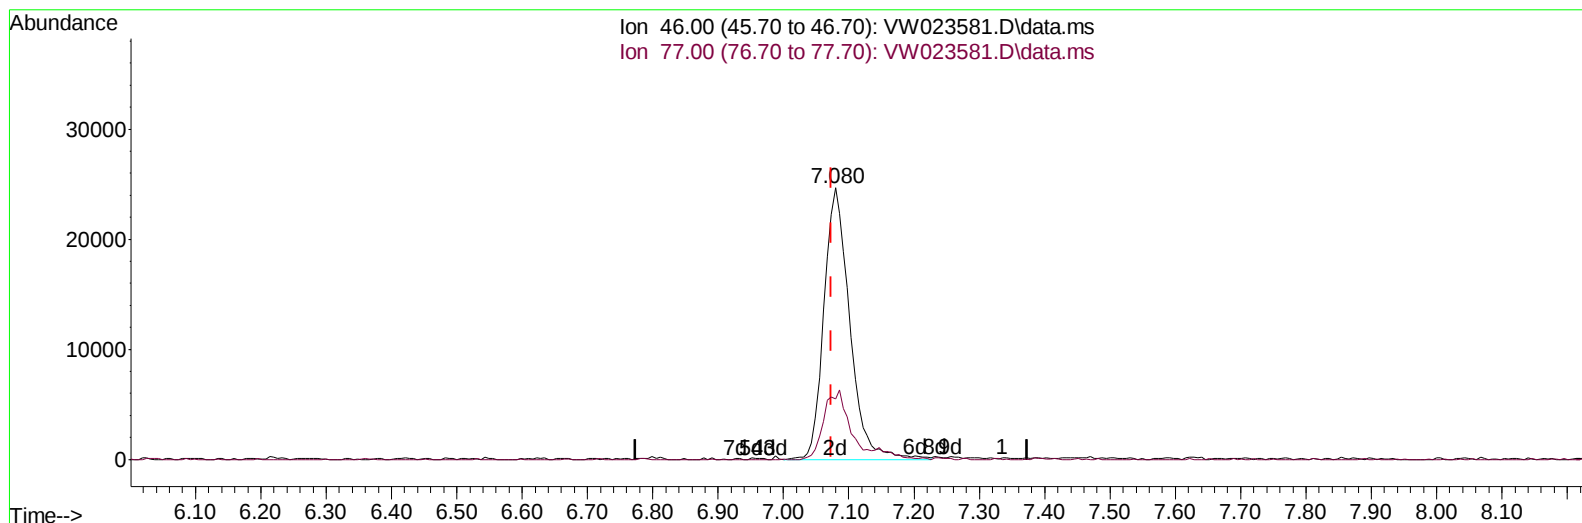

TIC: VW023581.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 52.79 ug/L m

response 67909

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	25.90	0.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070722\
 Data File : VW023581.D
 Acq On : 07 Jul 2022 18:21
 Operator : SY/VA
 Sample : N3626-05
 Misc : 5.61g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0ZC1

Manual IntegrationsAPPROVED

Quant Time: Jul 08 01:48:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jul 08 01:46:16 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/08/2022
 Supervised By :Mahesh Dadoda 07/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	342205	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	308458	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	112442	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	132998	21.470	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	85.880%	
7) Chloroethane-d5	2.879	69	83390	23.538	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	94.160%	
11) 1,1-Dichloroethene-d2	4.013	63	103347	14.798	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	59.200%	
21) 2-Butanone-d5	7.080	46	67909m	52.791	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	105.580%	
24) Chloroform-d	7.653	84	219369	22.506	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	90.040%	
26) 1,2-Dichloroethane-d4	8.305	65	125892	22.851	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	91.400%	
32) Benzene-d6	8.274	84	402820	23.602	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	94.400%	
36) 1,2-Dichloropropane-d6	9.274	67	122775	24.571	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	98.280%	
41) Toluene-d8	10.323	98	359586	21.737	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	86.960%	
43) trans-1,3-Dichloroprop...	10.579	79	44366	19.891	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	79.560%	
47) 2-Hexanone-d5	10.926	63	49587	50.741	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.480%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	124875	25.191	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	100.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152	95196	23.466	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.880%	
Target Compounds						
						Qvalue
13) Acetone	4.135	43	4659m	4.914	ug/L	
16) Methylene chloride	4.921	84	37489	6.460	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW070722\
Data File : VW023581.D
Acq On : 07 Jul 2022 18:21
Operator : SY/VA
Sample : N3626-05
Misc : 5.61g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0ZC1

Manual IntegrationsAPPROVED

Quant Time: Jul 08 01:48:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM070722SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jul 08 01:46:16 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/08/2022
Supervised By :Mahesh Dadoda 07/08/2022

