

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW070818\
 Data File : VW003765.D
 Acq On : 07 Jul 2018 13:46
 Operator : SY/AP
 Sample : J3661-06DL 2X
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL

Quant Time: Jul 09 04:44:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070818S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 09 04:42:46 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	352575	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	341801	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	174321	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.34	65	102441	24.17	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.68%
7) Chloroethane-d5	2.88	69	80208	24.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.52%
10) 1,1-Dichloroethene-d2	4.01	63	168475	18.56	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.24%
20) 2-Butanone-d5	7.09	46	82037	55.63	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	111.26%
24) Chloroform-d	7.65	84	220961	24.54	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.16%
26) 1,2-Dichloroethane-d4	8.31	65	139909	26.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.00%
29) Benzene-d6	8.27	84	418342	23.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.80%
33) 1,2-Dichloropropane-d6	9.27	67	138461	24.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.12%
37) Toluene-d8	10.32	98	398507	24.30	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.20%
38) trans-1,3-Dichloropropene-	10.58	79	63100	24.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.60%
39) 2-Hexanone-d5	10.93	63	61577	56.14	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.28%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	136117	26.21	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.84%
61) 1,2-Dichlorobenzene-d4	13.86	152	153634	24.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.20%

Target Compounds

					Qvalue
2) Dichlorodifluoromethane	2.00	85	17431	9.973 ug/L	99
5) Vinyl chloride	2.36	62	36121	7.027 ug/L	97
8) Chloroethane	2.92	64	29761	9.725 ug/L	100
12) 1,1-Dichloroethene	4.03	96	31420	7.288 ug/L	# 11
13) Acetone	4.14	43	139752	93.861 ug/L	98
14) Carbon disulfide	4.37	76	148192	10.610 ug/L	100
16) Methylene chloride	4.90	84	84411	16.755 ug/L	94
18) trans-1,2-Dichloroethene	5.41	96	62763	13.619 ug/L	95
19) 1,1-Dichloroethane	6.21	63	49048	5.644 ug/L	98
22) cis-1,2-Dichloroethene	7.17	96	80077	16.321 ug/L	97
23) Bromochloromethane	7.51	128	48170	21.356 ug/L	97
25) Chloroform	7.67	83	55784	6.250 ug/L	97
31) 1,1,1-Trichloroethane	7.87	97	149499	19.885 ug/L	100
32) Carbon tetrachloride	8.07	117	53582	7.531 ug/L	100
35) Trichloroethene	9.09	95	85311	15.934 ug/L	99
40) 1,2-Dichloropropane	9.37	63	53321	10.025 ug/L	99
41) Bromodichloromethane	9.65	83	43727	6.502 ug/L	99

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW070818\
 Data File : VW003765.D
 Acq On : 07 Jul 2018 13:46
 Operator : SY/AP
 Sample : J3661-06DL 2X
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL

Quant Time: Jul 09 04:44:21 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070818S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Jul 09 04:42:46 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
42) cis-1,3-Dichloropropene	10.07	75	46915	5.958	ug/L	95
43) 4-Methyl-2-pentanone	10.21	43	82130	22.200	ug/L	98
45) trans-1,3-Dichloropropene	10.61	75	75513	10.554	ug/L	100
46) 1,1,2-Trichloroethane	10.79	97	22048	5.583	ug/L	95
47) Tetrachloroethene	10.87	164	44200	10.147	ug/L	99
49) 2-Hexanone	10.98	43	89880	32.086	ug/L	95
50) Dibromochloromethane	11.13	129	30740	6.532	ug/L	98
51) 1,2-Dibromoethane	11.24	107	41654	10.827	ug/L #	98
56) Styrene	12.19	104	123805	8.510	ug/L	100
58) 1,1,2,2-Tetrachloroethane	12.72	83	82706	15.952	ug/L	98
62) Bromoform	12.35	173	31032	10.645	ug/L	100
63) 1,3-Dichlorobenzene	13.51	146	143892	13.335	ug/L	100
66) 1,2-Dibromo-3-chloropropan	14.49	75	20427	22.177	ug/L	96
70) 1,2,3-Trichlorobenzene	15.57	180	30113	4.747	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW070818\
Data File : VW003765.D
Acq On : 07 Jul 2018 13:46
Operator : SY/AP
Sample : J3661-06DL 2X
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
X2D24DL

Quant Time: Jul 09 04:44:21 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM070818S.M
Quant Title : VOC Analysis
QLast Update : Mon Jul 09 04:42:46 2018
Response via : Initial Calibration

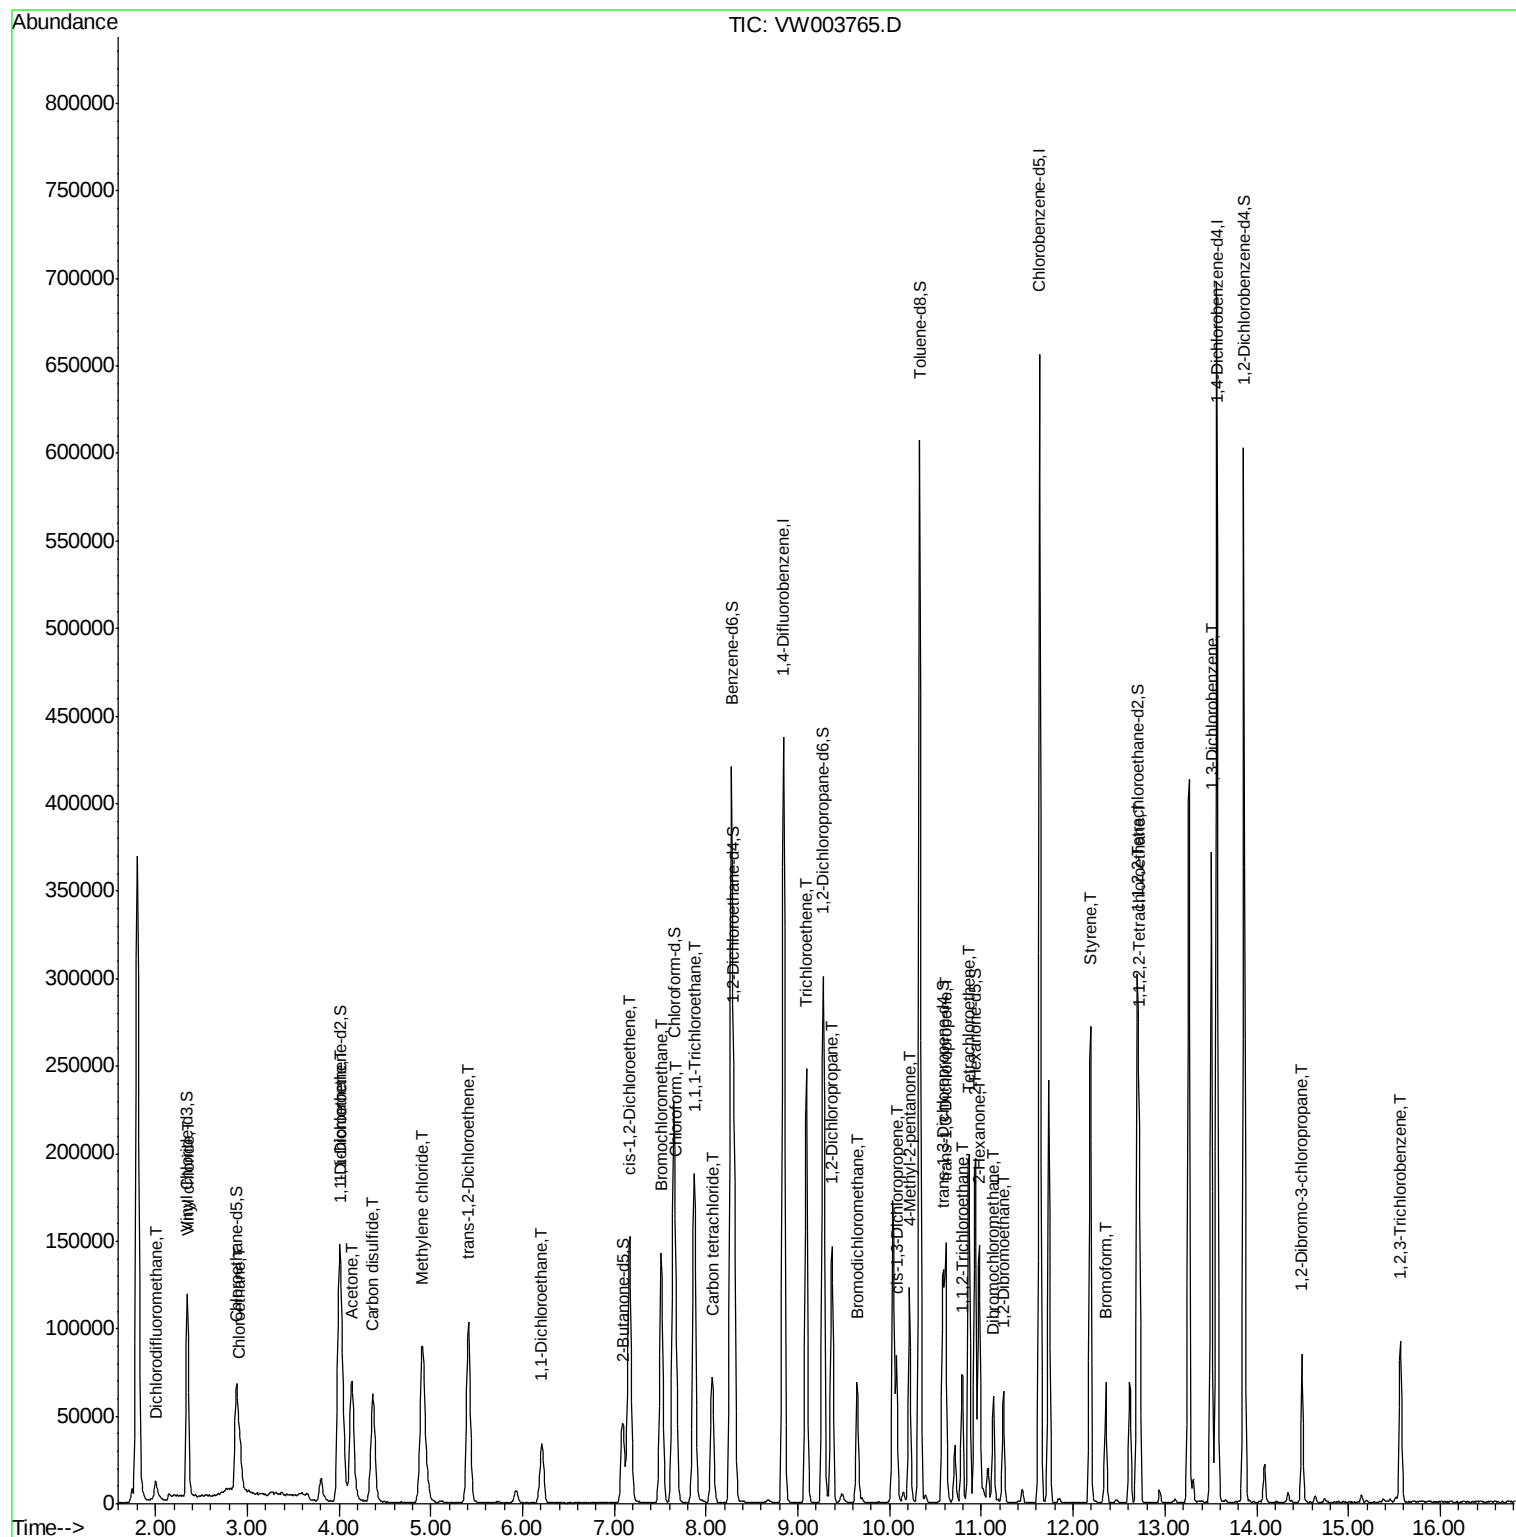



#2

Dichlorodifluoromethane

Concen: 9.973 ug/L

RT: 2.00 min Scan# 68

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :


X2D24DL

Tgt Ion: 85 Resp: 17431

Ion Ratio Lower Upper




85 100

87 23.8 16.4 30.4

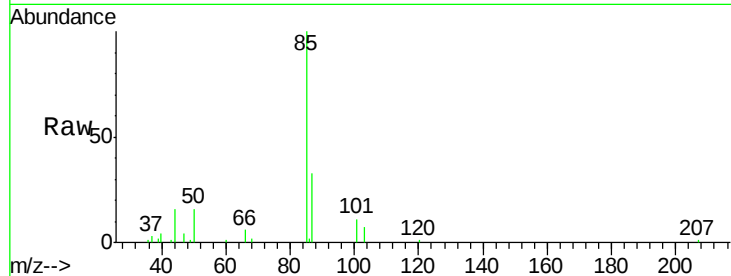

Abundance Ion 85.00 (84.70 to 85.70): VW

Ion 87.00 (86.70 to 87.70): VW

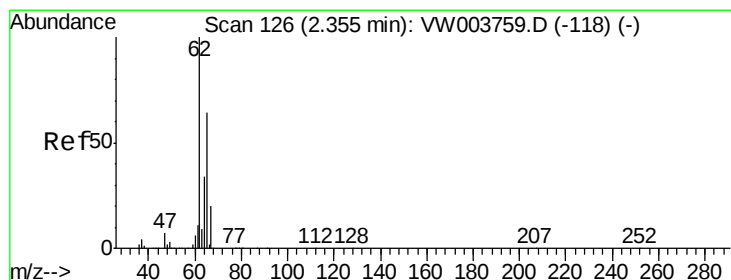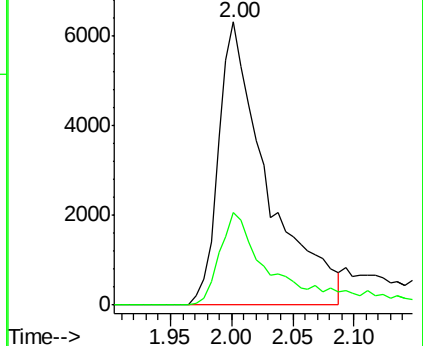

#5

Vinyl chloride

Concen: 7.027 ug/L

RT: 2.36 min Scan# 126

Delta R.T. -0.00 min

Lab File: VW003765.D


Acq: 07 Jul 2018 13:46

Tgt Ion: 62 Resp: 36121

Ion Ratio Lower Upper



62 100


64 35.2 23.4 43.6



Abundance Ion 62.00 (61.70 to 62.70): VW

Ion 64.00 (63.70 to 64.70): VW

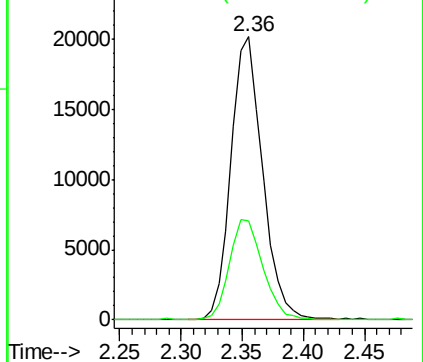

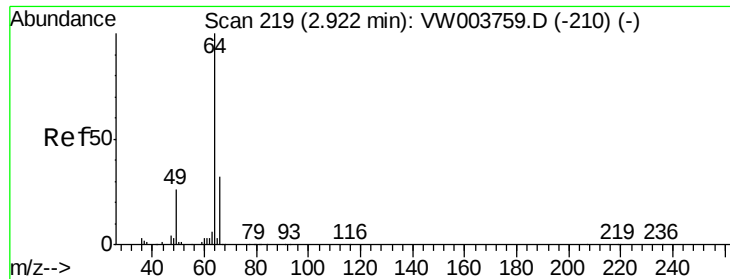

#8

Chloroethane

Concen: 9.725 ug/L

RT: 2.92 min Scan# 218

Delta R.T. -0.01 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :





X2D24DL

Tgt Ion: 64 Resp: 29761

Ion Ratio Lower Upper

64 100

66 31.4 22.1 41.1

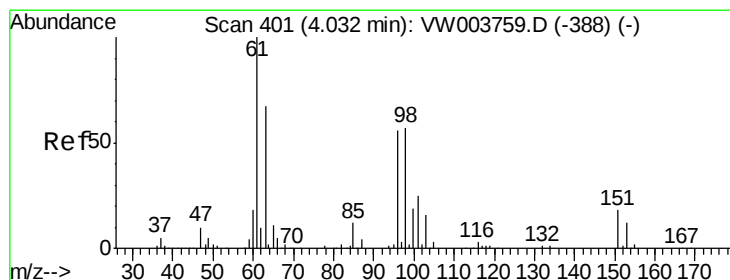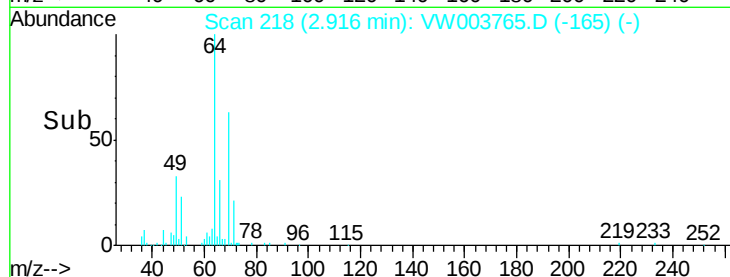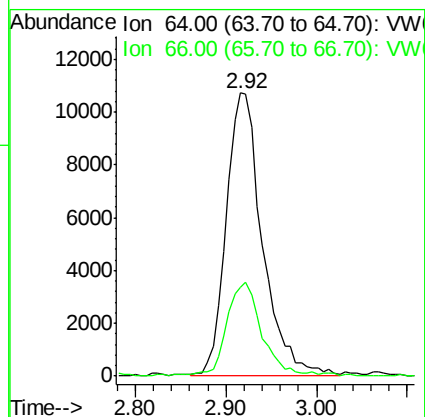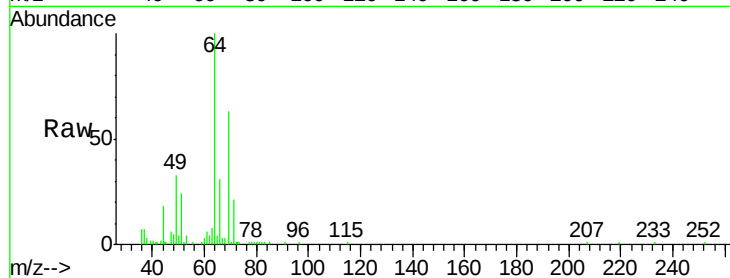

#12

1,1-Dichloroethene

Concen: 7.288 ug/L

RT: 4.03 min Scan# 400

Delta R.T. -0.01 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46




Tgt Ion: 96 Resp: 31420


Ion Ratio Lower Upper

96 100

61 194.0 126.2 234.4

63 354.5 85.8 159.4#

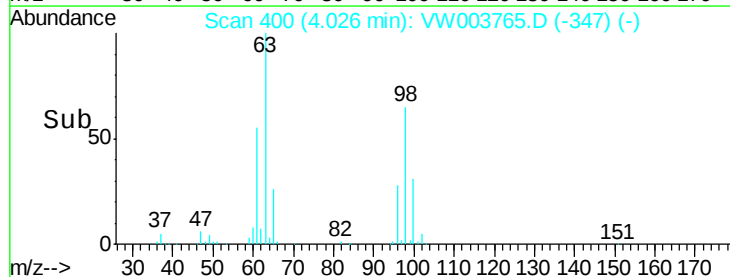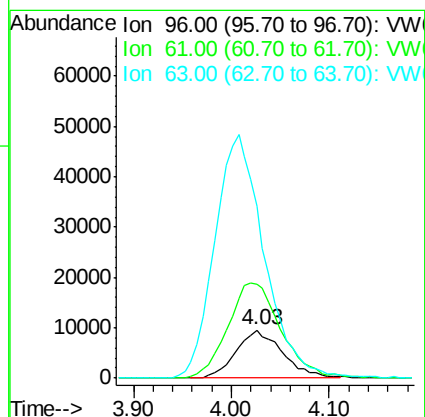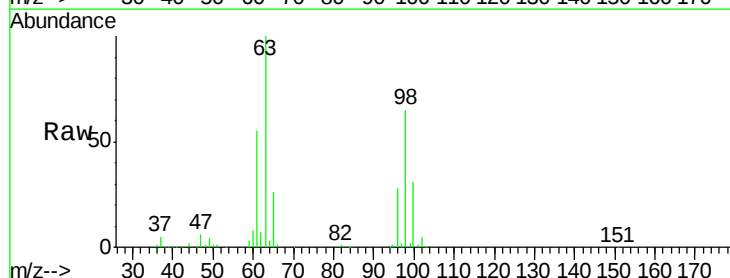



#13

Acetone

Concen: 93.861 ug/L

RT: 4.14 min Scan# 419

Delta R.T. -0.01 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :





X2D24DL

Tgt Ion: 43 Resp: 139752

Ion Ratio Lower Upper

43 100

58 27.8 0.0 58.2

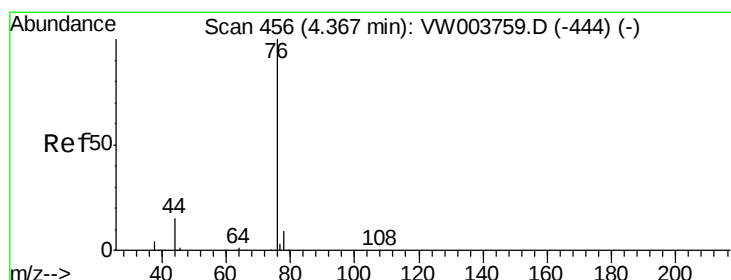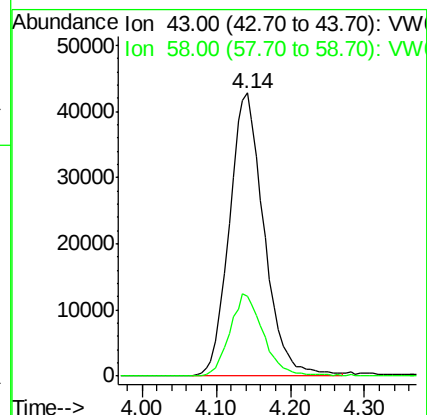

#14

Carbon disulfide

Concen: 10.610 ug/L

RT: 4.37 min Scan# 456

Delta R.T. -0.00 min

Lab File: VW003765.D




Acq: 07 Jul 2018 13:46


Tgt Ion: 76 Resp: 148192

Ion Ratio Lower Upper

76 100

78 9.1 7.2 10.8



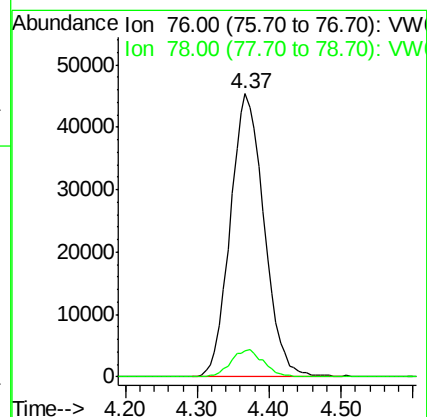





#16
Methylene chloride
Concen: 16.755 ug/L
RT: 4.90 min Scan# 544
Delta R.T. -0.01 min
Lab File: VW003765.D
Acq: 07 Jul 2018 13:46




Instrument :
MSVOA_W
ClientSampleId :
X2D24DL


Tgt Ion: 84 Resp: 84411
Ion Ratio Lower Upper
84 100
49 138.4 89.9 166.9
86 62.7 43.9 81.5

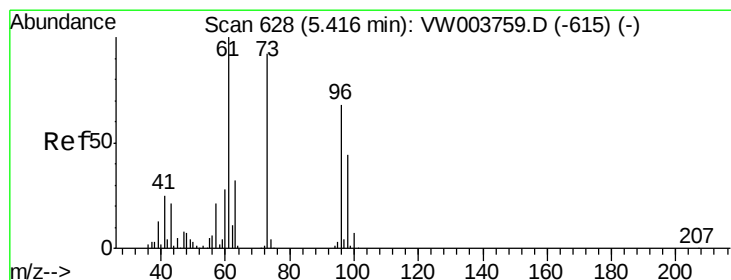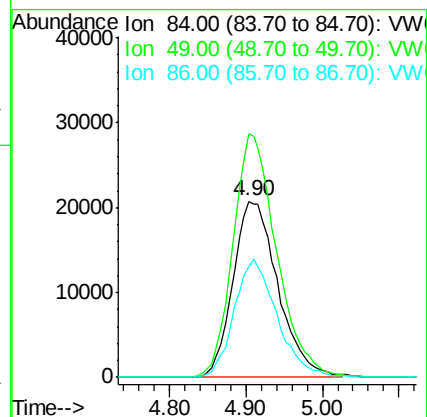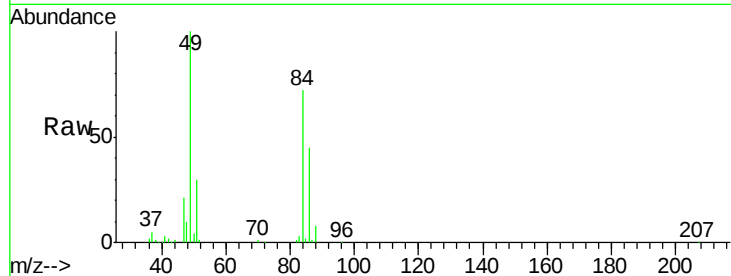

#18
trans-1,2-Dichloroethene
Concen: 13.619 ug/L
RT: 5.41 min Scan# 627
Delta R.T. -0.01 min
Lab File: VW003765.D
Acq: 07 Jul 2018 13:46

Tgt Ion: 96 Resp: 62763
Ion Ratio Lower Upper
96 100
61 139.7 103.0 191.2
98 62.1 45.8 85.2



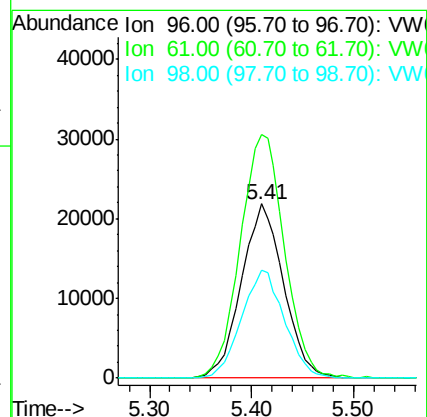





#19
 1,1-Dichloroethane
 Concen: 5.644 ug/L
 RT: 6.21 min Scan# 758
 Delta R.T. -0.01 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46




Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL


Tgt Ion: 63 Resp: 49048
 Ion Ratio Lower Upper
 63 100
 65 32.5 21.9 40.7
 83 13.3 9.6 17.8

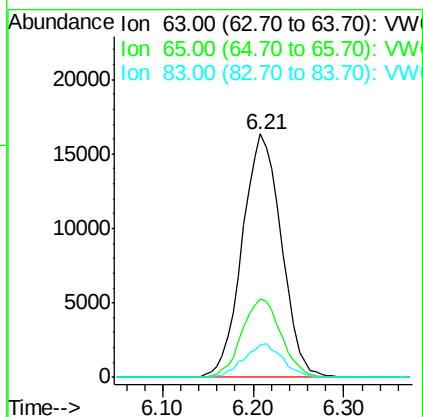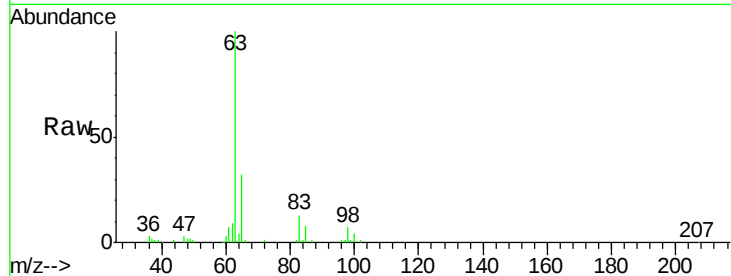

#22
 cis-1,2-Dichloroethene
 Concen: 16.321 ug/L
 RT: 7.17 min Scan# 915
 Delta R.T. -0.01 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Tgt Ion: 96 Resp: 80077
 Ion Ratio Lower Upper
 96 100
 61 141.9 96.4 179.0
 98 65.8 45.6 84.8

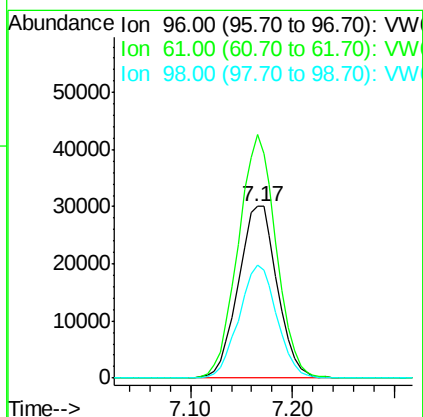

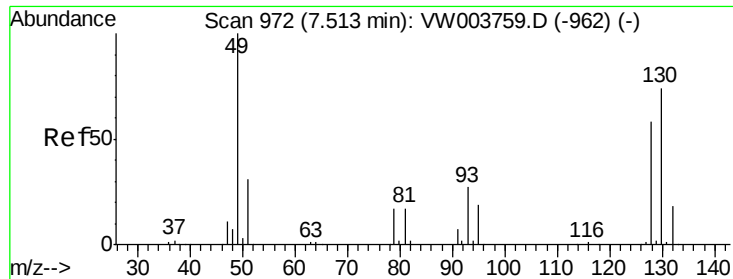

#23

Bromochloromethane

Concen: 21.356 ug/L

RT: 7.51 min Scan# 972

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :

X2D24DL

Tgt Ion:128 Resp: 48170


Ion Ratio Lower Upper

128 100

49 177.6 120.7 224.1

130 129.2 88.8 164.8

51 56.2 43.2 64.8



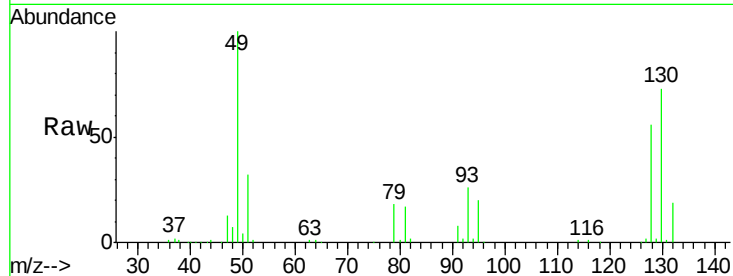


Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VW

Ion 130.00 (129.70 to 130.70): V

Ion 51.00 (50.70 to 51.70): VW

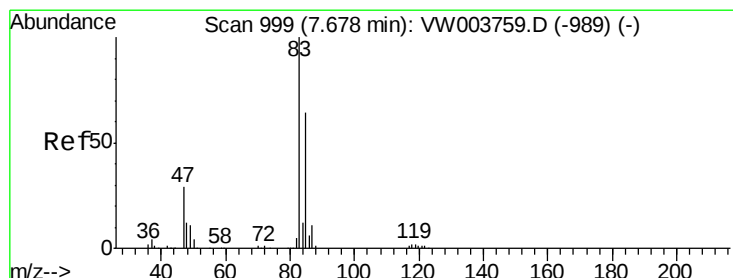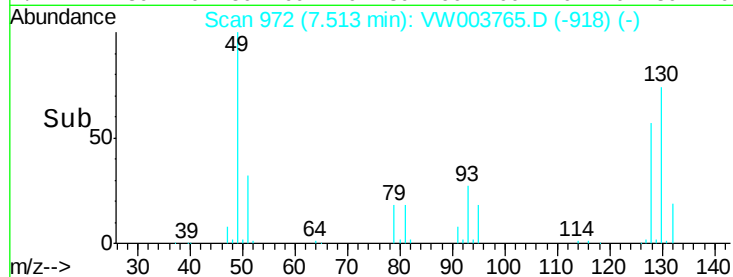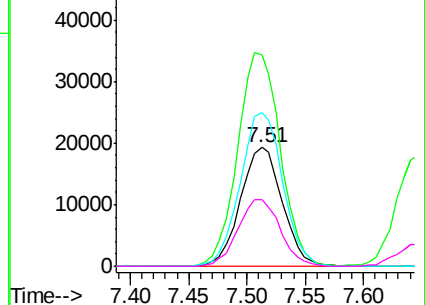

#25

Chloroform

Concen: 6.250 ug/L

RT: 7.67 min Scan# 998

Delta R.T. -0.01 min

Lab File: VW003765.D


Acq: 07 Jul 2018 13:46

Tgt Ion: 83 Resp: 55784

Ion Ratio Lower Upper



83 100


85 68.1 46.0 85.4

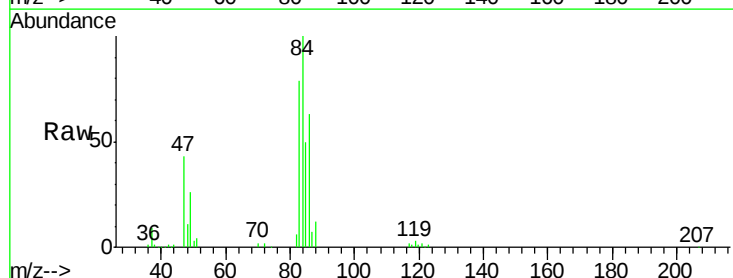

Abundance Ion 83.00 (82.70 to 83.70): VW

Ion 85.00 (84.70 to 85.70): VW

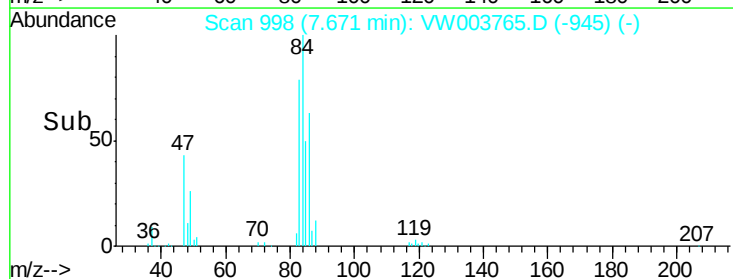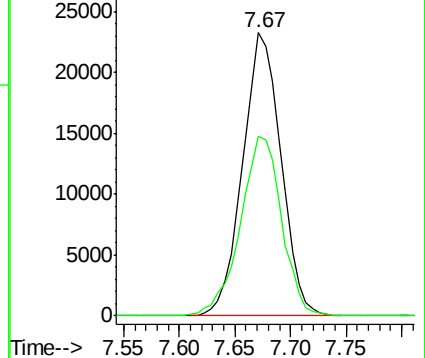



#31

1,1,1-Trichloroethane

Concen: 19.885 ug/L

RT: 7.87 min Scan# 1031

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :

X2D24DL


Tgt Ion: 97 Resp: 149499

Ion Ratio Lower Upper

97 100

99 64.2 51.3 76.9




61 47.7 38.1 57.1



Abundance Ion 97.00 (96.70 to 97.70): VW

Ion 99.00 (98.70 to 99.70): VW

Ion 61.00 (60.70 to 61.70): VW

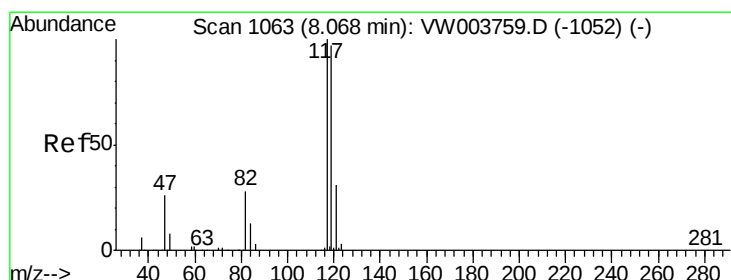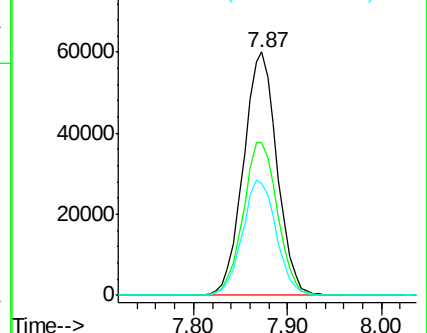

#32

Carbon tetrachloride

Concen: 7.531 ug/L

RT: 8.07 min Scan# 1063

Delta R.T. -0.00 min

Lab File: VW003765.D


Acq: 07 Jul 2018 13:46

Tgt Ion: 117 Resp: 53582

Ion Ratio Lower Upper



117 100


119 96.2 76.8 115.2

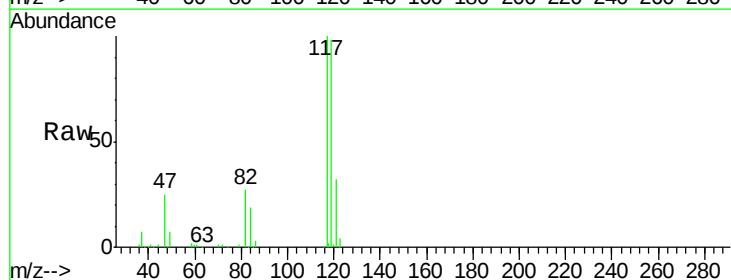

Abundance Ion 117.00 (116.70 to 117.70): V

Ion 119.00 (118.70 to 119.70): V

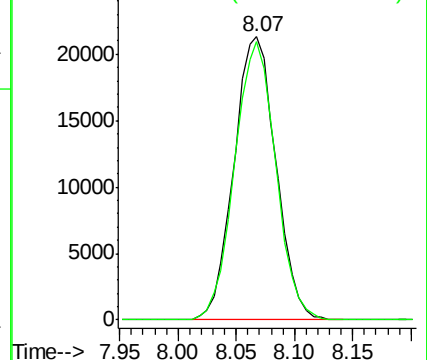







#35
 Trichloroethene
 Concen: 15.934 ug/L
 RT: 9.09 min Scan# 1231
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL

Tgt Ion: 95 Resp: 85311
 Ion Ratio Lower Upper
 95 100
 97 62.6 44.7 82.9
 132 93.5 66.2 123.0
 130 98.1 69.5 129.1

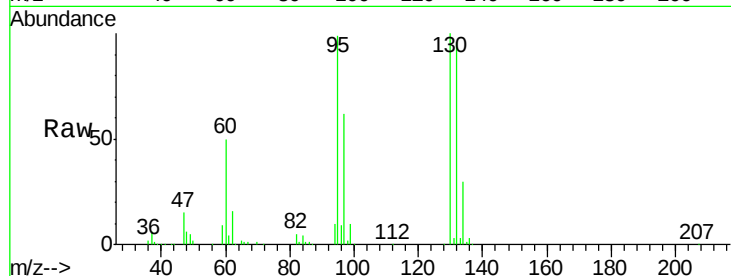


Abundance Ion 95.00 (94.70 to 95.70): VW
 Ion 97.00 (96.70 to 97.70): VW
 Ion 132.00 (131.70 to 132.70): V
 Ion 130.00 (129.70 to 130.70): V


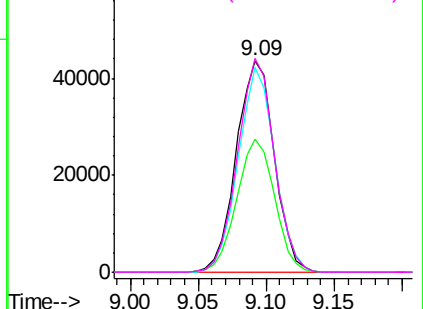



#40
 1,2-Dichloropropane
 Concen: 10.025 ug/L
 RT: 9.37 min Scan# 1277
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Tgt Ion: 63 Resp: 53321
 Ion Ratio Lower Upper
 63 100
 112 4.4 3.3 4.9



Abundance Ion 63.00 (62.70 to 63.70): VW
 Ion 112.00 (111.70 to 112.70): V




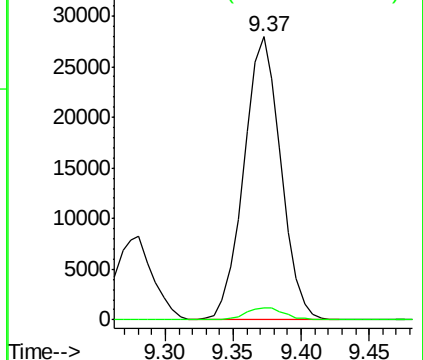




#41
 Bromodichloromethane
 Concen: 6.502 ug/L
 RT: 9.65 min Scan# 1322
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46




Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL


Tgt Ion: 83 Resp: 43727
 Ion Ratio Lower Upper
 83 100
 85 64.1 45.1 83.9
 127 7.9 6.8 10.2

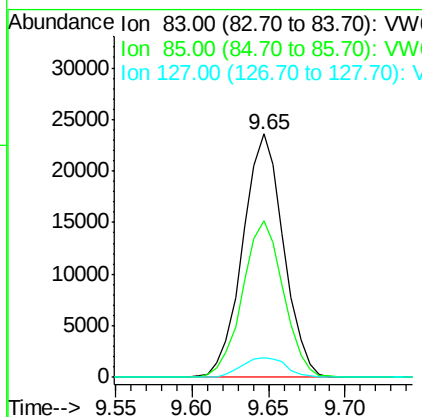

#42
 cis-1,3-Dichloropropene
 Concen: 5.958 ug/L
 RT: 10.07 min Scan# 1392
 Delta R.T. -0.01 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Tgt Ion: 75 Resp: 46915
 Ion Ratio Lower Upper
 75 100
 77 33.5 21.6 40.0

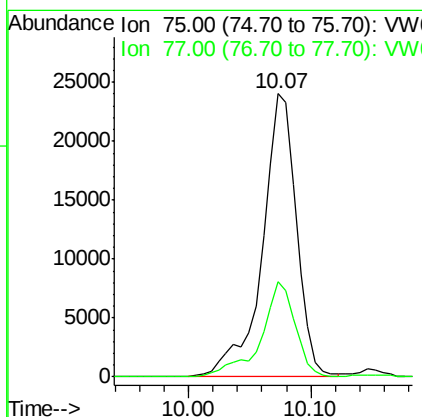

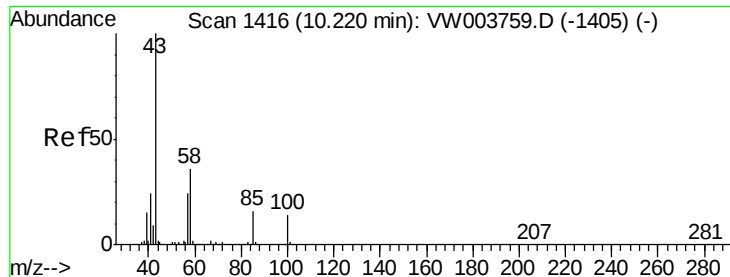

#43

4-Methyl-2-pentanone

Concen: 22.200 ug/L

RT: 10.21 min Scan# 1415

Delta R.T. -0.01 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :

X2D24DL


Tgt Ion: 43 Resp: 82130

Ion Ratio Lower Upper




43 100

58 35.4 29.0 43.4

100 12.7 10.7 16.1

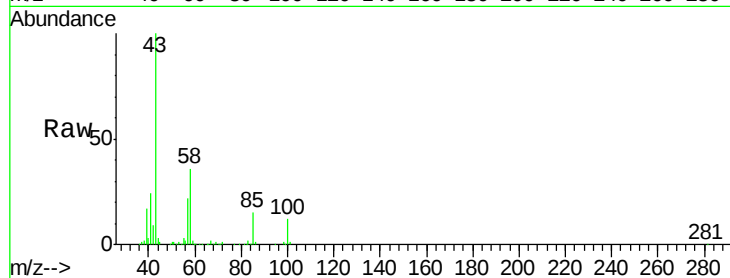

Abundance Ion 43.00 (42.70 to 43.70): VW
Ion 58.00 (57.70 to 58.70): VW
Ion 100.00 (99.70 to 100.70): VW

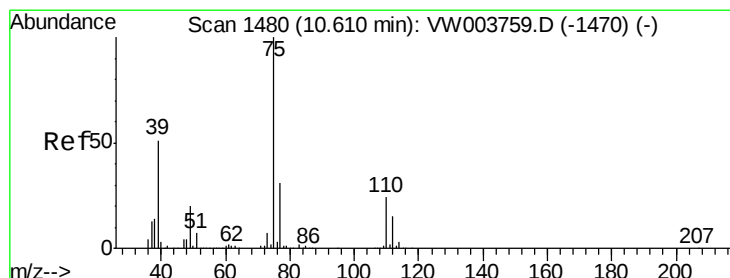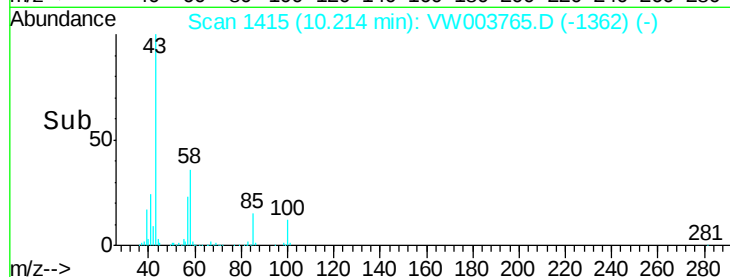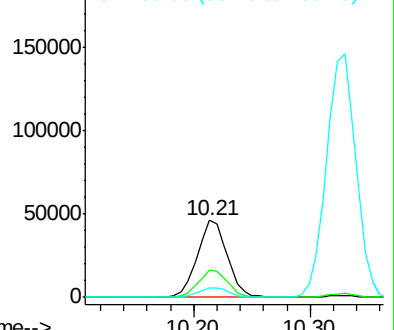

#45

trans-1,3-Dichloropropene

Concen: 10.554 ug/L

RT: 10.61 min Scan# 1480

Delta R.T. -0.00 min

Lab File: VW003765.D


Acq: 07 Jul 2018 13:46

Tgt Ion: 75 Resp: 75513



Ion Ratio Lower Upper


75 100

77 31.3 21.8 40.4

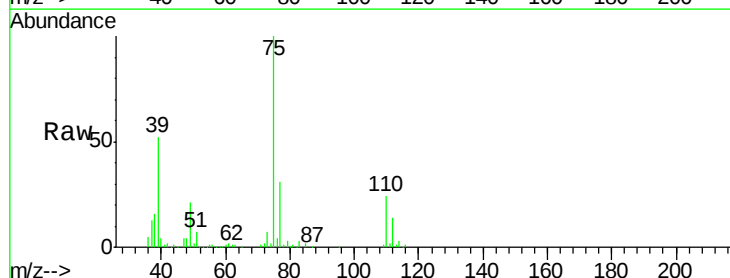

Abundance Ion 75.00 (74.70 to 75.70): VW
Ion 77.00 (76.70 to 77.70): VW



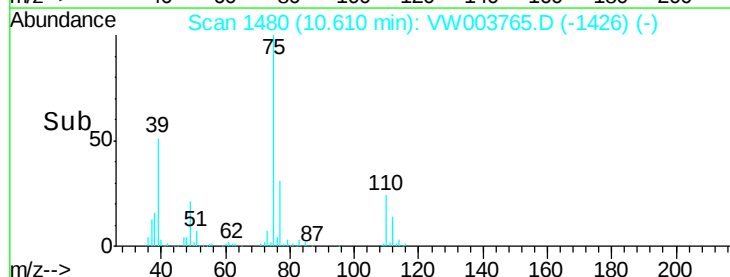
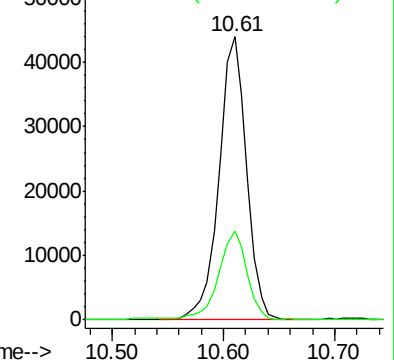




#46
 1,1,2-Trichloroethane
 Concen: 5.583 ug/L
 RT: 10.79 min Scan# 1509
 Delta R.T. -0.01 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46




Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL


Tgt Ion:	97	Resp:	22048
Ion	Ratio	Lower	Upper
97	100		
83	91.9	60.1	111.5
85	54.0	40.0	74.2
99	61.5	44.0	81.8

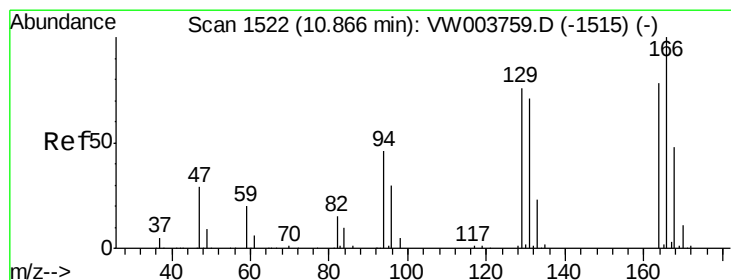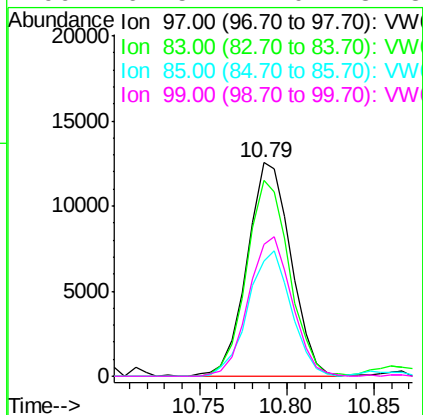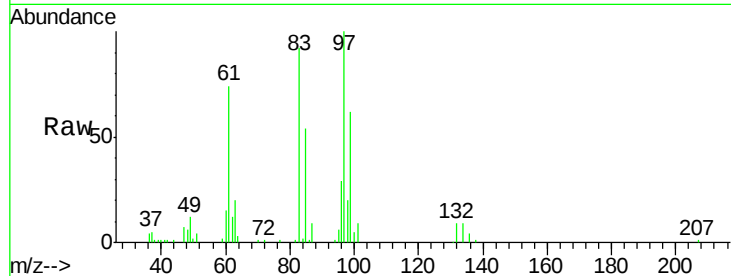

#47
 Tetrachloroethene
 Concen: 10.147 ug/L
 RT: 10.87 min Scan# 1522
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Tgt Ion:	164	Resp:	44200
Ion	Ratio	Lower	Upper
164	100		
129	96.5	68.3	126.8
131	89.7	63.8	118.4
166	128.9	89.5	166.1


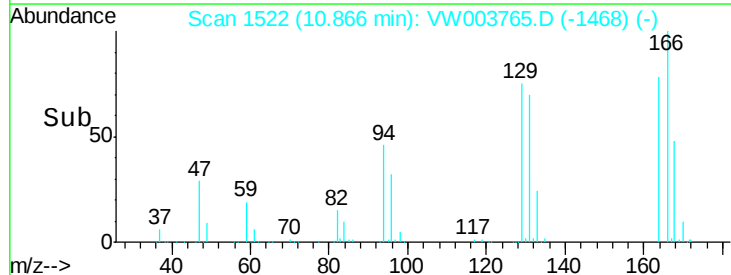
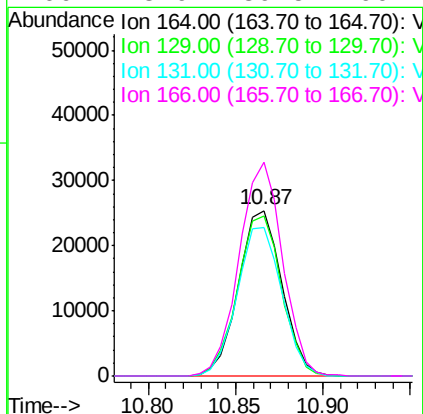





#49
2-Hexanone
Concen: 32.086 ug/L
RT: 10.98 min Scan# 1540
Delta R.T. -0.00 min
Lab File: VW003765.D
Acq: 07 Jul 2018 13:46




Instrument :
MSVOA_W
ClientSampleId :
X2D24DL


Tgt Ion:	43	Resp:	89880
Ion	Ratio	Lower	Upper
43	100		
58	53.7	39.5	59.3
57	19.4	13.8	20.8
100	10.4	8.2	12.2

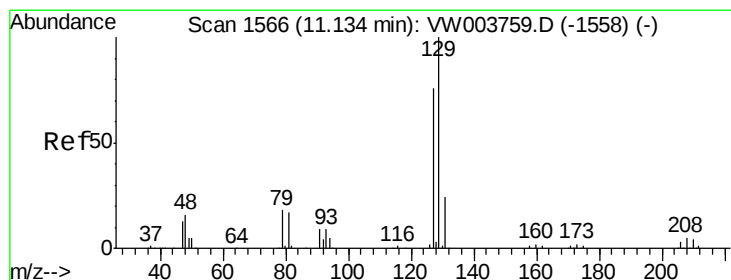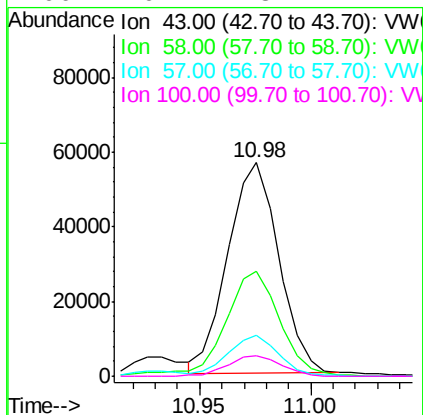

#50
Dibromochloromethane
Concen: 6.532 ug/L
RT: 11.13 min Scan# 1565
Delta R.T. -0.01 min
Lab File: VW003765.D
Acq: 07 Jul 2018 13:46

Tgt Ion:	129	Resp:	30740
Ion	Ratio	Lower	Upper
129	100		
127	78.0	53.1	98.7



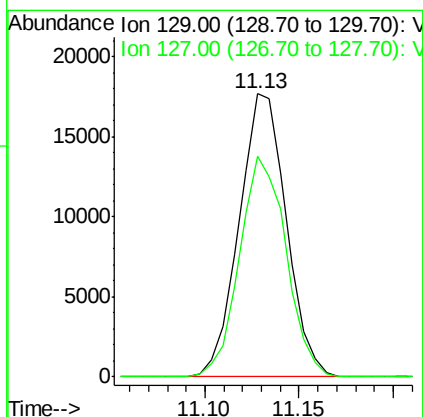
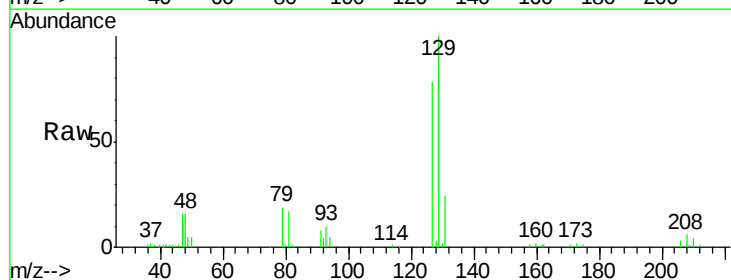




#51
 1,2-Dibromoethane
 Concen: 10.827 ug/L
 RT: 11.24 min Scan# 1583
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46




Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL


Tgt Ion:107 Resp: 41654
 Ion Ratio Lower Upper
 107 100
 109 93.4 63.7 118.3
 188 2.9 2.9 4.3#

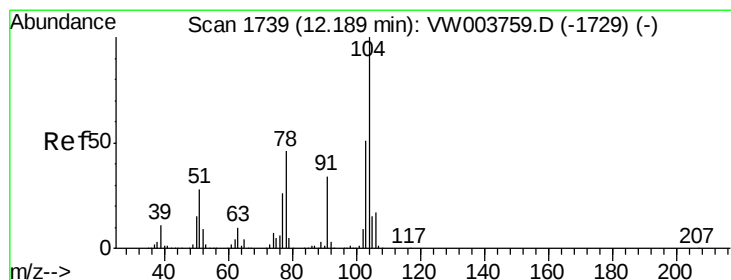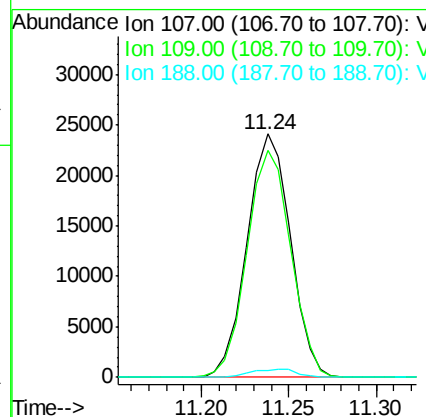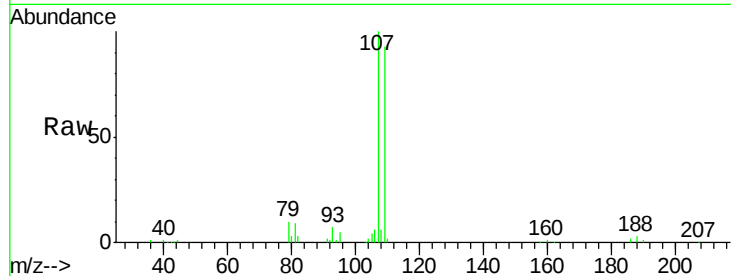

#56
 Styrene
 Concen: 8.510 ug/L
 RT: 12.19 min Scan# 1739
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Tgt Ion:104 Resp: 123805
 Ion Ratio Lower Upper
 104 100
 78 46.0 32.1 59.7

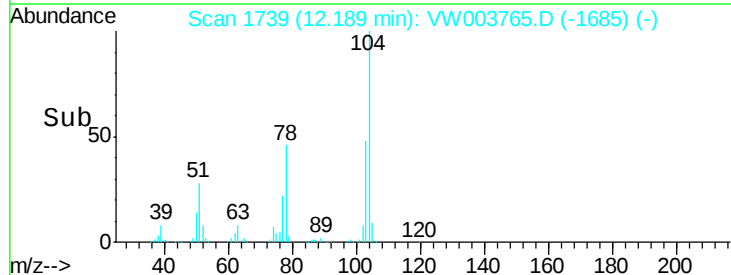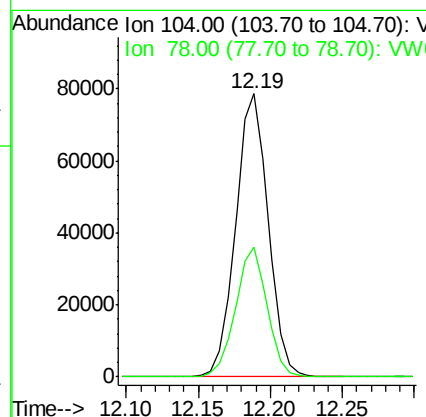

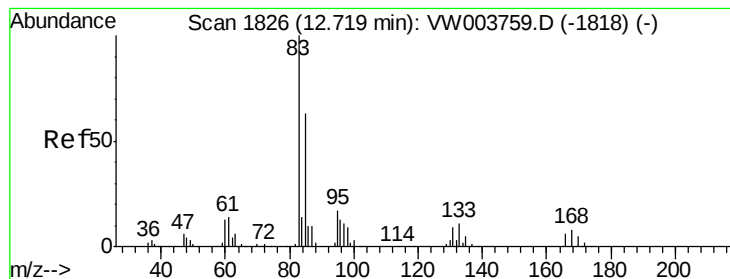

#58

1,1,2,2-Tetrachloroethane

Concen: 15.952 ug/L

RT: 12.72 min Scan# 1826

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :

X2D24DL


Tgt Ion: 83 Resp: 82706

Ion Ratio Lower Upper

83 100

85 64.9 44.2 82.0




131 9.4 7.5 11.3

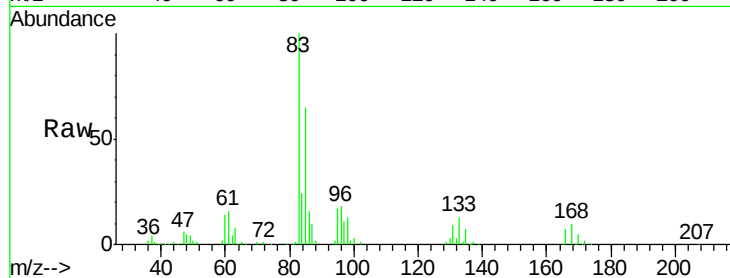

Abundance Ion 83.00 (82.70 to 83.70): VW

Ion 85.00 (84.70 to 85.70): VW

Ion 131.00 (130.70 to 131.70): V

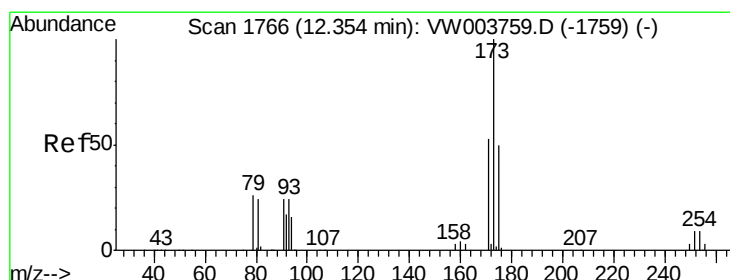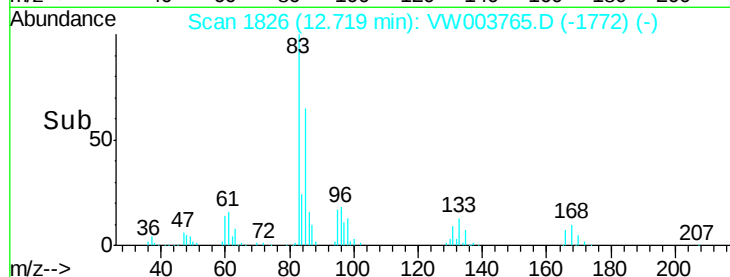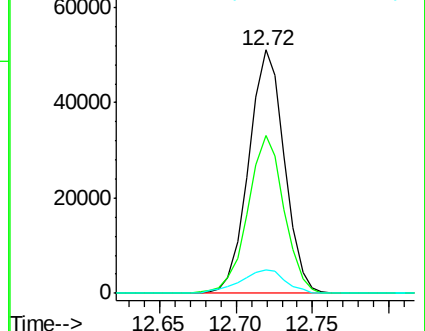

#62

Bromoform

Concen: 10.645 ug/L

RT: 12.35 min Scan# 1766

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46


Tgt Ion: 173 Resp: 31032

Ion Ratio Lower Upper

173 100

175 48.1 38.7 58.1



254 9.4 7.7 11.5

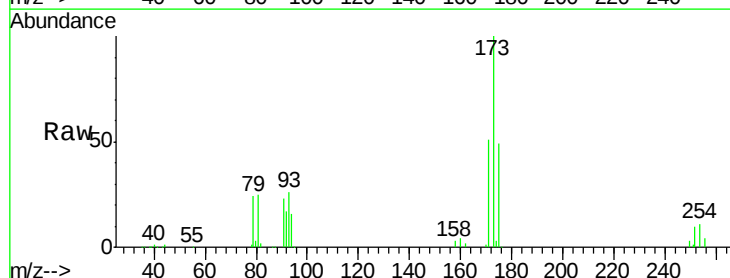


Abundance Ion 173.00 (172.70 to 173.70): V

Ion 175.00 (174.70 to 175.70): V

Ion 254.00 (253.70 to 254.70): V

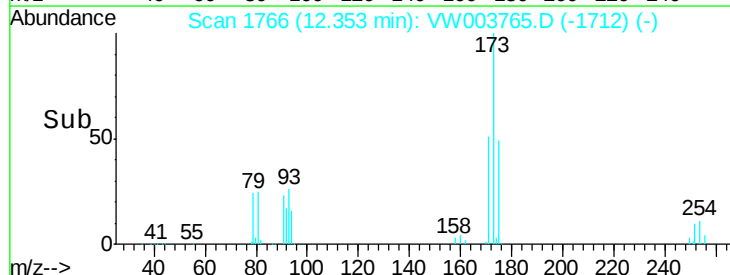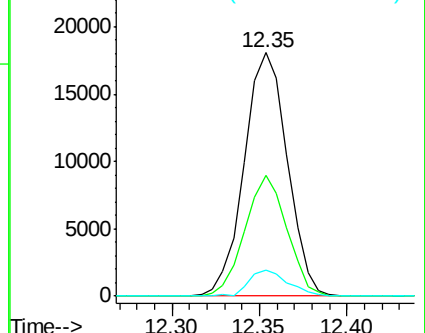



#63

1,3-Dichlorobenzene

Concen: 13.335 ug/L

RT: 13.51 min Scan# 1955

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46

Instrument :

MSVOA_W

ClientSampleId :

X2D24DL


Tgt Ion:146 Resp: 143892

Ion Ratio Lower Upper

146 100

111 41.0 28.3 52.7




148 64.3 45.1 83.7

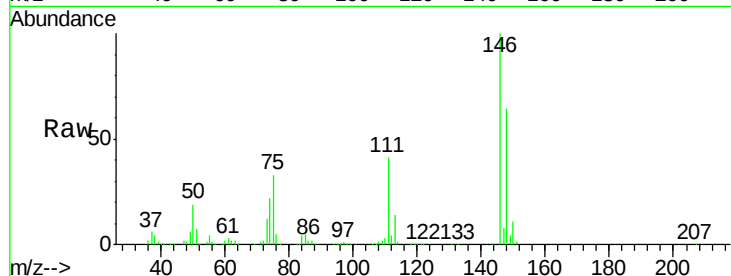

Abundance Ion 146.00 (145.70 to 146.70): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

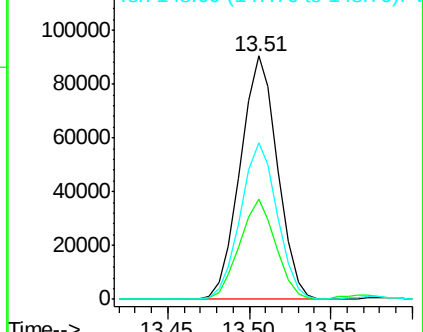

#66

1,2-Dibromo-3-chloropropane

Concen: 22.177 ug/L

RT: 14.49 min Scan# 2117

Delta R.T. -0.00 min

Lab File: VW003765.D

Acq: 07 Jul 2018 13:46


Tgt Ion: 75 Resp: 20427

Ion Ratio Lower Upper

75 100

157 99.4 78.6 118.0



155 72.3 63.7 95.5




Abundance Ion 75.00 (74.70 to 75.70): VW

Ion 157.00 (156.70 to 157.70): V

Ion 155.00 (154.70 to 155.70): V

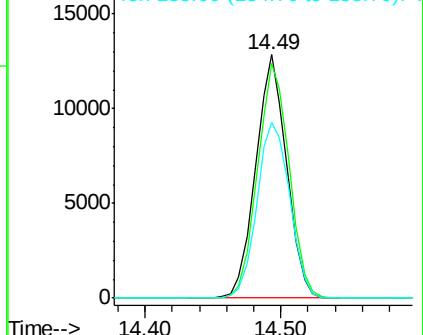




#70
 1,2,3-Trichlorobenzene
 Concen: 4.747 ug/L
 RT: 15.57 min Scan# 2293
 Delta R.T. -0.00 min
 Lab File: VW003765.D
 Acq: 07 Jul 2018 13:46

Instrument :
 MSVOA_W
 ClientSampleId :
 X2D24DL

Tgt Ion:180 Resp: 30113
 Ion Ratio Lower Upper
 180 100
 182 97.8 75.8 113.6
 145 32.6 25.3 37.9



Abundance Ion 180.00 (179.70 to 180.70): V
 Ion 182.00 (181.70 to 182.70): V
 Ion 145.00 (144.70 to 145.70): V

