


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW070918\
 Data File : VW003792.D
 Acq On : 09 Jul 2018 22:29
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
 Title : SW846 8260
 Last Update : Sat Jul 07 05:07:25 2018

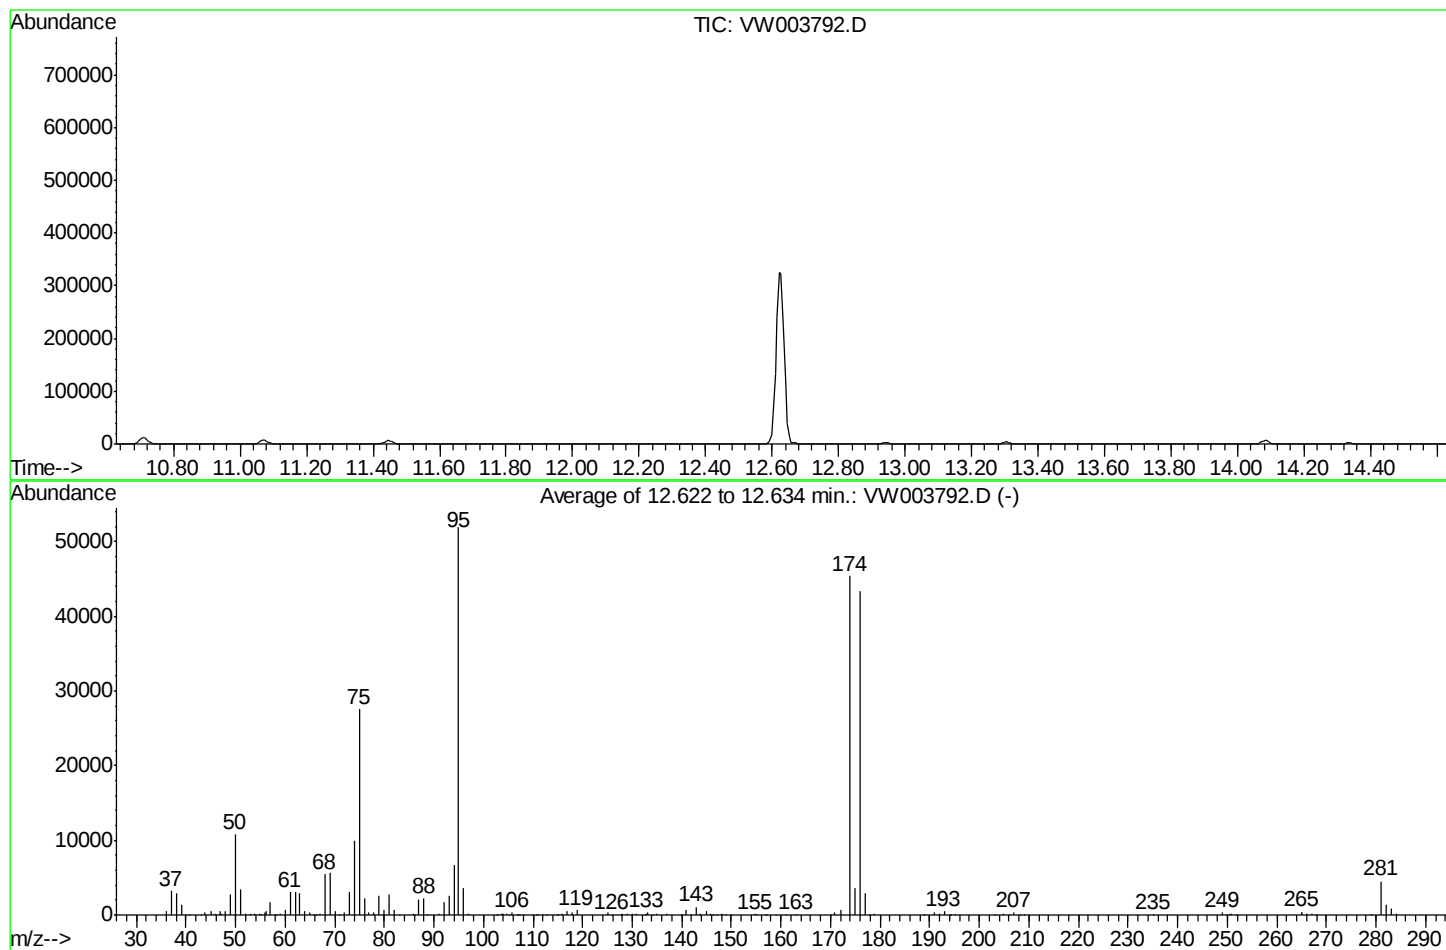

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	10723	PASS
75	95	30	60	53.1	27573	PASS
95	95	100	100	100.0	51925	PASS
96	95	5	9	6.9	3596	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.4	45381	PASS
175	174	5	9	7.9	3604	PASS
176	174	95	101	95.6	43368	PASS
177	176	5	9	6.6	2851	PASS