


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071018\  
Data File : VW003817.D  
Acq On : 10 Jul 2018 10:35  
Operator : SY/AP  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W070718S.M  
Title : SW846 8260  
Last Update : Sat Jul 07 05:07:25 2018

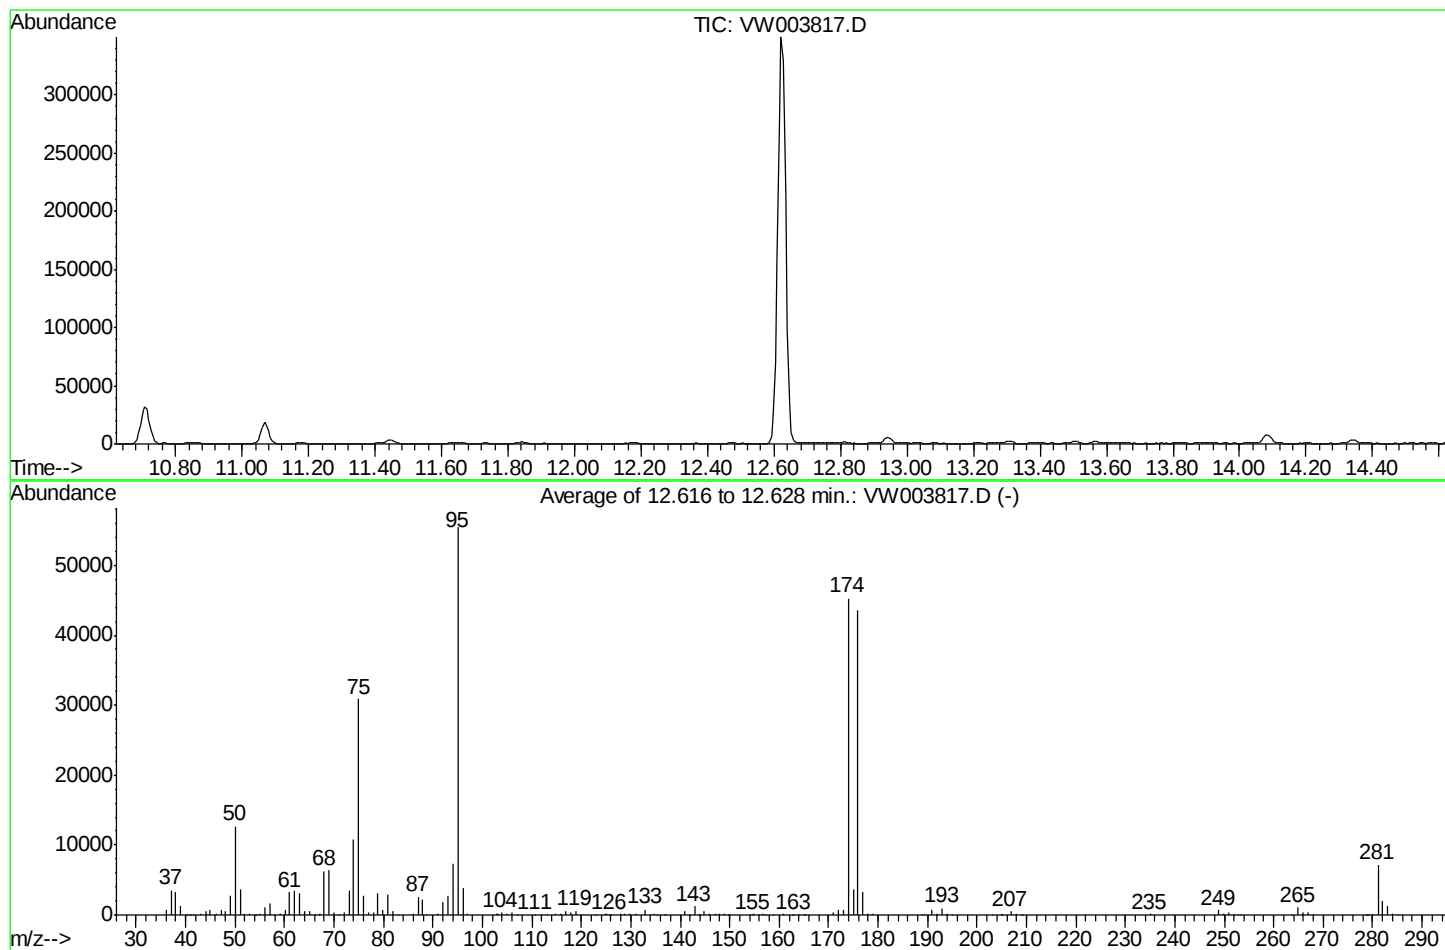

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.9      | 12677   | PASS             |
| 75          | 95           | 30           | 60           | 55.7      | 30866   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 55440   | PASS             |
| 96          | 95           | 5            | 9            | 6.9       | 3805    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.7       | 757     | PASS             |
| 174         | 95           | 50           | 100          | 81.7      | 45277   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 3617    | PASS             |
| 176         | 174          | 95           | 101          | 96.3      | 43624   | PASS             |
| 177         | 176          | 5            | 9            | 7.4       | 3243    | PASS             |