


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW071018\
Data File : VW003842.D
Acq On : 10 Jul 2018 23:27
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W070718S.M
Title : SW846 8260
Last Update : Sat Jul 07 05:07:25 2018

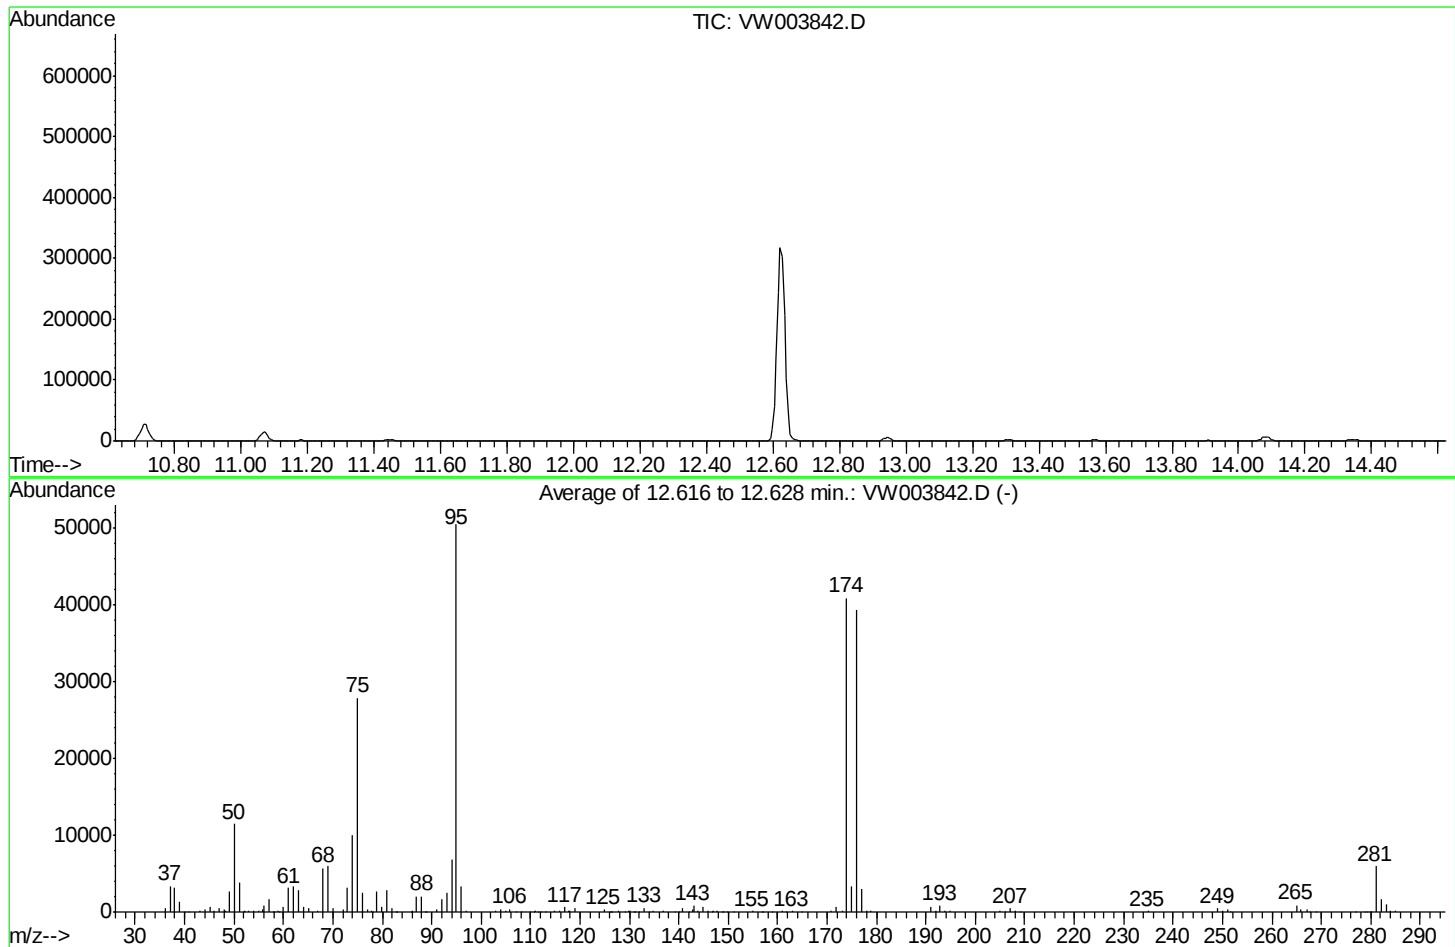

AutoFind: Scans 1809, 1810, 1811; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	11461	PASS
75	95	30	60	55.2	27818	PASS
95	95	100	100	100.0	50392	PASS
96	95	5	9	6.8	3409	PASS
173	174	0.00	2	0.6	252	PASS
174	95	50	100	81.0	40810	PASS
175	174	5	9	8.2	3365	PASS
176	174	95	101	96.4	39346	PASS
177	176	5	9	7.4	2928	PASS